




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM051322\
 Data File : BM035038.D
 Acq On : 13 May 2022 21:28
 Operator : CG/JU
 Sample : N2603-13
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW494

Manual IntegrationsAPPROVED

Quant Time: May 13 23:13:14 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM051222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu May 12 18:15:39 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/16/2022
 Supervised By :Yogesh Patel 05/17/2022

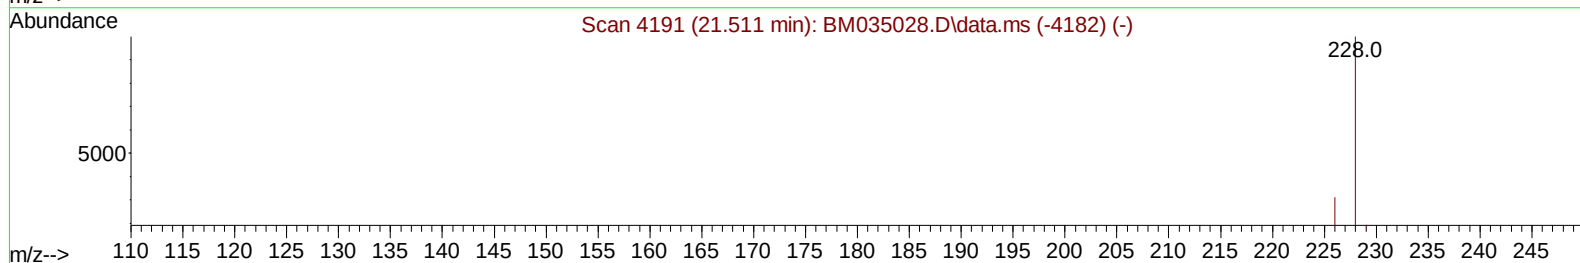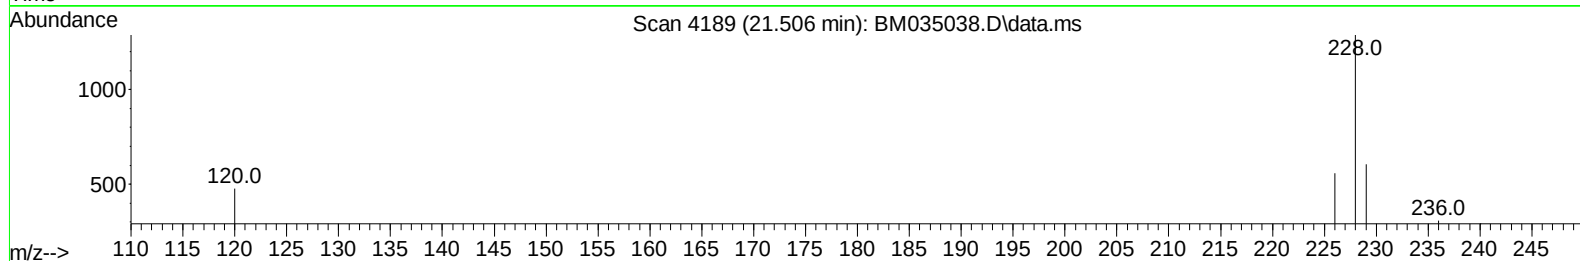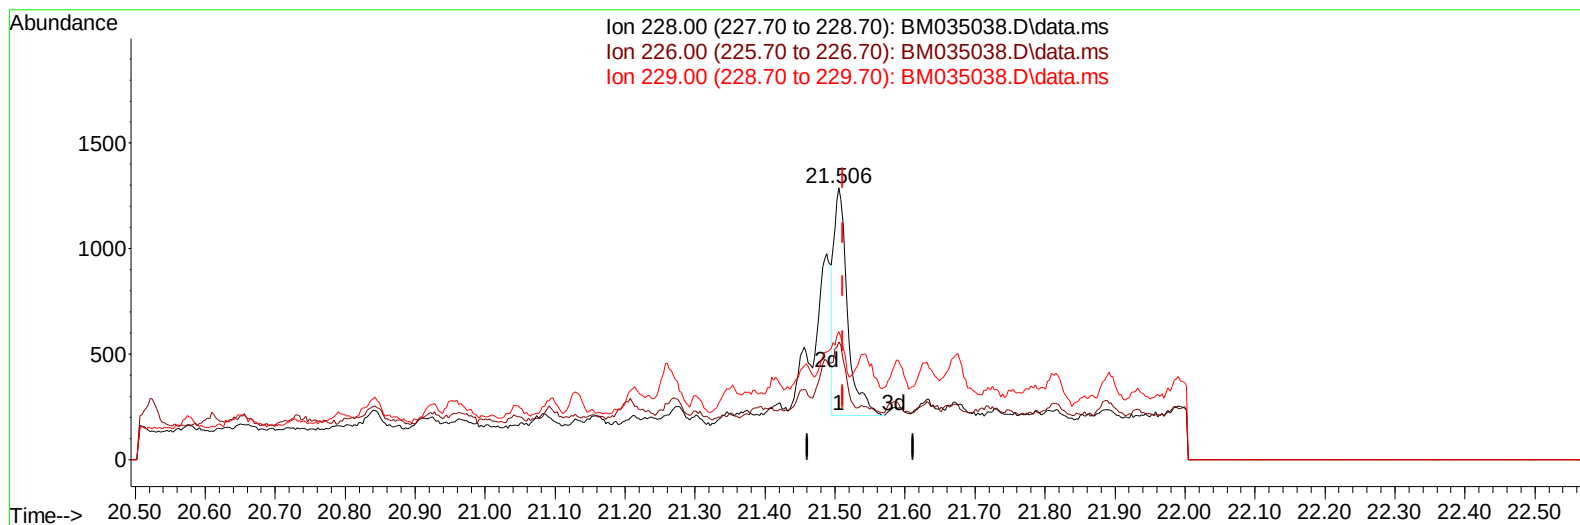

TIC: BM035038.D\data.ms

(22) Chrysene

21.506min (-0.006) 0.02 ng/u1

response 1499

Ion	Exp%	Act%
228.00	100.00	100.00
226.00	32.30	43.25#
229.00	20.90	46.97#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM051322\
 Data File : BM035038.D
 Acq On : 13 May 2022 21:28
 Operator : CG/JU
 Sample : N2603-13
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW494

Manual IntegrationsAPPROVED

Quant Time: May 13 23:13:14 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM051222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu May 12 18:15:39 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/16/2022
 Supervised By :Yogesh Patel 05/17/2022

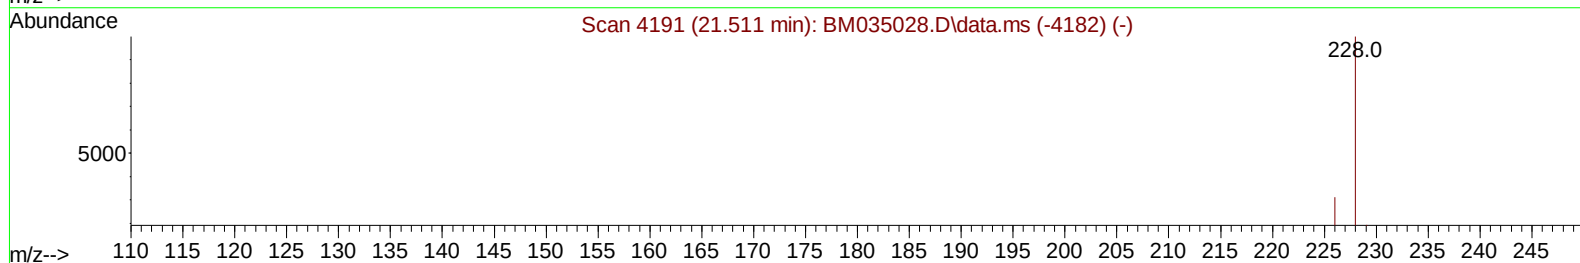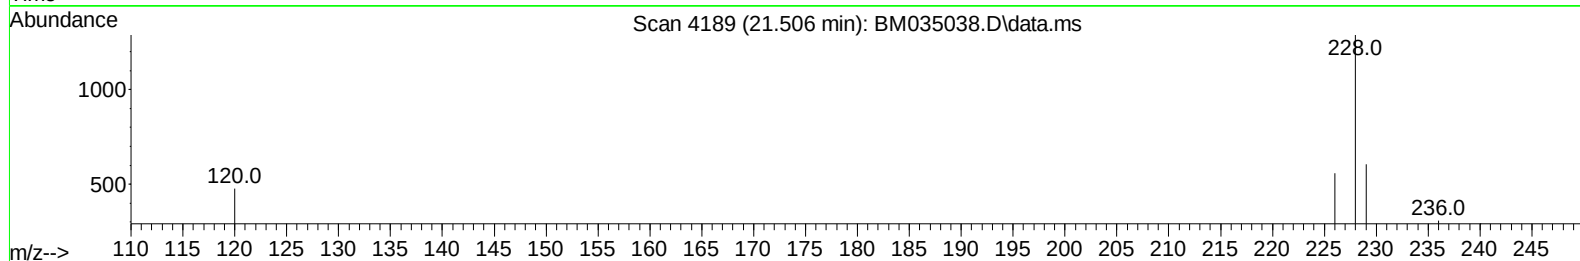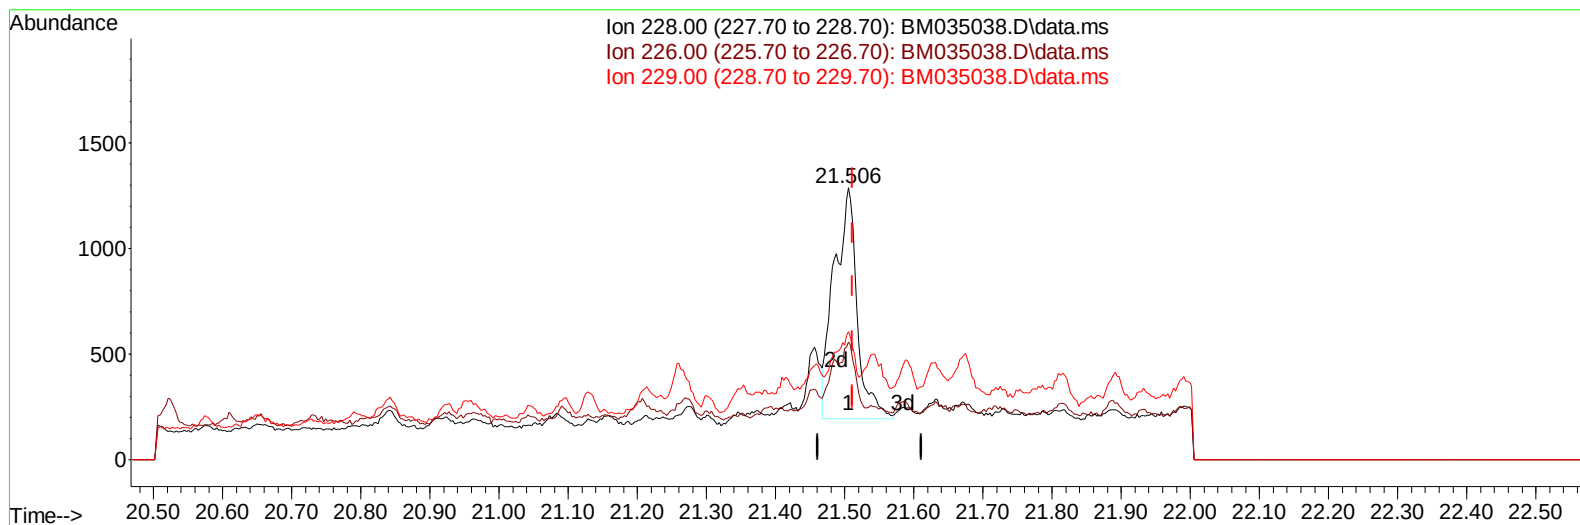

TIC: BM035038.D\data.ms

(22) Chrysene

21.506min (-0.006) 0.03 ng/ul m

response 2524

Ion	Exp%	Act%
228.00	100.00	100.00
226.00	32.30	43.25#
229.00	20.90	46.97#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM051322\
 Data File : BM035038.D
 Acq On : 13 May 2022 21:28
 Operator : CG/JU
 Sample : N2603-13
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW494

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/16/2022
 Supervised By :Yogesh Patel 05/17/2022

Quant Time: May 13 23:13:14 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM051222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu May 12 18:15:39 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.917	152	4593	0.400	ng/ul	0.00
4) Naphthalene-d8	10.715	136	14850	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.552	164	9988	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.292	188	21531	0.400	ng/ul	0.00
17) Chrysene-d12	21.471	240	16244	0.400	ng/ul	# 0.00
23) Perylene-d12	23.856	264	15850	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.356	96	21024	3.821	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.310	152	5988	0.253	ng/ul	0.00
18) Fluoranthene-d10	19.317	212	15363	0.276	ng/ul	0.00
Target Compounds						Qvalue
15) Phenanthrene	17.334	178	5615	0.068	ng/ul	97
19) Fluoranthene	19.350	202	2024	0.022	ng/ul#	61
22) Chrysene	21.506	228	2524m	0.032	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM051322\
Data File : BM035038.D
Acq On : 13 May 2022 21:28
Operator : CG/JU
Sample : N2603-13
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW494

Manual IntegrationsAPPROVED

Quant Time: May 13 23:13:14 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM051222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 12 18:15:39 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/16/2022
Supervised By :Yogesh Patel 05/17/2022

