




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM051322\
 Data File : BM035070.D
 Acq On : 14 May 2022 17:53
 Operator : CG/JU
 Sample : N2632-15
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4B7

Manual IntegrationsAPPROVED

Quant Time: May 15 01:31:44 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM051222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu May 12 18:15:39 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/16/2022
 Supervised By :Yogesh Patel 05/17/2022

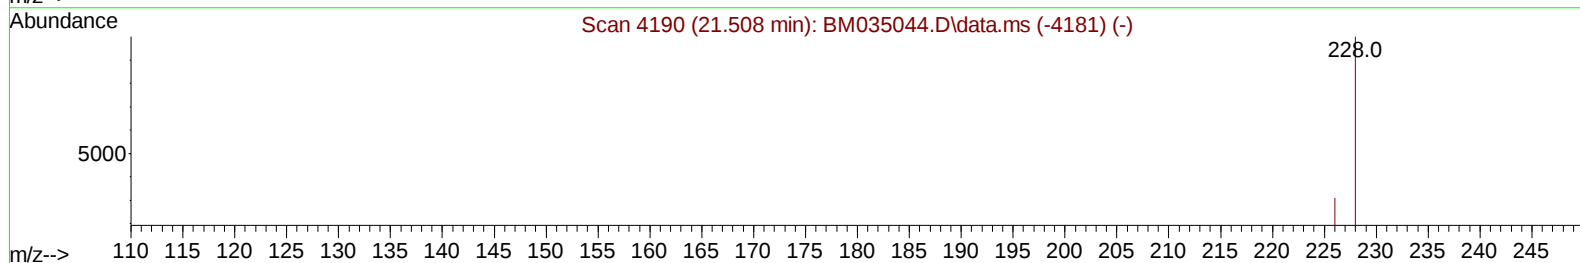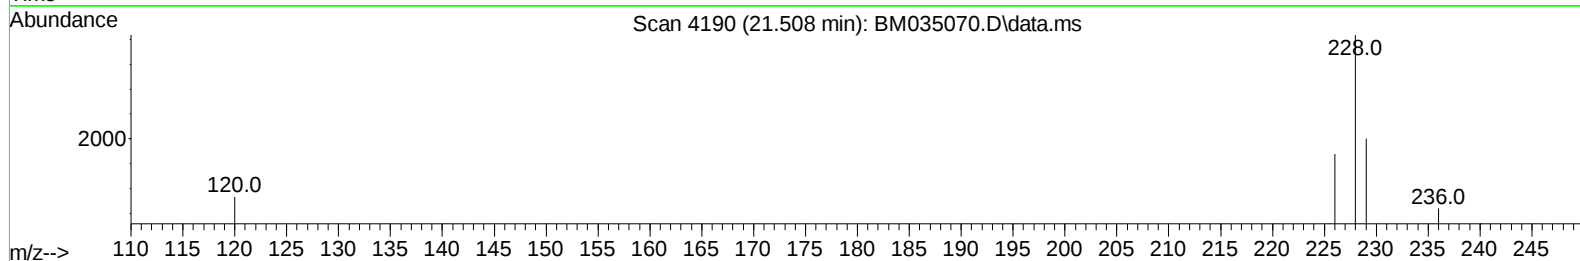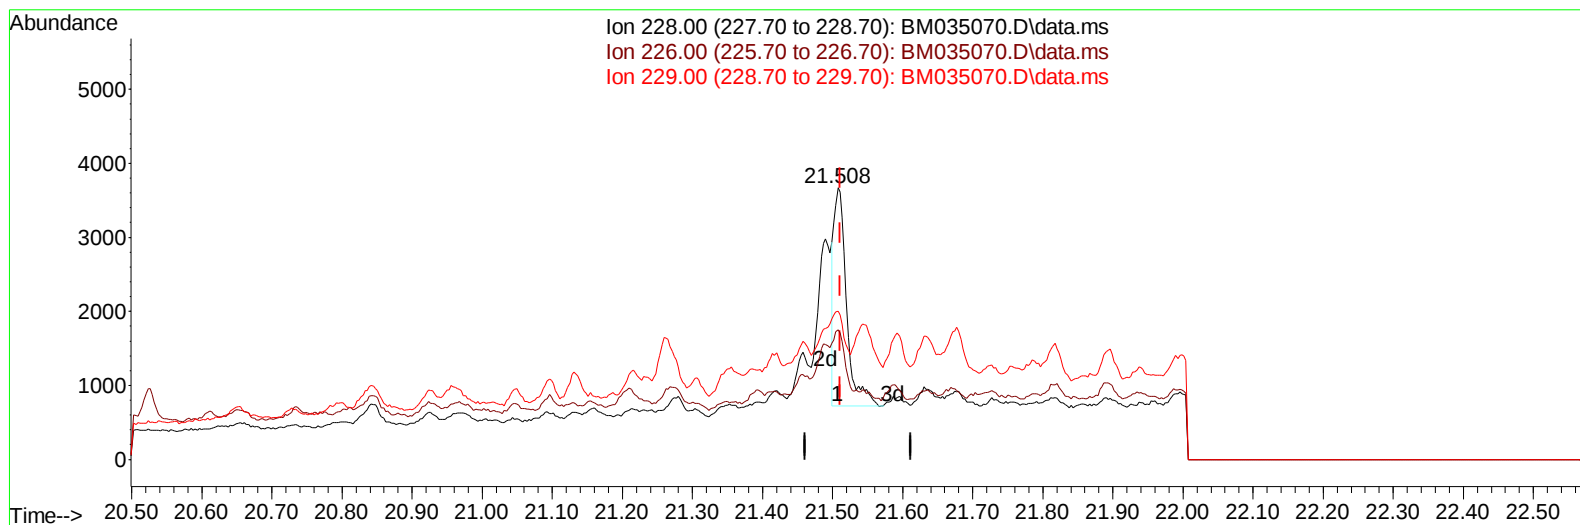

TIC: BM035070.D\data.ms

(22) Chrysene

21.508min (-0.004) 0.04 ng/u1

response 3729

Ion	Exp%	Act%
228.00	100.00	100.00
226.00	32.30	47.79#
229.00	20.90	54.61#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM051322\
 Data File : BM035070.D
 Acq On : 14 May 2022 17:53
 Operator : CG/JU
 Sample : N2632-15
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4B7

Manual IntegrationsAPPROVED

Quant Time: May 15 01:31:44 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM051222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu May 12 18:15:39 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/16/2022
 Supervised By :Yogesh Patel 05/17/2022

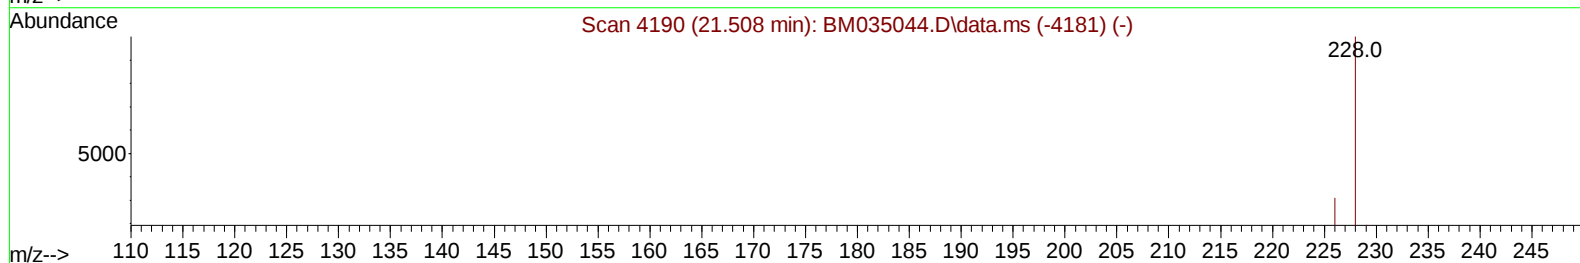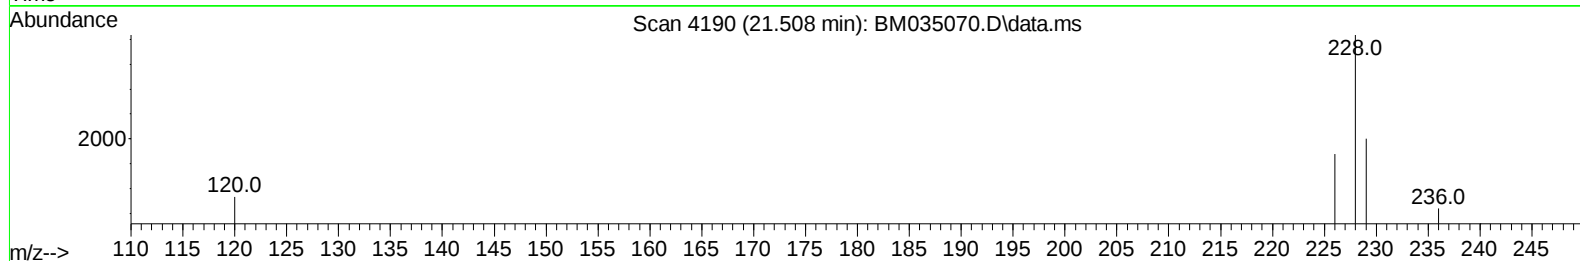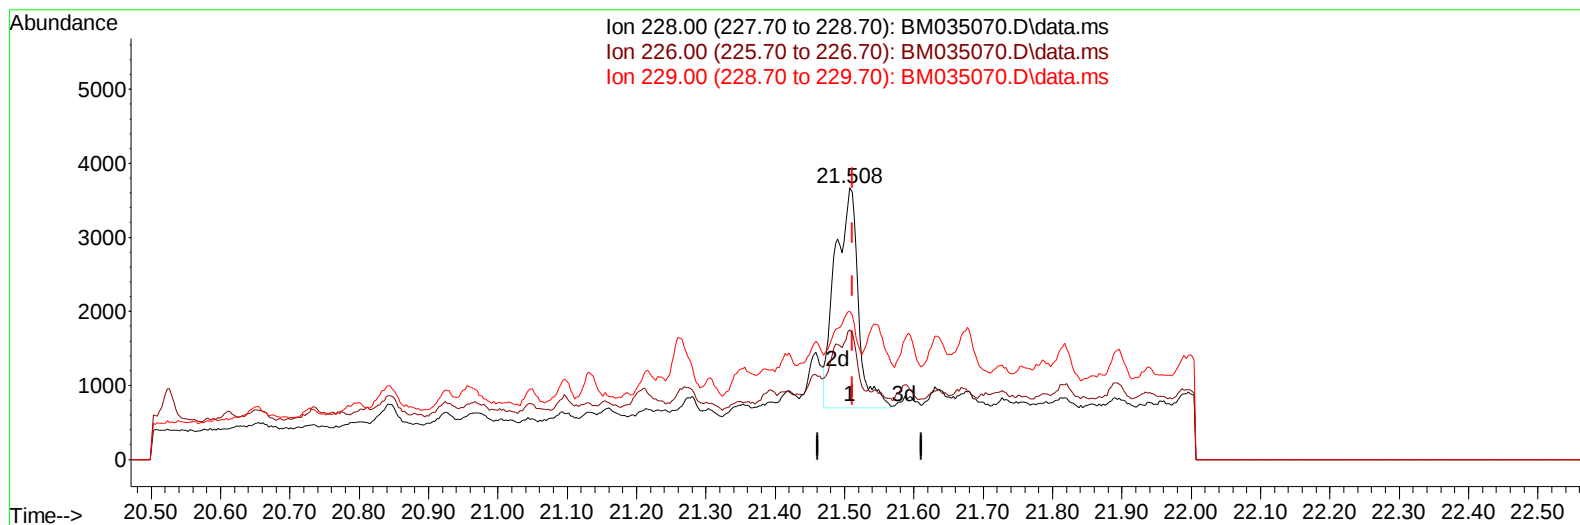

TIC: BM035070.D\data.ms

(22) Chrysene

21.508min (-0.004) 0.07 ng/ul m

response 6914

Ion	Exp%	Act%
228.00	100.00	100.00
226.00	32.30	47.79#
229.00	20.90	54.61#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM051322\
 Data File : BM035070.D
 Acq On : 14 May 2022 17:53
 Operator : CG/JU
 Sample : N2632-15
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4B7

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/16/2022
 Supervised By :Yogesh Patel 05/17/2022

Quant Time: May 15 01:31:44 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM051222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu May 12 18:15:39 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.917	152		5064	0.400	ng/ul	0.00
4) Naphthalene-d8	10.715	136		15793	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.553	164		10762	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.293	188		23758	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.473	240		19360	0.400	ng/ul	# 0.00
23) Perylene-d12	23.861	264		17312	0.400	ng/ul	# 0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.356	96		18905	3.116	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.305	152		5998	0.238	ng/ul	0.00
18) Fluoranthene-d10	19.323	212		18298	0.276	ng/ul	0.00
Target Compounds							Qvalue
7) 2-Methylnaphthalene	12.382	142		1585	0.046	ng/ul	89
8) 1-Methylnaphthalene	12.602	142		1393	0.044	ng/ul	87
15) Phenanthrene	17.335	178		9440	0.104	ng/ul	96
20) Pyrene	19.713	202		4845	0.044	ng/ul#	73
22) Chrysene	21.508	228		6914m	0.074	ng/ul	
24) Benzo(b)fluoranthene	23.136	252		2109	0.023	ng/ul#	1
29) Benzo(g,h,i)perylene	27.087	276		3562	0.051	ng/ul#	54

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM051322\
Data File : BM035070.D
Acq On : 14 May 2022 17:53
Operator : CG/JU
Sample : N2632-15
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4B7

Manual IntegrationsAPPROVED

Quant Time: May 15 01:31:44 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM051222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 12 18:15:39 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/16/2022
Supervised By :Yogesh Patel 05/17/2022

