

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM051322\
 Data File : BM035036.D
 Acq On : 13 May 2022 20:16
 Operator : CG/JU
 Sample : N2603-02
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW483

Quant Time: May 13 23:13:00 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM051222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu May 12 18:15:39 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.921	152	4200	0.400	ng/ul	0.00
4) Naphthalene-d8	10.721	136	13644	0.400	ng/ul #	0.00
9) Acenaphthene-d10	14.552	164	8907	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.292	188	18364	0.400	ng/ul	0.00
17) Chrysene-d12	21.470	240	13856	0.400	ng/ul #	0.00
23) Perylene-d12	23.856	264	14092	0.400	ng/ul #	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.356	96	25385	5.046	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.310	152	6614	0.304	ng/ul	0.00
18) Fluoranthene-d10	19.322	212	14297	0.301	ng/ul	0.00
Target Compounds						
					Qvalue	
19) Fluoranthene	19.349	202	2277	0.029	ng/ul#	65
24) Benzo(b)fluoranthene	23.133	252	1725	0.023	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM051322\
Data File : BM035036.D
Acq On : 13 May 2022 20:16
Operator : CG/JU
Sample : N2603-02
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW483

Quant Time: May 13 23:13:00 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM051222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 12 18:15:39 2022
Response via : Initial Calibration




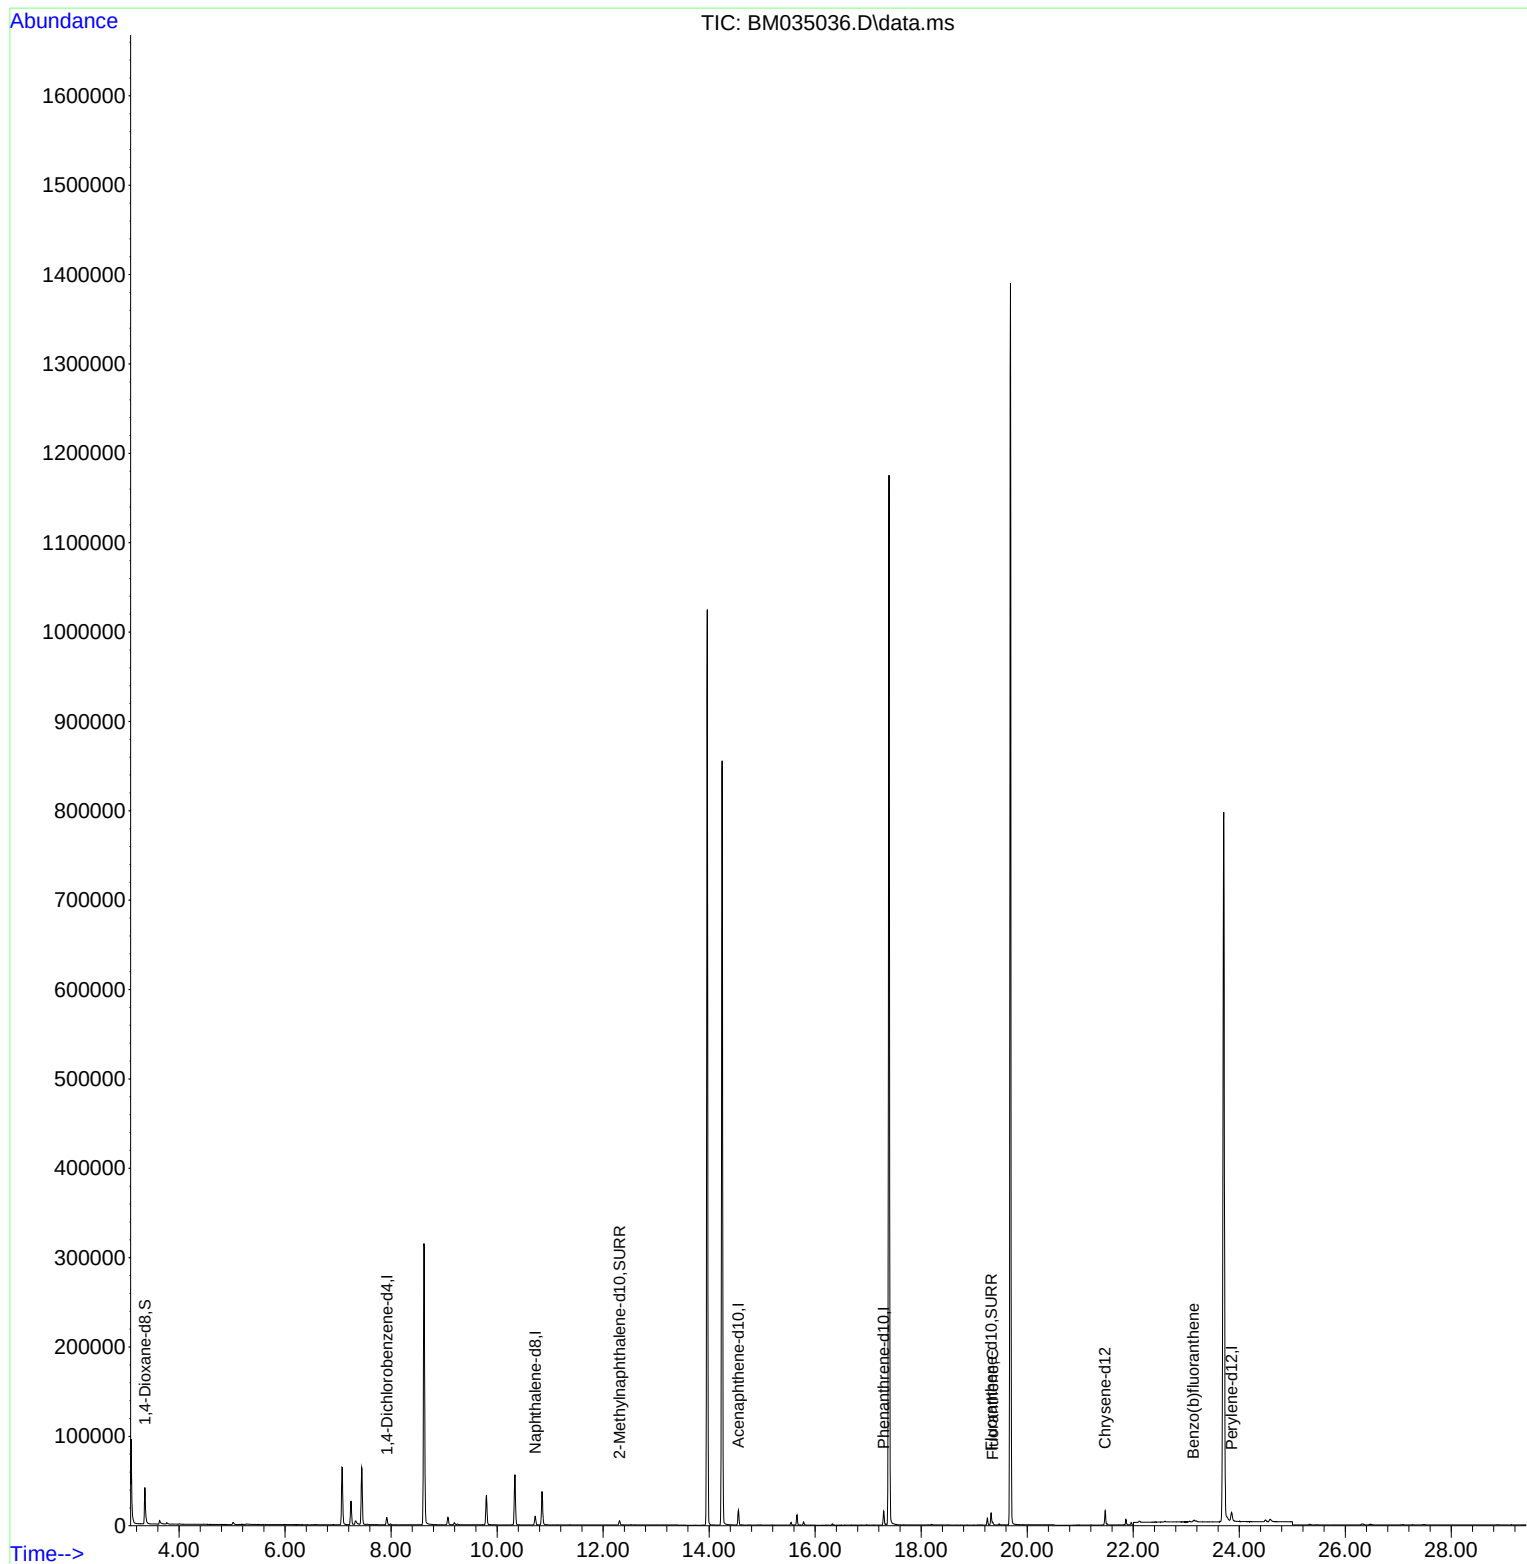


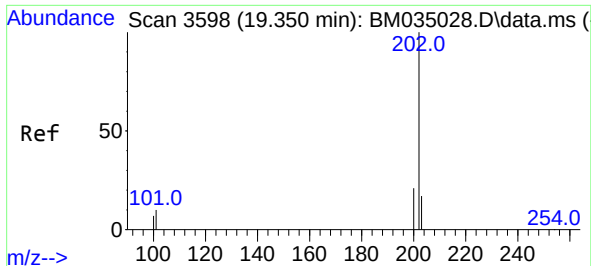

#19
Fluoranthene
Concen: 0.029 ng/u1
RT: 19.349 min Scan# 31
Delta R.T. -0.000 min
Lab File: BM035036.D
Acq: 13 May 2022 20:16

Instrument :
BNA_M
ClientSampleId :
EW483

Tgt Ion:202 Resp: 2277
Ion Ratio Lower Upper
202 100
101 26.1 9.2 13.8#
100 20.1 7.2 10.8#

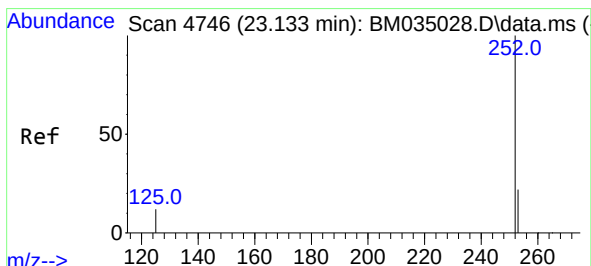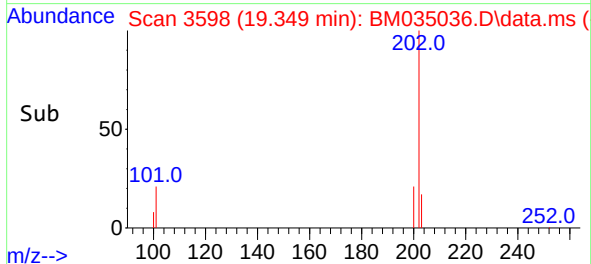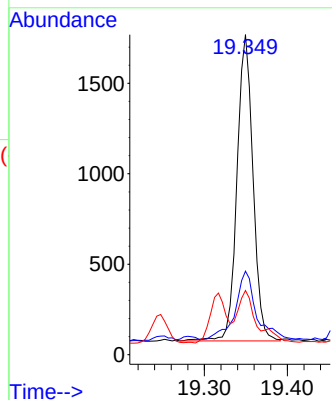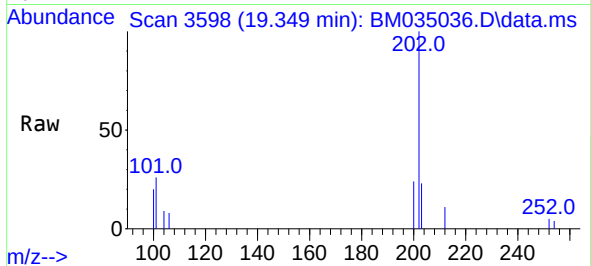

#24
Benzo(b)fluoranthene
Concen: 0.023 ng/u1
RT: 23.133 min Scan# 4746
Delta R.T. -0.000 min
Lab File: BM035036.D
Acq: 13 May 2022 20:16

Tgt Ion:252 Resp: 1725
Ion Ratio Lower Upper
252 100
253 65.1 0.0 64.2#
125 95.6 0.0 28.8#

