

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM051322\
 Data File : BM035091.D
 Acq On : 15 May 2022 07:10
 Operator : CG/JU
 Sample : N2632-07
 Misc :
 ALS Vial : 67 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4A8

Quant Time: May 16 00:56:17 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM051222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu May 12 18:15:39 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.917	152	4641	0.400	ng/ul	0.00
4) Naphthalene-d8	10.715	136	14518	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.548	164	10160	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.293	188	21788	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.473	240	16449	0.400	ng/ul	0.00
23) Perylene-d12	23.858	264	14058	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.356	96	27951	5.028	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.305	152	7374	0.318	ng/ul	0.00
18) Fluoranthene-d10	19.318	212	17186	0.305	ng/ul	0.00
Target Compounds						
					Qvalue	
15) Phenanthrene	17.331	178	1924	0.023	ng/ul#	89
22) Chrysene	21.508	228	2879	0.036	ng/ul#	81


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM051322\
Data File : BM035091.D
Acq On : 15 May 2022 07:10
Operator : CG/JU
Sample : N2632-07
Misc :
ALS Vial : 67 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4A8

Quant Time: May 16 00:56:17 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM051222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 12 18:15:39 2022
Response via : Initial Calibration




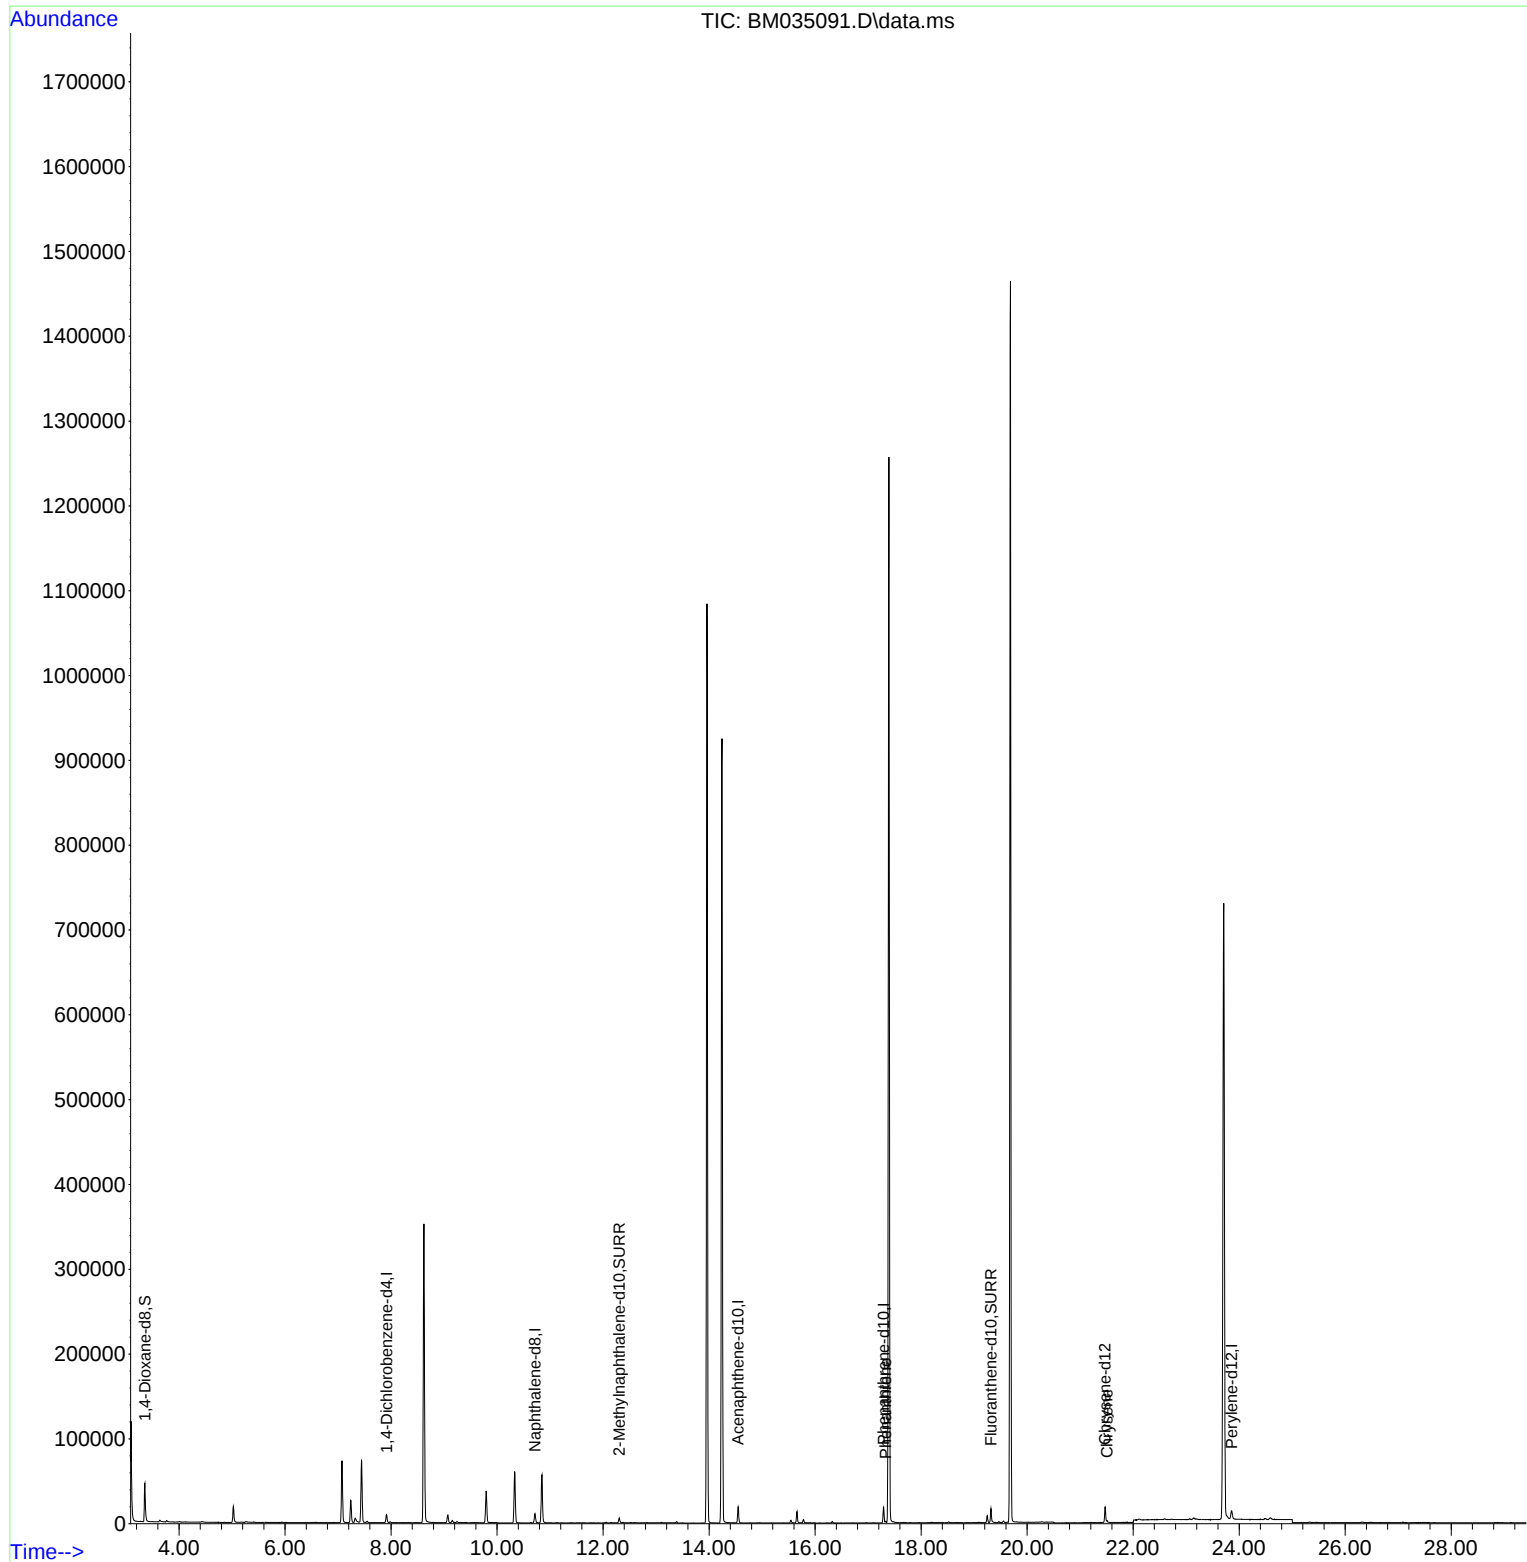


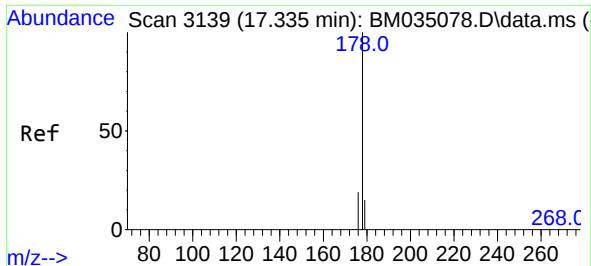

#15
Phenanthrene
Concen: 0.023 ng/u1
RT: 17.331 min Scan# 3139
Delta R.T. -0.003 min
Lab File: BM035091.D
Acq: 15 May 2022 07:10

Instrument :
BNA_M
ClientSampleId :
EW4A8

Tgt Ion:	178	Resp:	1924
Ion Ratio	Lower	Upper	
178	100		
179	26.3	15.0	22.6#
176	25.4	17.9	26.9

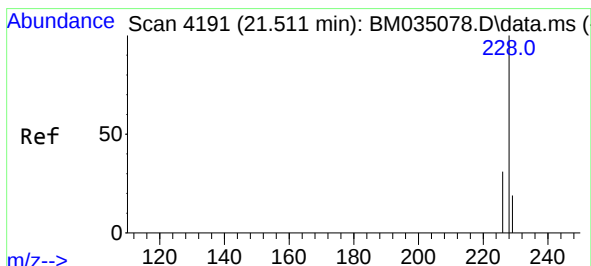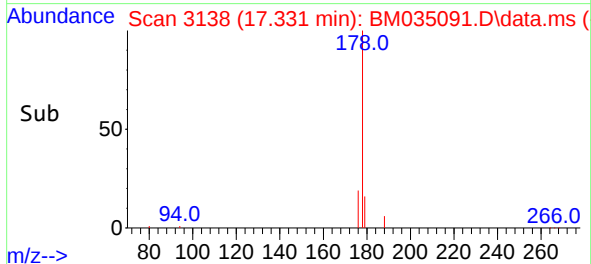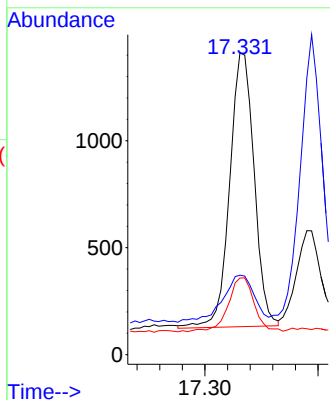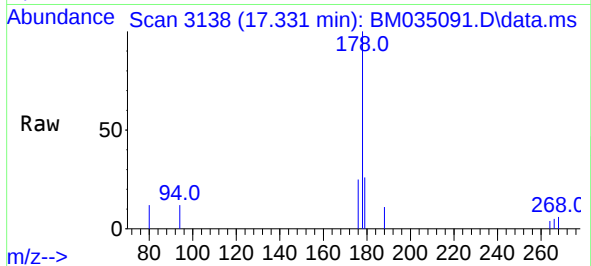

#22
Chrysene
Concen: 0.036 ng/u1
RT: 21.508 min Scan# 4190
Delta R.T. -0.004 min
Lab File: BM035091.D
Acq: 15 May 2022 07:10

Tgt Ion:	228	Resp:	2879
Ion Ratio	Lower	Upper	
228	100		
226	40.3	25.8	38.8#
229	33.3	16.7	25.1#

