
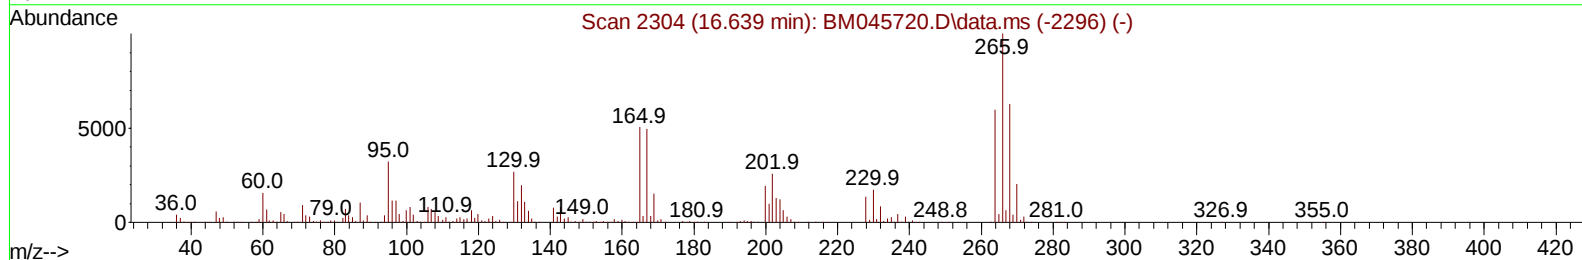
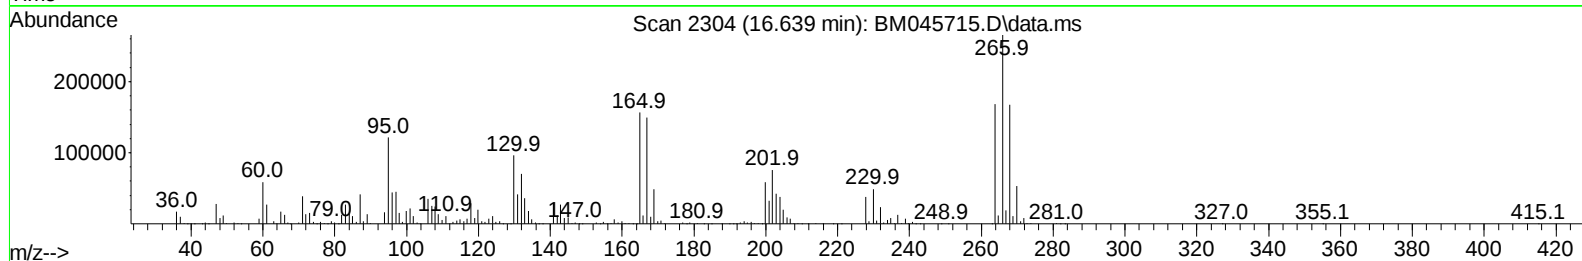


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM051324\
Data File : BM045715.D
Acq On : 13 May 2024 15:59
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 14 04:35:45 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM051324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 14 02:40:40 2024
Response via : Initial Calibration

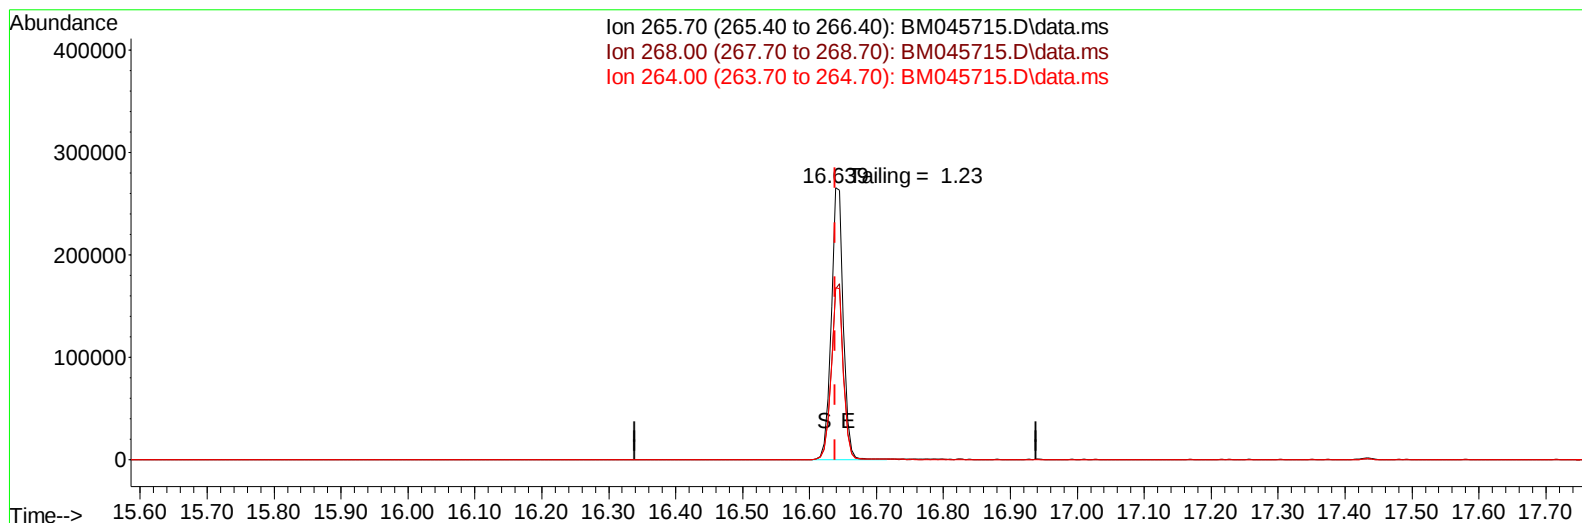

TIC: BM045715.D\data.ms

(70) Pentachlorophenol (C)




16.639min (+ 0.000) 0.00 ng

response 332683

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.90	62.96
264.00	59.70	63.27
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM051324\
Data File : BM045715.D
Acq On : 13 May 2024 15:59
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 14 04:35:45 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM051324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 14 02:40:40 2024
Response via : Initial Calibration

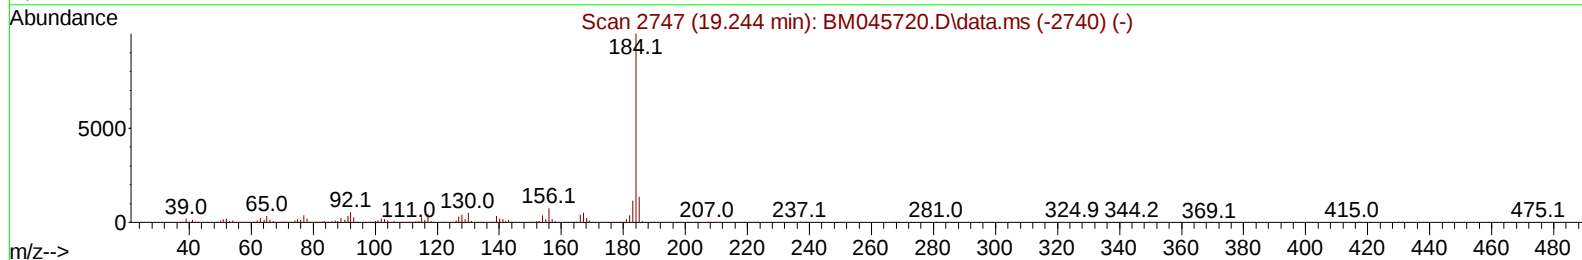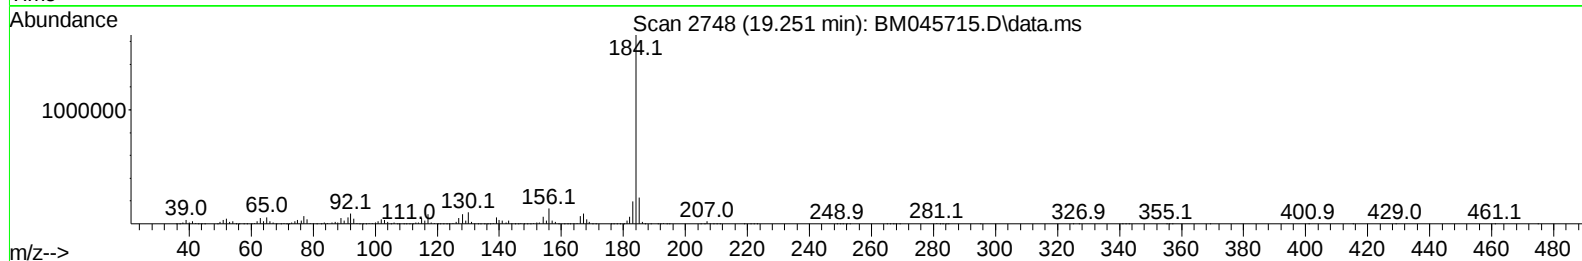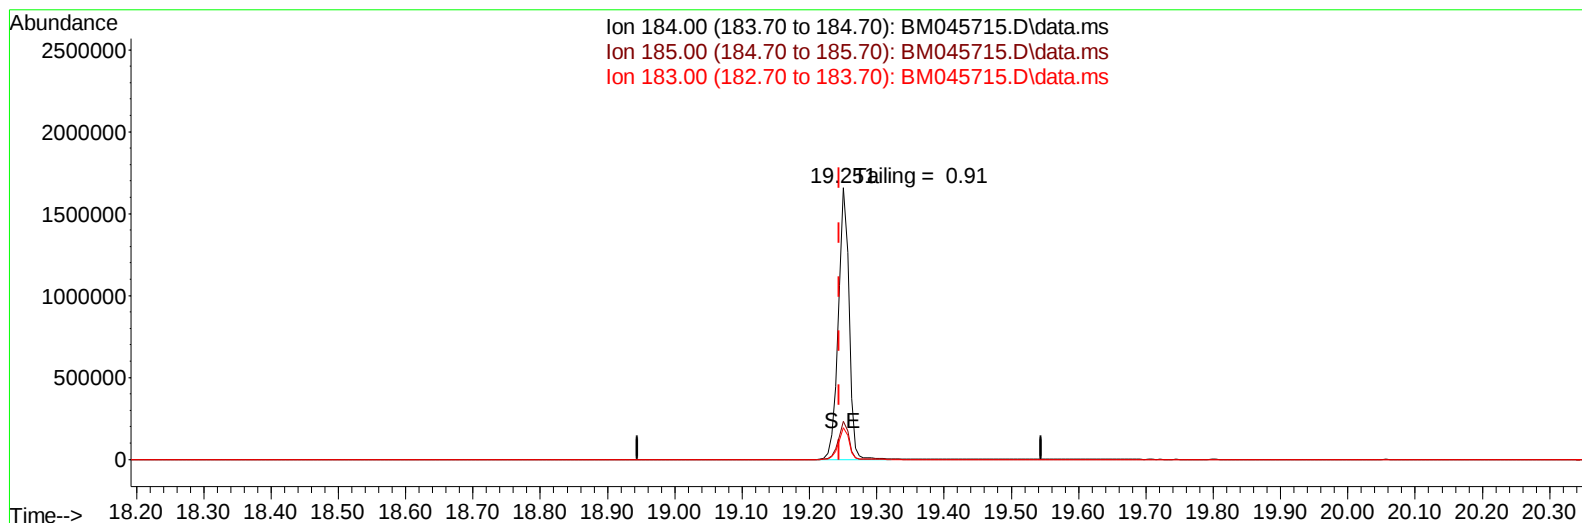

TIC: BM045715.D\data.ms

(77) Benzidine**19.251min (+ 0.006) 0.00 ng****response 1818774**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	13.98
183.00	11.60	11.74
0.00	0.00	0.00