

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM051324\
Data File : BM045725.D
Acq On : 13 May 2024 23:14
Operator : MA/JU
Sample : PB160855BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB160855BL

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM051324.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM045725.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.269	364	371	382	rBV	2066660	2881915	49.38%	11.732%
2	6.863	634	642	651	rBV	1769905	2864616	49.09%	11.662%
3	7.581	757	764	771	rBV	380863	566572	9.71%	2.307%
4	8.751	955	963	974	rVB	1105304	1877170	32.17%	7.642%
5	10.351	1228	1235	1244	rVB	400159	666447	11.42%	2.713%
6	12.839	1650	1658	1666	rVB	2497068	3547970	60.79%	14.444%
7	14.210	1885	1891	1898	rVB	513052	707260	12.12%	2.879%
8	15.710	2140	2146	2153	rBV	2534987	3153169	54.03%	12.837%
9	16.957	2352	2358	2366	rVB	596464	819327	14.04%	3.336%
10	19.598	2801	2807	2811	rVB	5225904	5835986	100.00%	23.759%
11	21.168	3069	3074	3079	rVB2	557667	741915	12.71%	3.020%
12	23.968	3544	3550	3561	rVB	384446	901356	15.44%	3.669%




Sum of corrected areas: 24563703

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM051324\
Data File : BM045725.D
Acq On : 13 May 2024 23:14
Operator : MA/JU
Sample : PB160855BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB160855BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM051324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

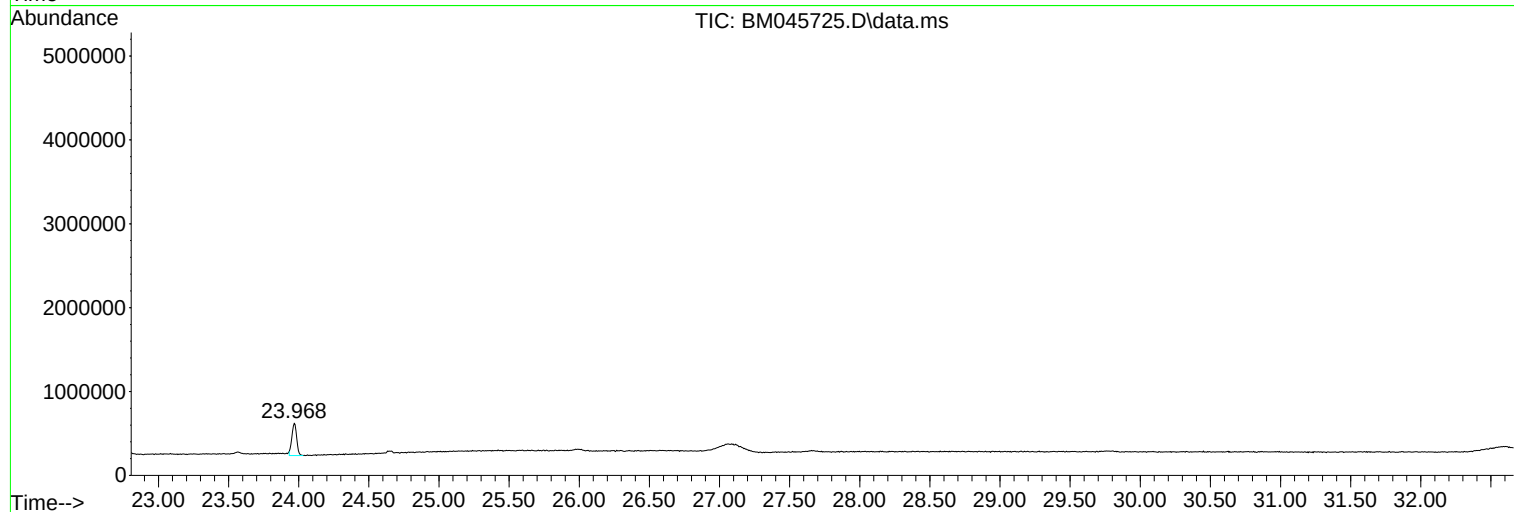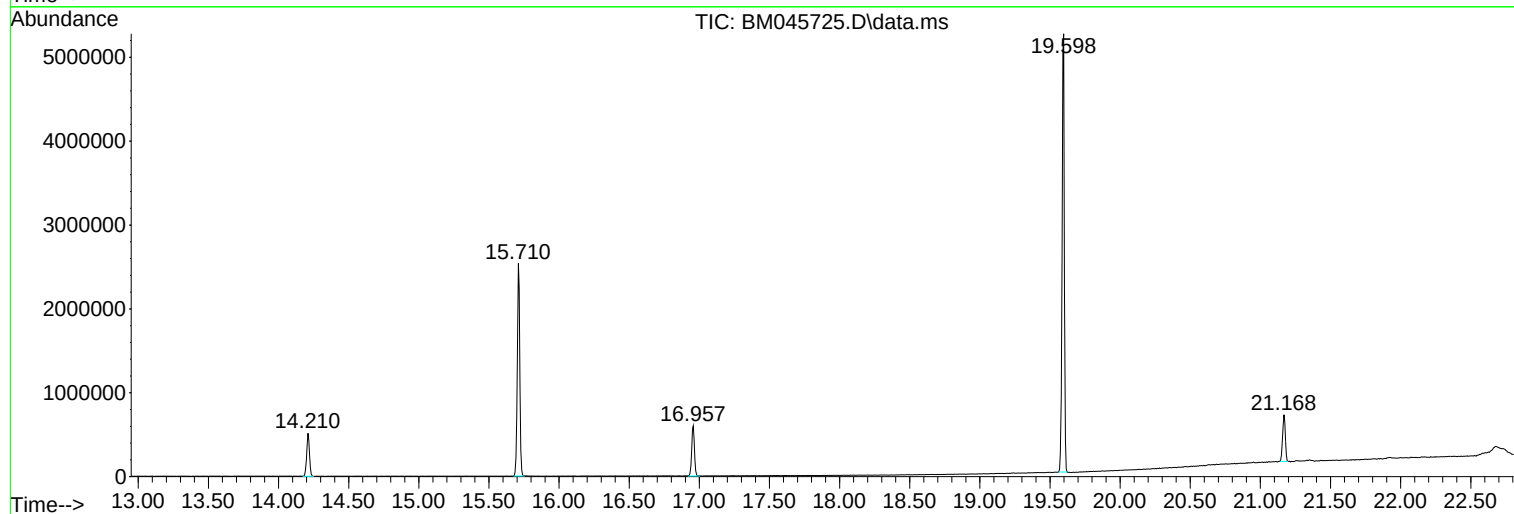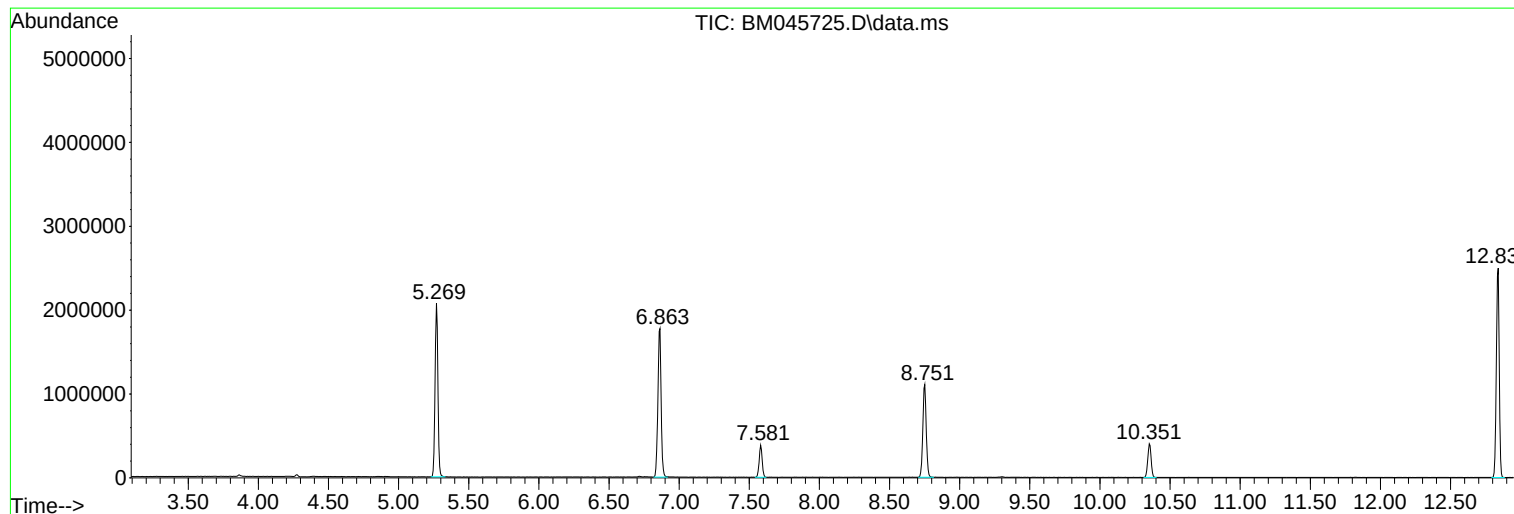

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM051324\
Data File : BM045725.D
Acq On : 13 May 2024 23:14
Operator : MA/JU
Sample : PB160855BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB160855BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM051324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM051324\
Data File : BM045725.D
Acq On : 13 May 2024 23:14
Operator : MA/JU
Sample : PB160855BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB160855BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM051324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------