


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM051324\
Data File : BM045715.D
Acq On : 13 May 2024 15:59
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM051324.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue May 14 02:40:40 2024

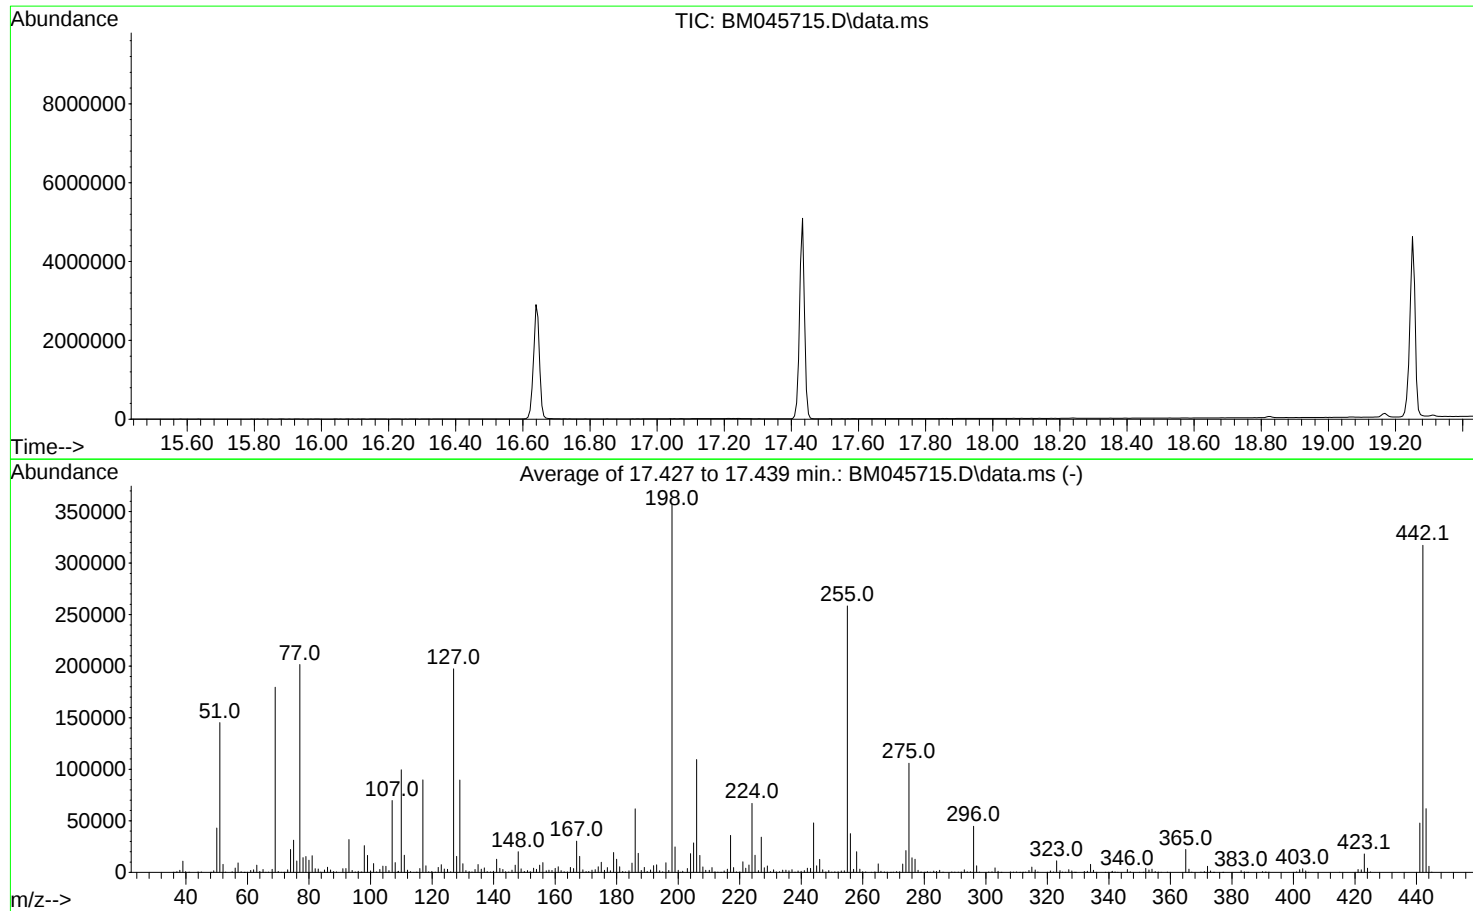




AutoFind: Scans 2438, 2439, 2440; Background Corrected with Scan 2431

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.7	145272	PASS
68	69	0.00	2	1.7	2992	PASS
69	198	0.00	100	50.3	179581	PASS
70	69	0.00	2	0.6	1013	PASS
127	198	10	80	55.3	197496	PASS
197	198	0.00	2	0.5	1927	PASS
198	198	100	100	100.0	356843	PASS
199	198	5	9	6.9	24619	PASS
275	198	10	60	29.7	105819	PASS
365	198	1	100	6.2	22261	PASS
441	198	0.01	100	13.4	47752	PASS
442	442	50	100	100.0	317248	PASS
443	442	15	24	19.5	61811	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM051324\
Data File : BM045715.D
Acq On : 13 May 2024 15:59
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: May 14 04:35:45 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM051324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 14 02:40:40 2024
Response via : Initial Calibration

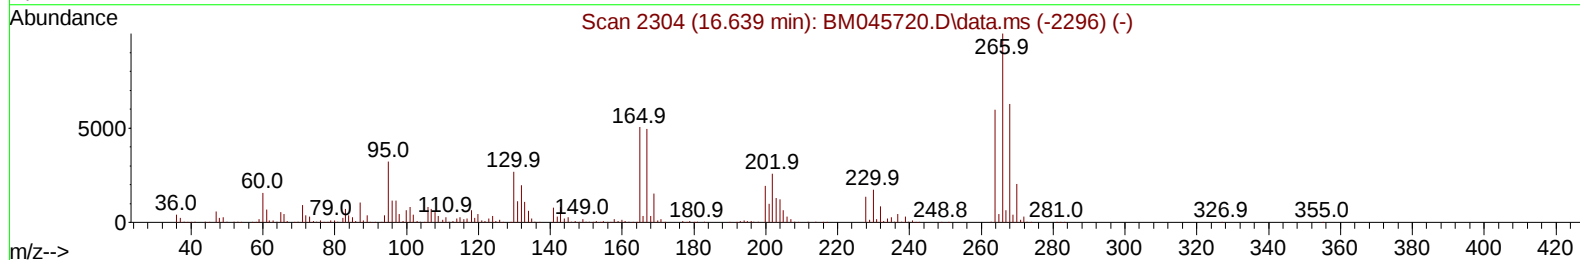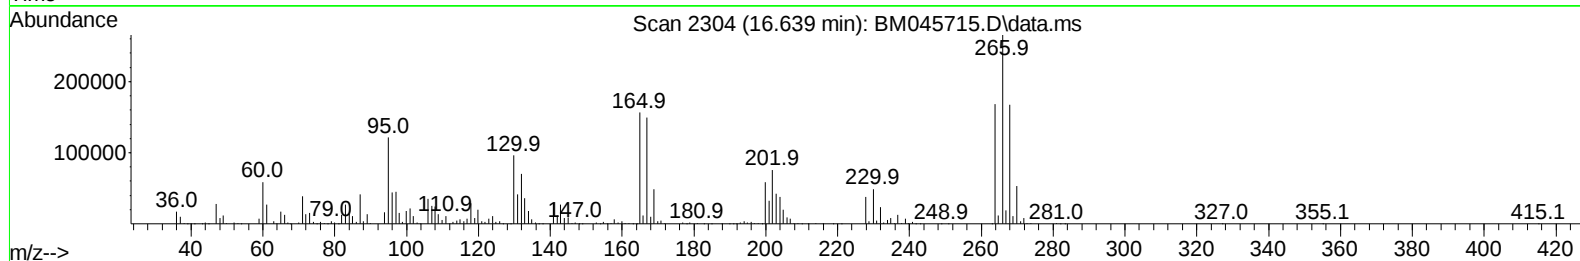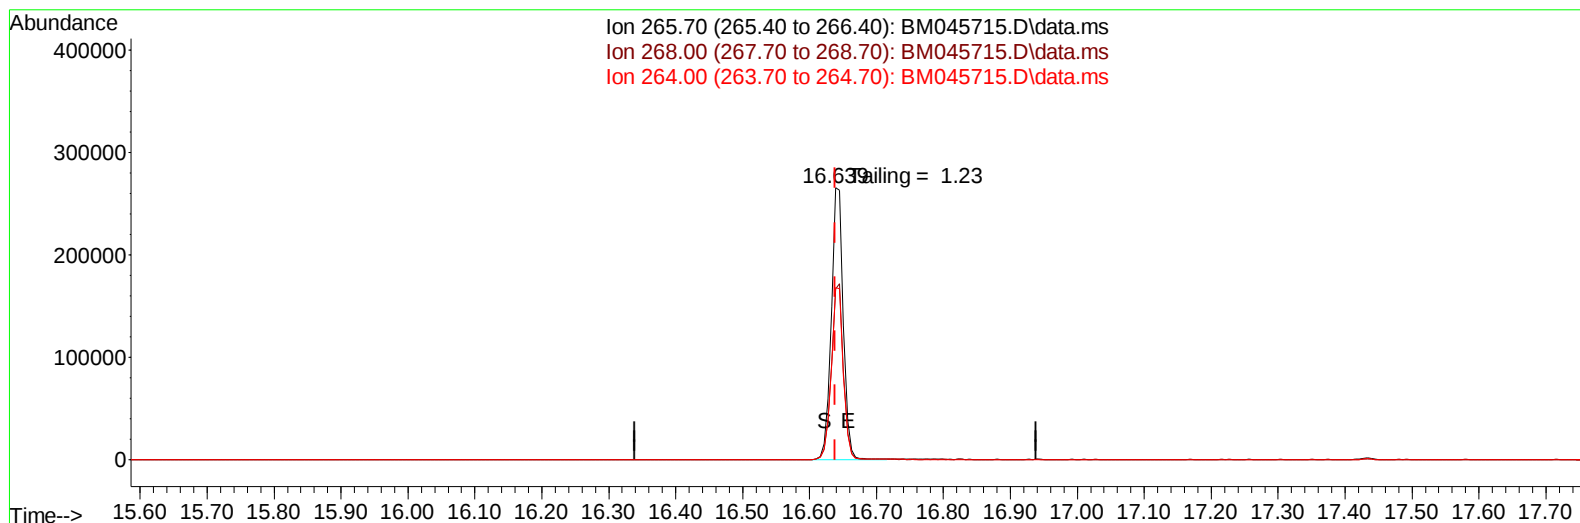

TIC: BM045715.D\data.ms

(70) Pentachlorophenol (C)

16.639min (+ 0.000) 0.00 ng




response 332683

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.90	62.96
264.00	59.70	63.27
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM051324\
Data File : BM045715.D
Acq On : 13 May 2024 15:59
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: May 14 04:35:45 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM051324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 14 02:40:40 2024
Response via : Initial Calibration

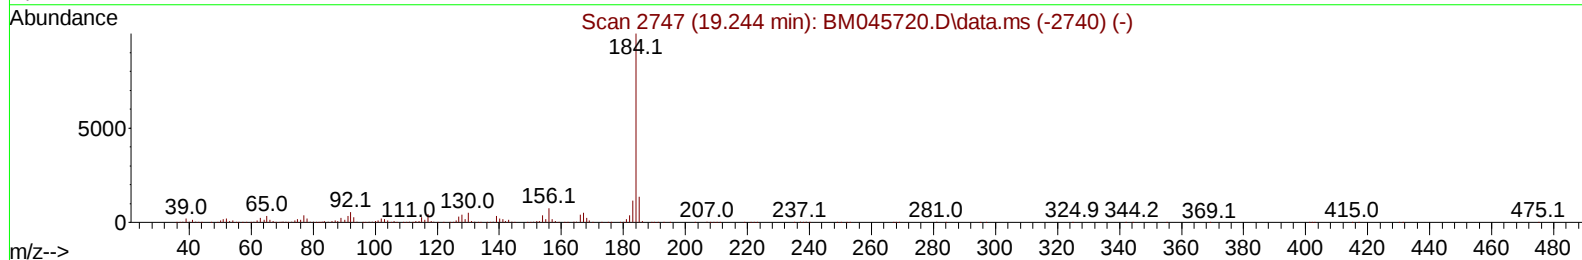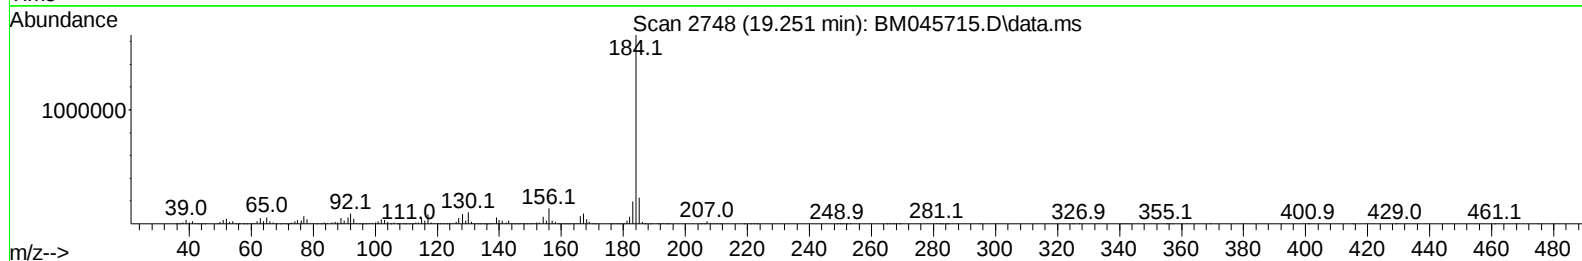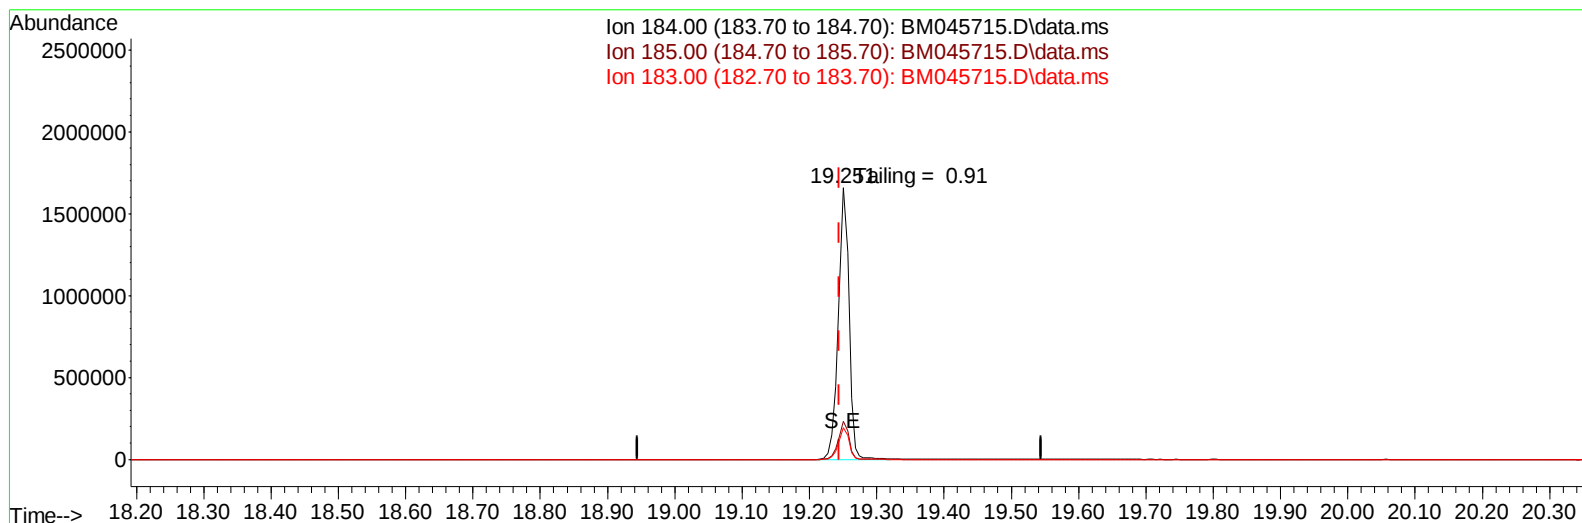

TIC: BM045715.D\data.ms

(77) Benzidine

19.251min (+ 0.006) 0.00 ng

response 1818774

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	13.98
183.00	11.60	11.74
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/13/2024	BNA_M	<u>BM045715.D</u>
Compound Name	Response	Retention Time
DDT	14442766	20.462
DDD	12495	20.074
DDE	190	19.509
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
12685	14455451	0.09

Instrument :
BNA_M
ClientSampleId :
DFTPP