


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM051421\
Data File : BM030036.D
Acq On : 15 May 2021 02:31
Operator : CG/JU
Sample : M2194-05
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YARH6

Manual Integrations
APPROVED

mohammad
5/16/2021 12:21:07 AM

Quant Time: May 15 05:11:29 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SFAM-EPA-SIM-BM051421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 14 17:21:45 2021
Response via : Initial Calibration

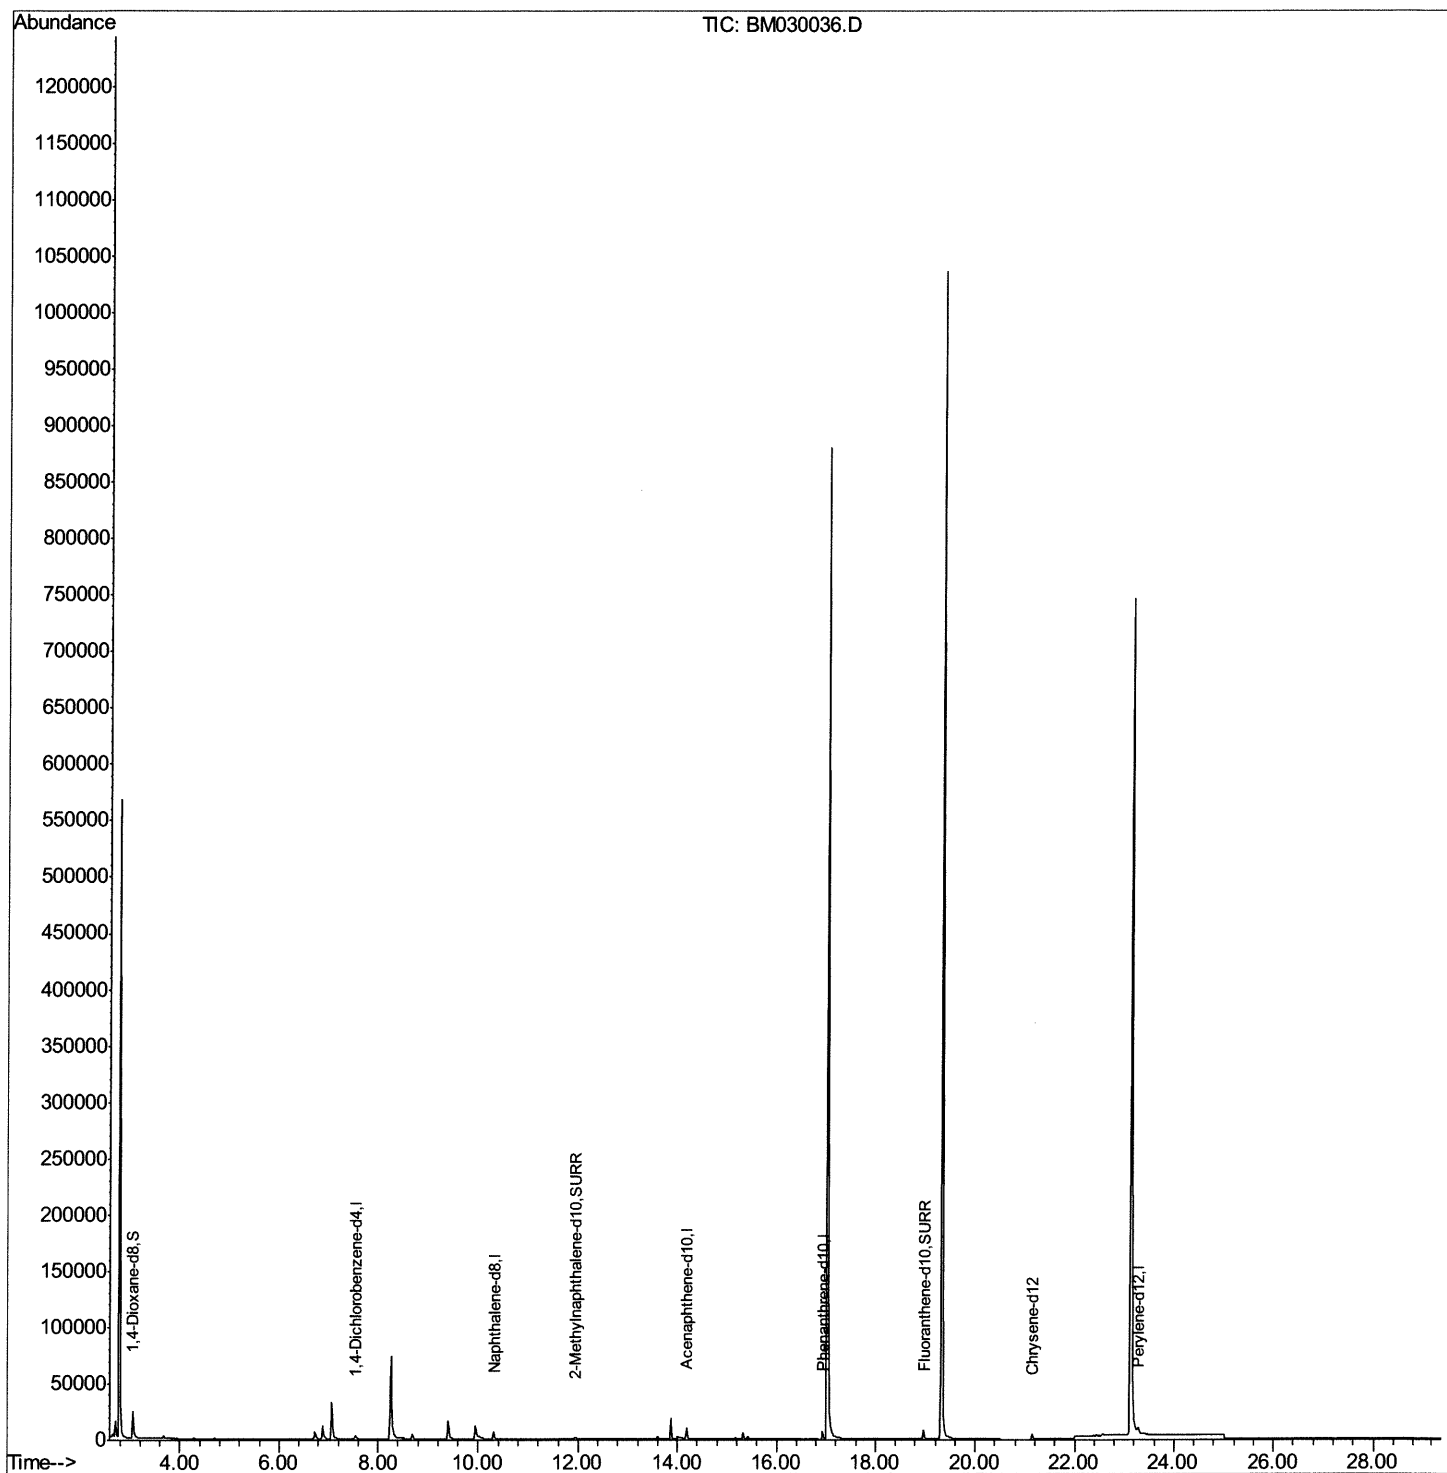

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM051421\
 Data File : BM030036.D
 Acq On : 15 May 2021 02:31
 Operator : CG/JU
 Sample : M2194-05
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
ClientSampleId :
 YARH6

Manual Integrations
APPROVED

mohammad
 5/16/2021 12:21:07 AM

Quant Time: May 15 03:08:31 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SFAM-EPA-SIM-BM051421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri May 14 17:21:45 2021
 Response via : Initial Calibration

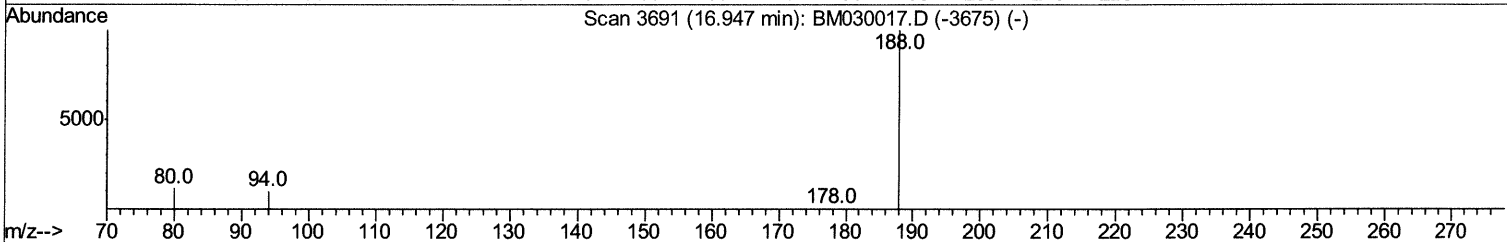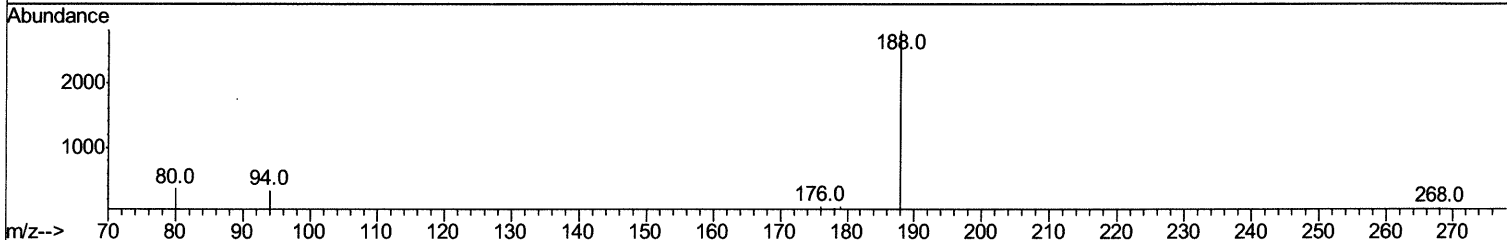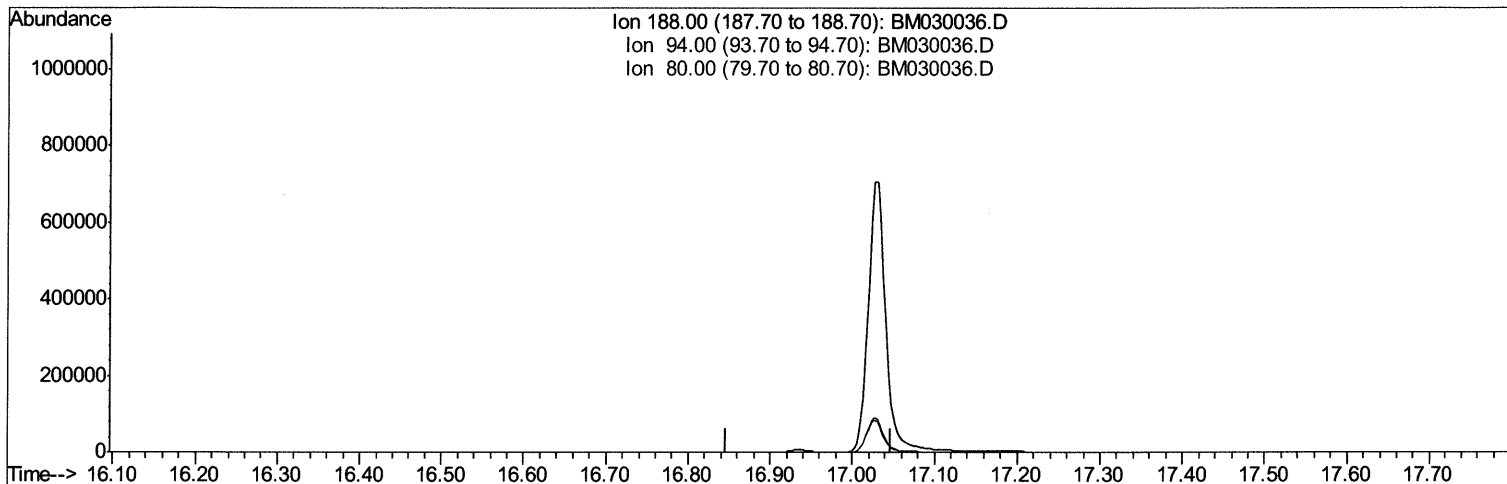

TIC: BM030036.D

(13) Phenanthrene-d10 (I)

16.947min (-16.947) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	11.10	0.00#
80.00	12.80	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM051421\
 Data File : BM030036.D
 Acq On : 15 May 2021 02:31
 Operator : CG/JU
 Sample : M2194-05
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
ClientSampleId :
 YARH6

Manual Integrations
APPROVED

mohammad
 5/16/2021 12:21:07 AM

Quant Time: May 15 03:08:31 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SFAM-EPA-SIM-BM051421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri May 14 17:21:45 2021
 Response via : Initial Calibration

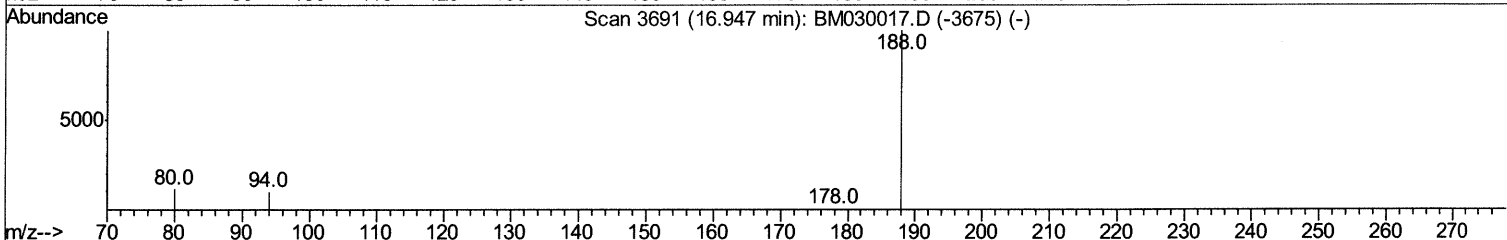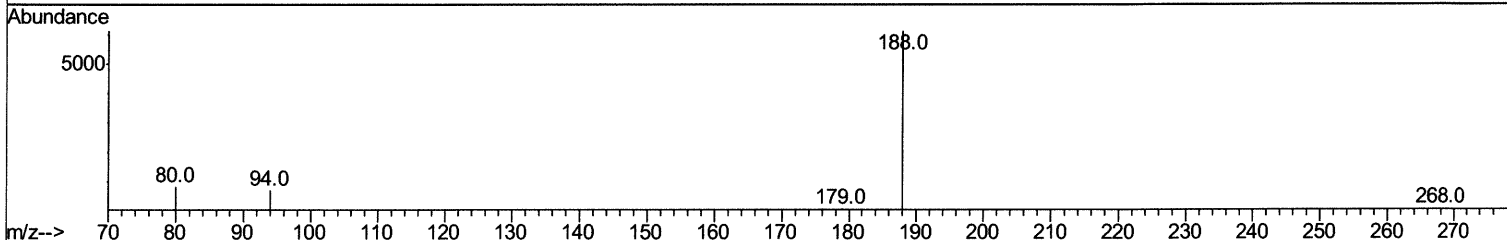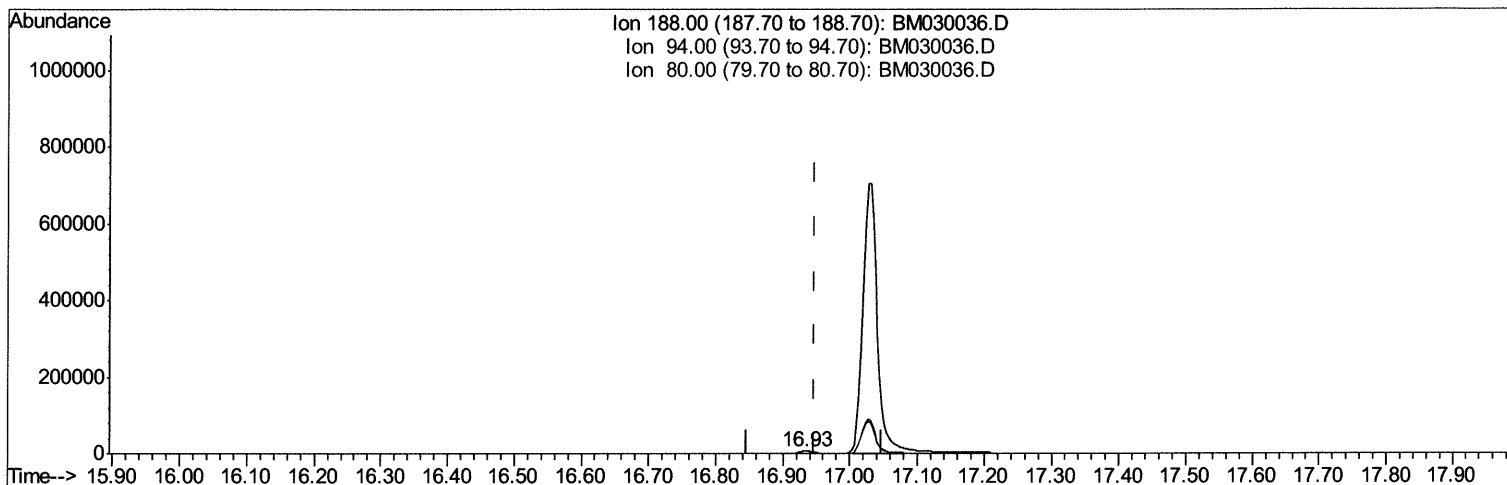

TIC: BM030036.D

(13) Phenanthrene-d10 (I)

16.933min (-0.014) 0.40ng/ul m 05/17/21 JV

response 9516

Ion	Exp%	Act%
188.00	100	100
94.00	11.10	11.40
80.00	12.80	13.50
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM051421\
Data File : BM030036.D
Acq On : 15 May 2021 02:31
Operator : CG/JU
Sample : M2194-05
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YARH6

Manual Integrations
APPROVED

mohammad
5/16/2021 12:21:07 AM

Quant Time: May 15 05:11:29 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SFAM-EPA-SIM-BM051421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 14 17:21:45 2021
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.55	152	2245	0.40	ng/ul	0.00
4) Naphthalene-d8	10.31	136	9562	0.40	ng/ul	-0.02
9) Acenaphthene-d10	14.19	164	5701	0.40	ng/ul	0.00
13) Phenanthrene-d10	16.93	188	9516m>	0.40	ng/ul>	-0.010517/213J
17) Chrysene-d12	21.15	240	6564	0.40	ng/ul	0.01
23) Perylene-d12	23.28	264	10483	0.40	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.05	96	16650	4.76	ng/ul	-0.02
6) 2-Methylnaphthalene-d10	11.94	152	4262	0.31	ng/ul	0.01
18) Fluoranthene-d10	18.97	212	10436	0.51	ng/ul	0.00

Target Compounds Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed