
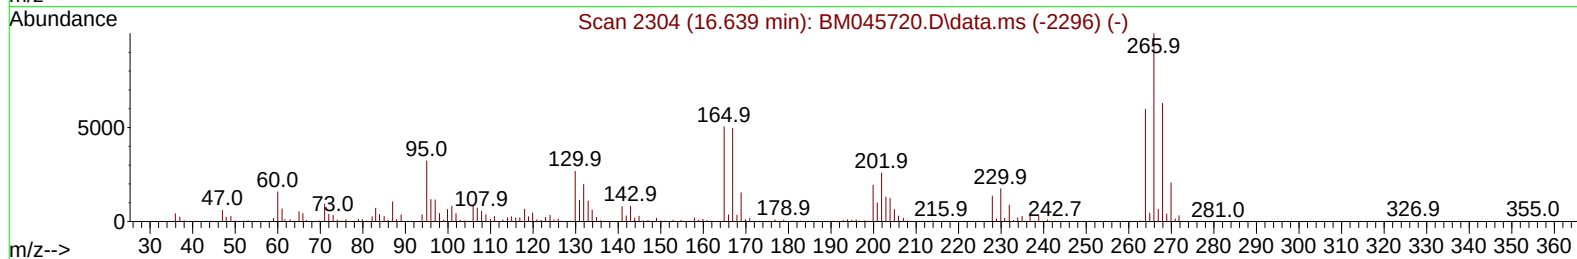
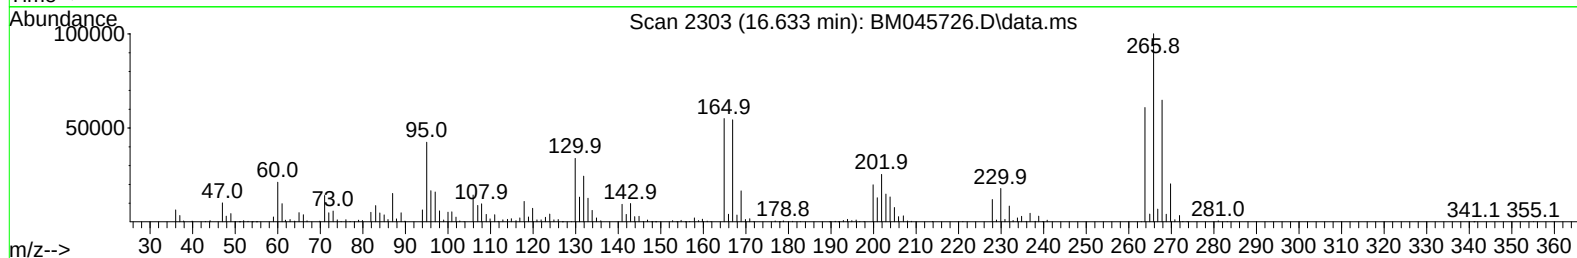


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM051424\
Data File : BM045726.D
Acq On : 14 May 2024 10:50
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 14 12:21:55 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM051424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 14 02:40:40 2024
Response via : Initial Calibration

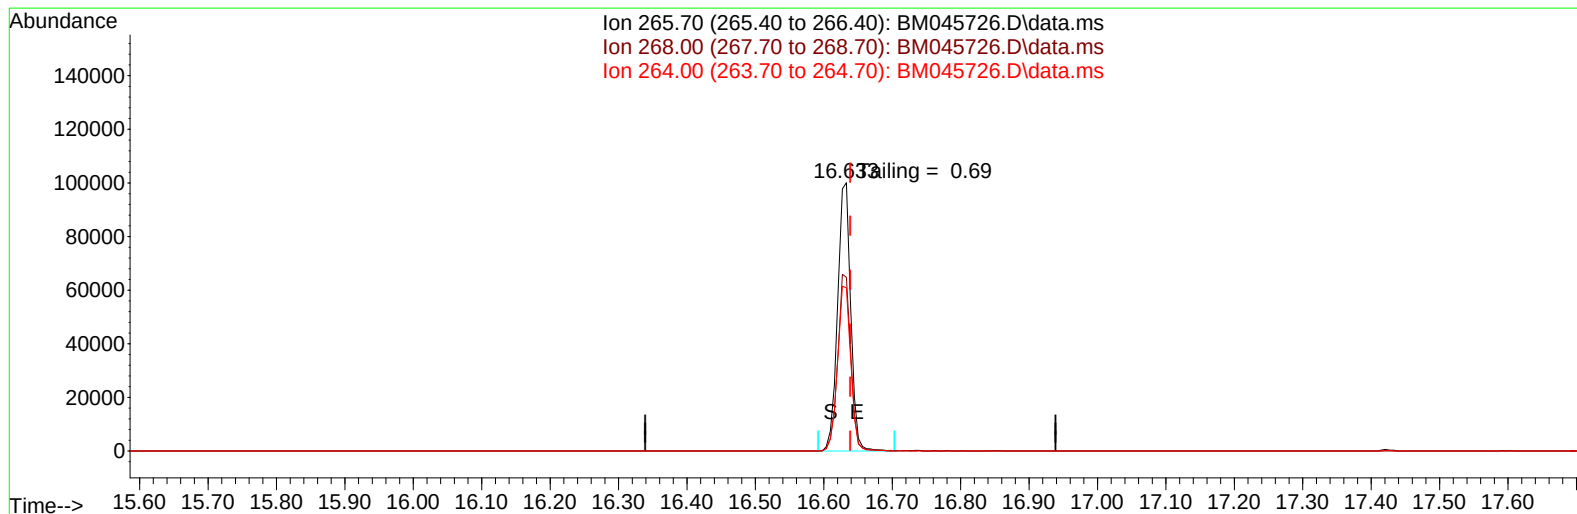

TIC: BM045726.D\data.ms

(70) Pentachlorophenol (C)




16.633min (-0.006) 0.00 ng

response 134028

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.90	64.73
264.00	59.70	60.82
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM051424\
Data File : BM045726.D
Acq On : 14 May 2024 10:50
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 14 12:21:55 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM051424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 14 02:40:40 2024
Response via : Initial Calibration

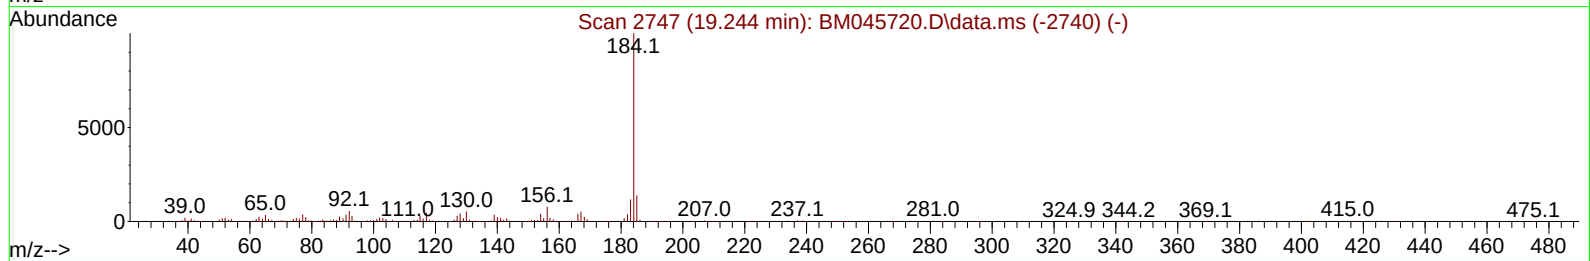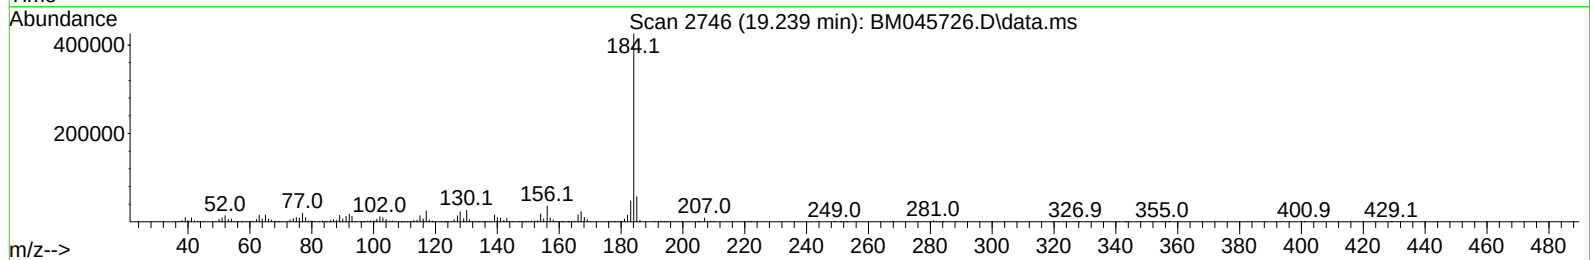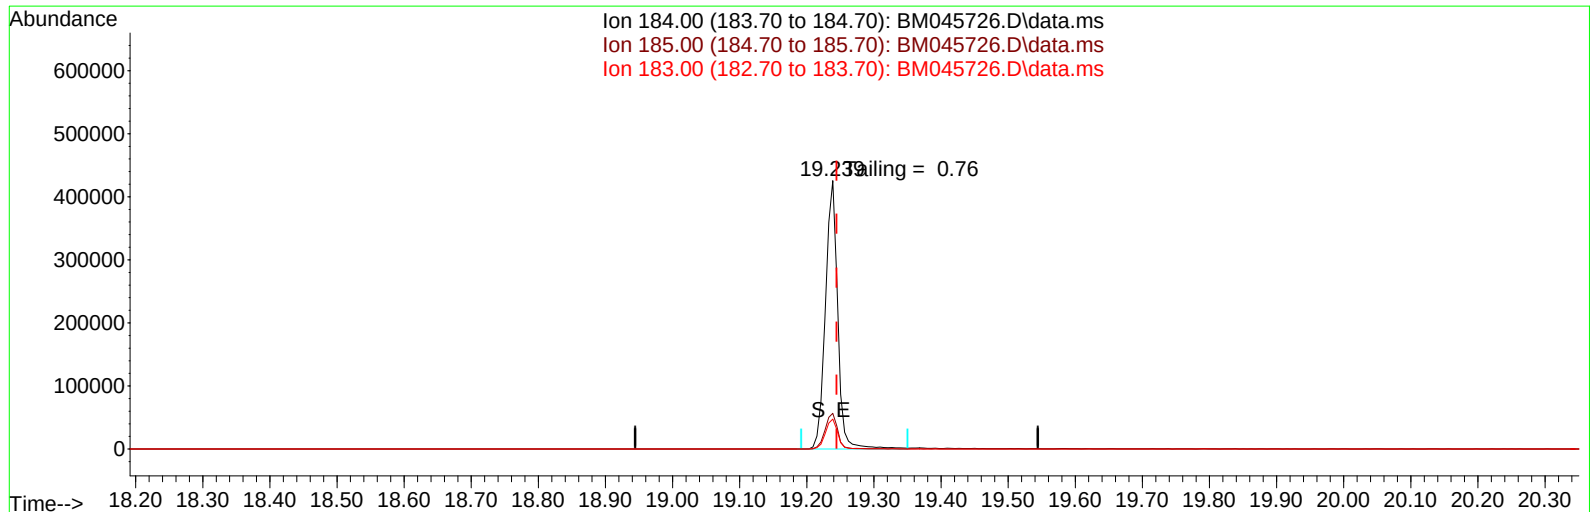

TIC: BM045726.D\data.ms

(77) Benzidine**19.239min (-0.006) 7037.69 ng****response 540941**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	13.30
183.00	11.60	11.15
0.00	0.00	0.00