

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM051424\
Data File : BM045736.D
Acq On : 14 May 2024 18:06
Operator : MA/JU
Sample : PB160855BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB160855BL

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM051424.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM045736.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.263	363	370	383	rVB	2073033	2800193	53.36%	12.502%
2	6.851	632	640	650	rBV	1733229	2672449	50.93%	11.932%
3	7.575	757	763	770	rVB	342109	515582	9.82%	2.302%
4	8.745	952	962	971	rBV	1036039	1746620	33.28%	7.798%
5	10.345	1228	1234	1242	rVB	356978	590656	11.26%	2.637%
6	12.833	1650	1657	1664	rVB	2398041	3263914	62.20%	14.572%
7	14.210	1884	1891	1897	rVB	419466	614755	11.71%	2.745%
8	15.704	2139	2145	2156	rBV	2187615	2874317	54.77%	12.833%
9	16.951	2351	2357	2363	rVB	532450	705943	13.45%	3.152%
10	19.592	2800	2806	2811	rBV	5330800	5247782	100.00%	23.429%
11	21.168	3069	3074	3079	rVB	473089	623140	11.87%	2.782%
12	23.968	3543	3550	3558	rVB	318975	742835	14.16%	3.316%




Sum of corrected areas: 22398186

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM051424\
Data File : BM045736.D
Acq On : 14 May 2024 18:06
Operator : MA/JU
Sample : PB160855BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB160855BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM051424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

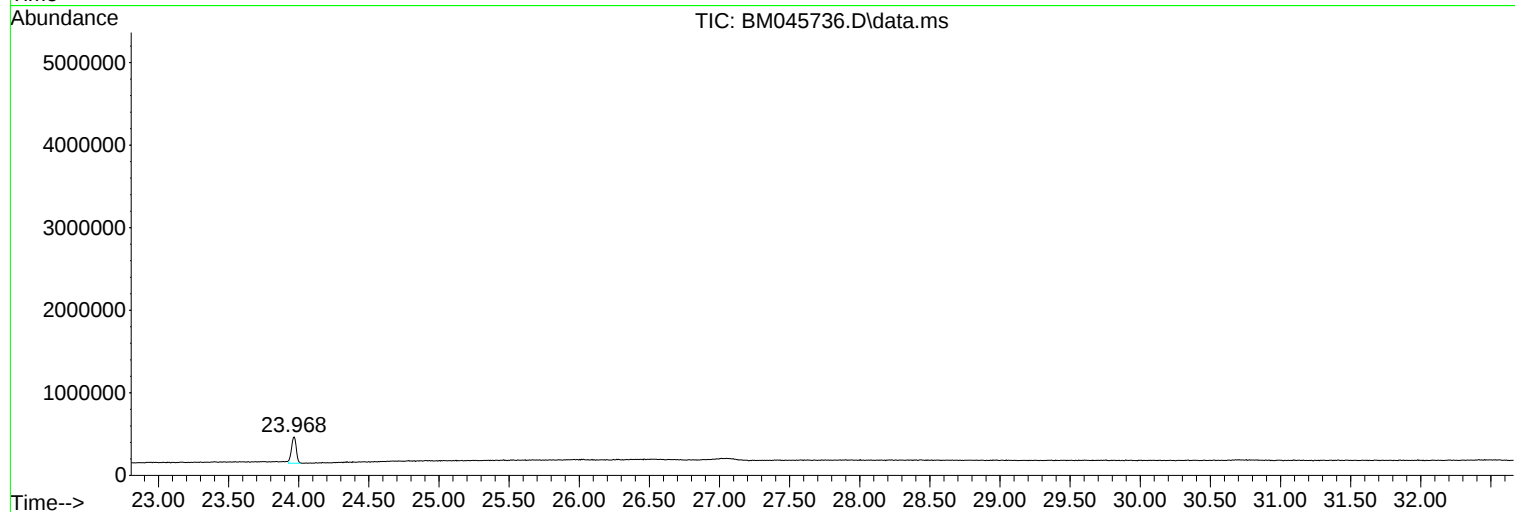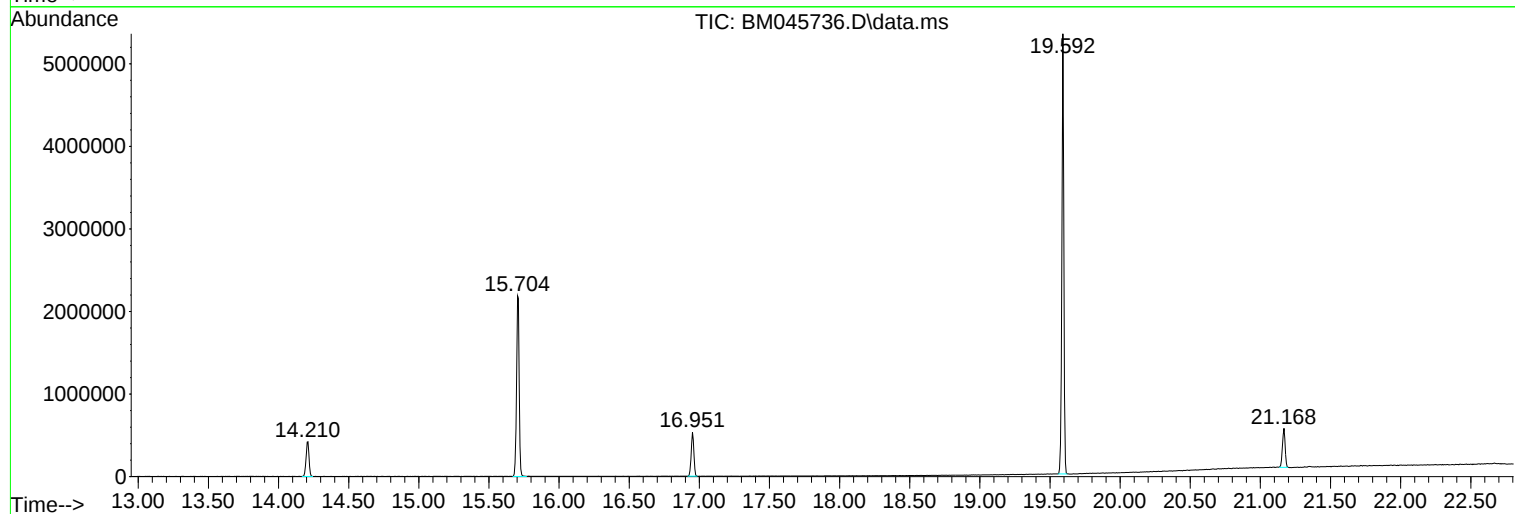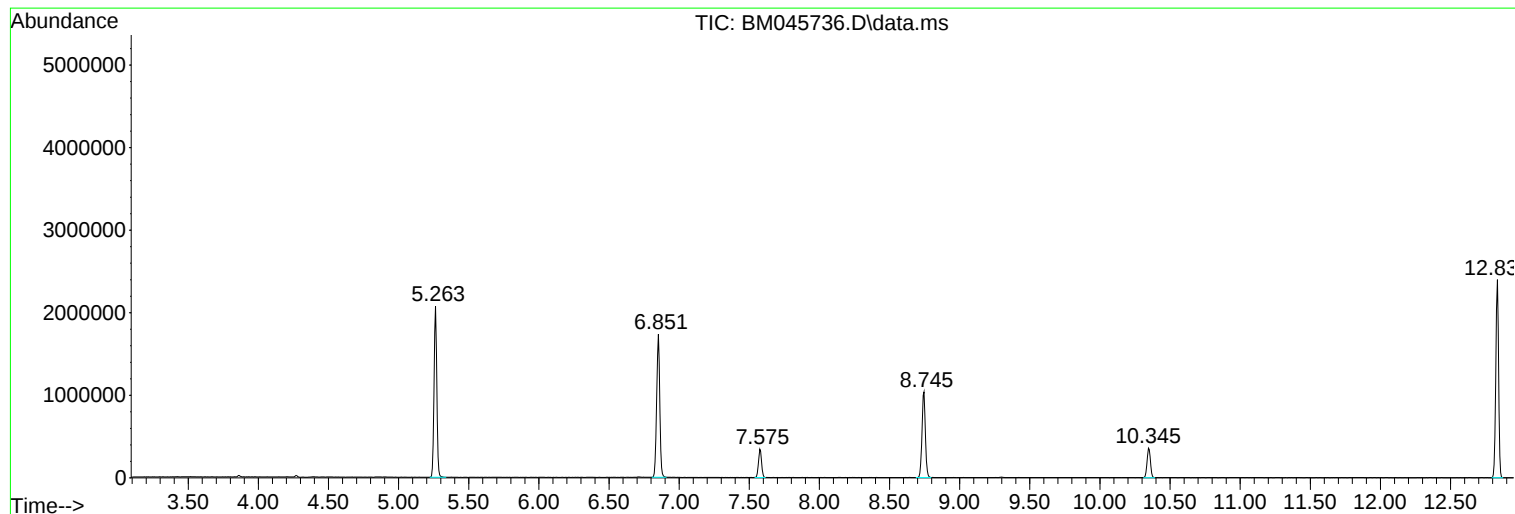

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM051424\
Data File : BM045736.D
Acq On : 14 May 2024 18:06
Operator : MA/JU
Sample : PB160855BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB160855BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM051424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM051424\
Data File : BM045736.D
Acq On : 14 May 2024 18:06
Operator : MA/JU
Sample : PB160855BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB160855BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM051424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------