
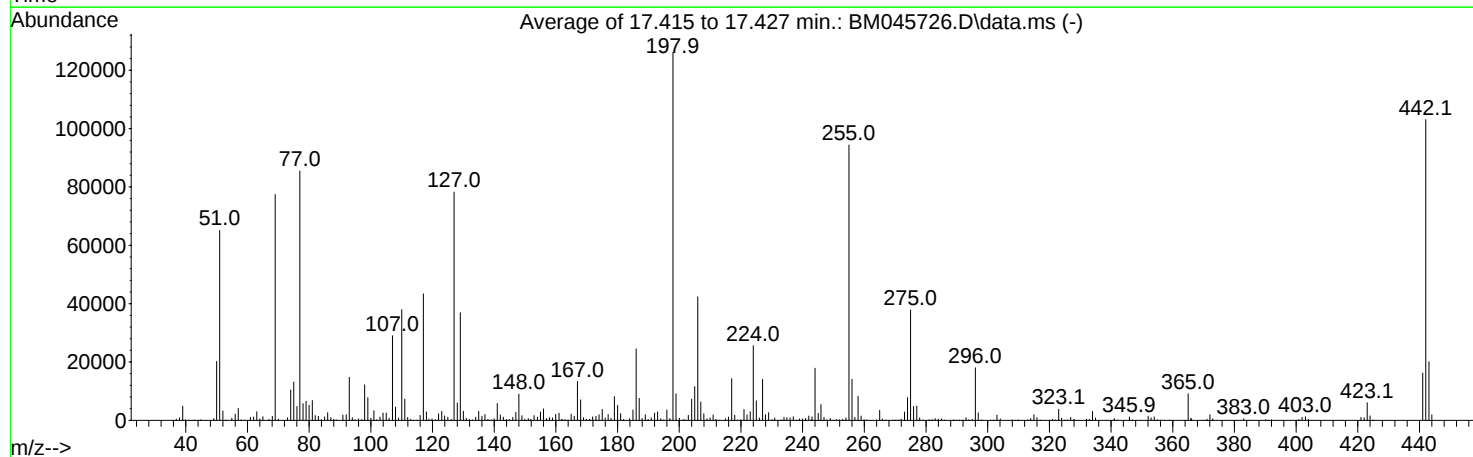


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM051424\
Data File : BM045726.D
Acq On : 14 May 2024 10:50
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM051424.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed May 15 01:43:14 2024

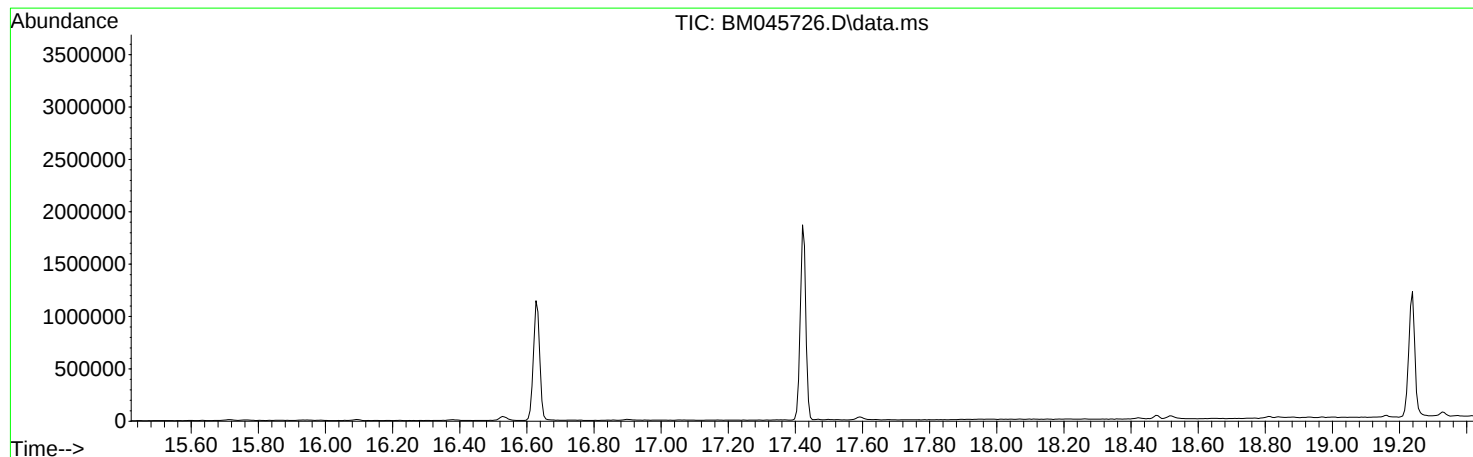




AutoFind: Scans 2436, 2437, 2438; Background Corrected with Scan 2430

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	51.6	65120	PASS
68	69	0.00	2	1.8	1357	PASS
69	198	0.00	100	61.4	77469	PASS
70	69	0.00	2	0.6	458	PASS
127	198	10	80	62.1	78288	PASS
197	198	0.00	2	0.5	679	PASS
198	198	100	100	100.0	126101	PASS
199	198	5	9	7.2	9134	PASS
275	198	10	60	30.0	37867	PASS
365	198	1	100	7.2	9117	PASS
441	198	0.01	100	12.9	16243	PASS
442	442	50	100	100.0	103117	PASS
443	442	15	24	19.5	20086	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM051424\
Data File : BM045726.D
Acq On : 14 May 2024 10:50
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: May 14 12:21:55 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM051424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 14 02:40:40 2024
Response via : Initial Calibration

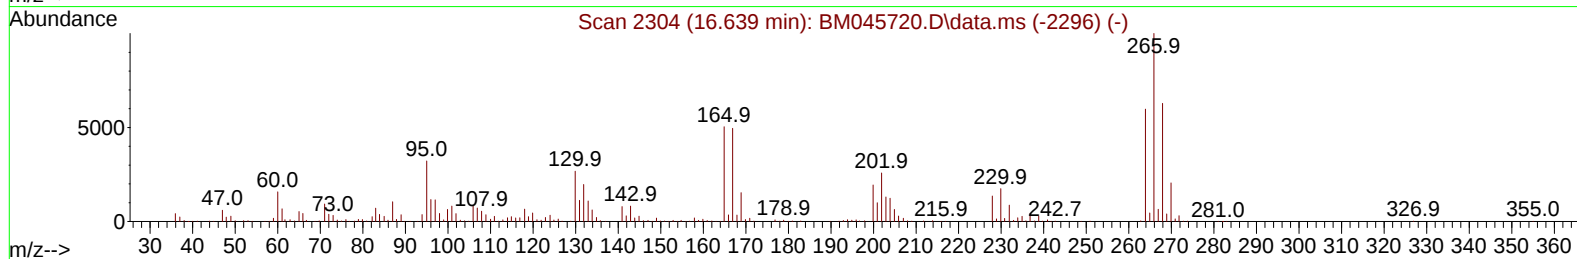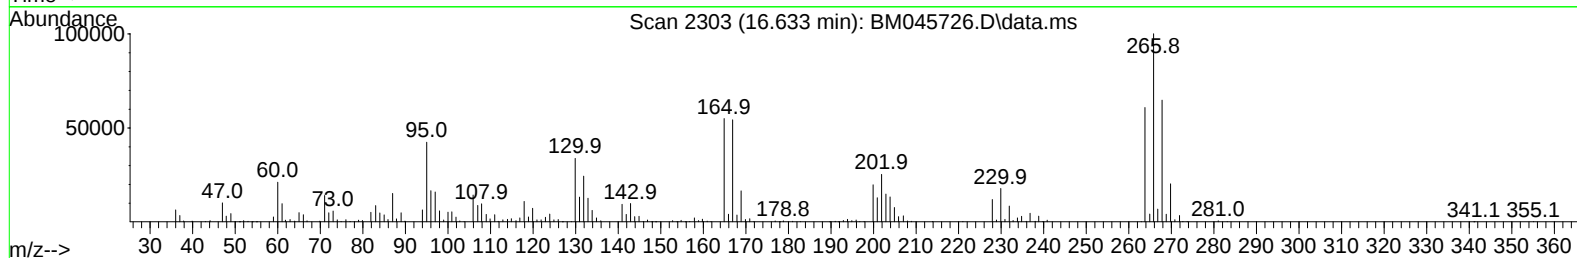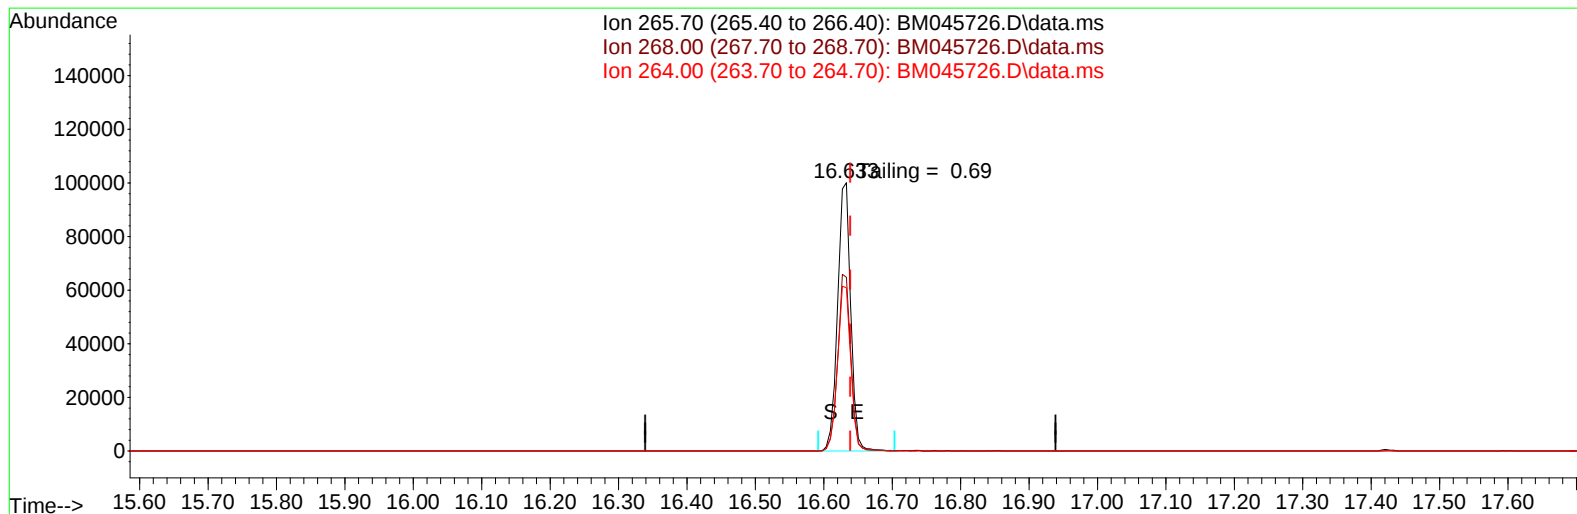

TIC: BM045726.D\data.ms

(70) Pentachlorophenol (C)

16.633min (-0.006) 0.00 ng




response 134028

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.90	64.73
264.00	59.70	60.82
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM051424\
Data File : BM045726.D
Acq On : 14 May 2024 10:50
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: May 14 12:21:55 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM051424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 14 02:40:40 2024
Response via : Initial Calibration

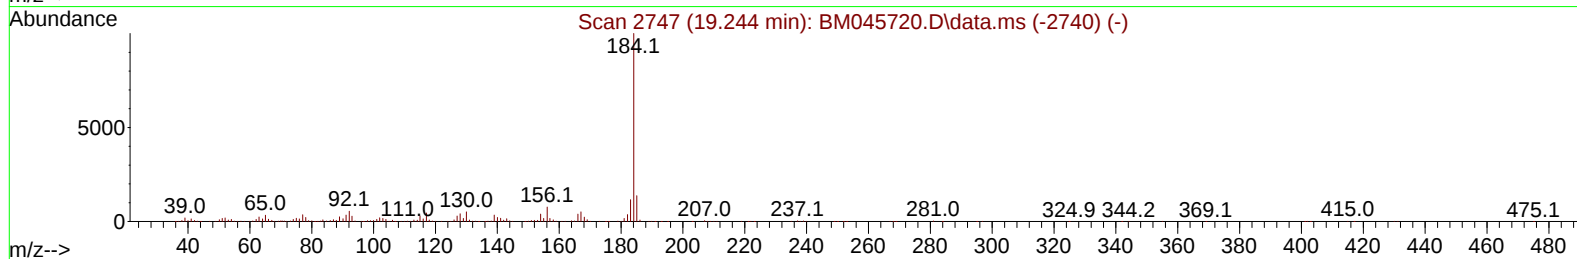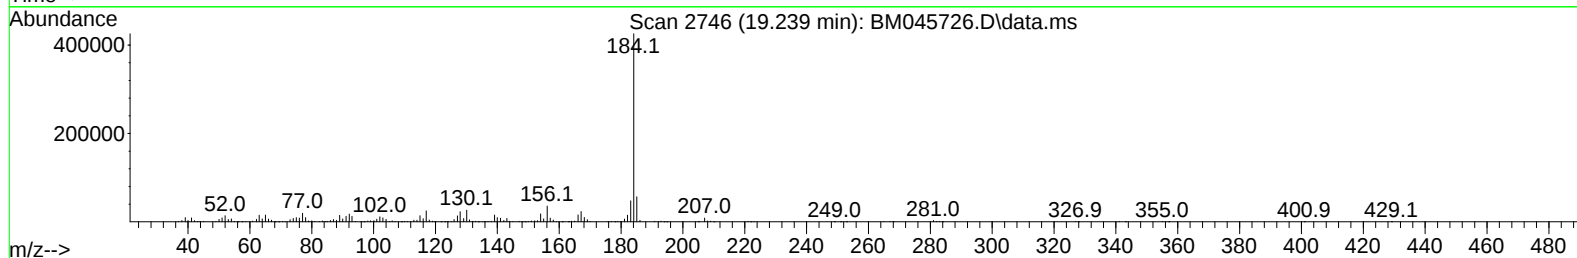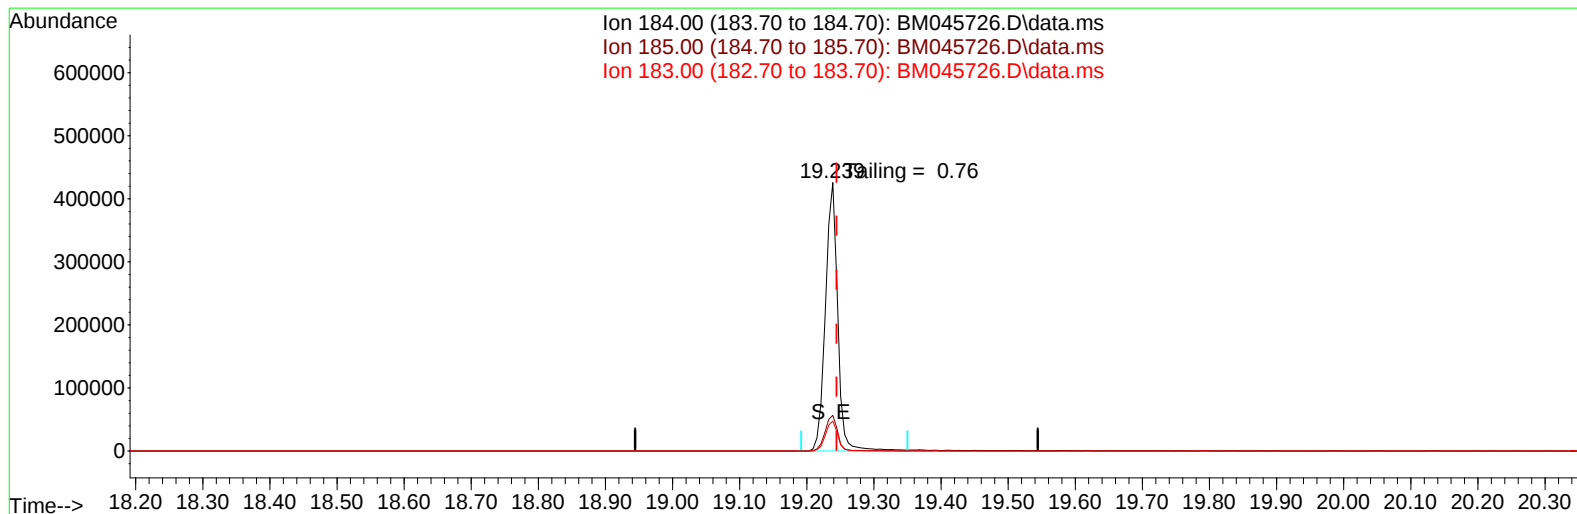

TIC: BM045726.D\data.ms

(77) Benzidine**19.239min (-0.006) 7037.69 ng****response 540941**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	13.30
183.00	11.60	11.15
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/14/2024	BNA_M	<u>BM045726.D</u>
Compound Name	Response	Retention Time
DDT	534735	20.45
DDD	8366	20.015
DDE	299	19.503
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8665	543400	1.59

Instrument :
BNA_M
ClientSampleId :
DFTPP