

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM051515\
 Data File : BM001291.D
 Acq On : 14 May 2015 13:38
 Operator : TP/IZ
 Sample : PB83265BL
 Misc : SBLK60
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK60

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM051515.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.869	28	31	36	rBV2	59152	78009	1.53%	0.137%
2	3.187	81	85	86	rBV4	3985	5334	0.10%	0.009%
3	3.440	123	128	134	rVB2	25649	38358	0.75%	0.067%
4	5.651	500	504	508	rBV5	8094	13526	0.27%	0.024%
5	6.440	631	638	641	rBV8	3470	7022	0.14%	0.012%
6	6.628	661	670	684	rBV	1108533	1668108	32.68%	2.932%
7	6.781	690	696	707	rVV	823292	1231323	24.13%	2.165%
8	6.875	711	712	716	rVB3	4681	5146	0.10%	0.009%
9	6.969	722	728	740	rBV	1092422	1680049	32.92%	2.953%
10	7.069	740	745	752	rVB3	27129	43451	0.85%	0.076%
11	7.439	801	808	815	rBV	865162	1348203	26.42%	2.370%
12	7.663	842	846	851	rBV7	9483	16460	0.32%	0.029%
13	7.981	895	900	905	rVB4	7161	10100	0.20%	0.018%
14	8.110	917	922	925	rBV4	8996	13635	0.27%	0.024%
15	8.163	925	931	946	rVB	1406261	2114712	41.43%	3.718%
16	8.316	953	957	958	rBV4	4754	5370	0.11%	0.009%
17	8.598	997	1005	1012	rBV	1061125	1622973	31.80%	2.853%
18	8.669	1014	1017	1023	rVB3	18500	28116	0.55%	0.049%
19	9.034	1073	1079	1082	rBV7	3623	5899	0.12%	0.010%
20	9.316	1120	1127	1137	rBV	890771	1419830	27.82%	2.496%
21	9.851	1211	1218	1228	rBV	1330366	2110033	41.34%	3.709%
22	10.222	1273	1281	1288	rBV	1181748	1903699	37.30%	3.347%
23	10.369	1299	1306	1321	rBV	1373168	2252431	44.13%	3.960%
24	12.451	1656	1660	1667	rVB4	9611	15416	0.30%	0.027%
25	12.710	1698	1704	1708	rBV3	13777	21422	0.42%	0.038%
26	13.533	1838	1844	1856	rVB	2130455	2919383	57.20%	5.132%
27	13.804	1883	1890	1899	rBV	2704757	3709547	72.68%	6.521%
28	14.116	1937	1943	1952	rBV2	1575637	2336111	45.77%	4.107%
29	14.339	1975	1981	1997	rBV	1006299	1424885	27.92%	2.505%
30	14.557	2014	2018	2021	rVB3	11280	15017	0.29%	0.026%
31	15.115	2107	2113	2123	rBV	3247893	4480871	87.79%	7.877%
32	15.251	2130	2136	2148	rBV	1138241	1494133	29.27%	2.627%
33	15.357	2150	2154	2158	rVB3	25033	32837	0.64%	0.058%
34	16.657	2371	2375	2379	rVB	6776	9805	0.19%	0.017%

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM051515\
Data File : BM001291.D
Acq On : 14 May 2015 13:38
Operator : TP/IZ
Sample : PB83265BL
Misc : SBLK60
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK60

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0.1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM051515.M
Title : SVOA CALIBRATION

35	16.868	2404	2411	2417	rBV	1845148	2503204	49.04%	4.400%
36	16.968	2421	2428	2439	rBV	3349902	4661542	91.33%	8.195%
37	17.080	2445	2447	2450	rVB4	6947	6731	0.13%	0.012%
38	17.780	2562	2566	2569	rBV3	4513	7333	0.14%	0.013%
39	18.651	2709	2714	2717	rVV4	6451	7710	0.15%	0.014%
40	19.156	2795	2800	2806	rBV	27146	33198	0.65%	0.058%
41	19.227	2806	2812	2813	rBV5	6804	8779	0.17%	0.015%
42	19.274	2813	2820	2828	rBV	3968513	5103904	100.00%	8.972%
43	20.274	2985	2990	2996	rBV9	12409	26832	0.53%	0.047%
44	20.580	3040	3042	3044	rBV3	4870	5691	0.11%	0.010%
45	20.874	3089	3092	3096	rVB2	27499	30759	0.60%	0.054%
46	21.074	3120	3126	3134	rBV	2229361	2701606	52.93%	4.749%
47	23.056	3456	3463	3474	rBV2	3012114	5011208	98.18%	8.809%
48	23.191	3479	3486	3494	rVB	1585505	2694954	52.80%	4.738%


Sum of corrected areas: 56884665

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM051515\
Data File : BM001291.D
Acq On : 14 May 2015 13:38
Operator : TP/IZ
Sample : PB83265BL
Misc : SBLK60
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK60

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM051515.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

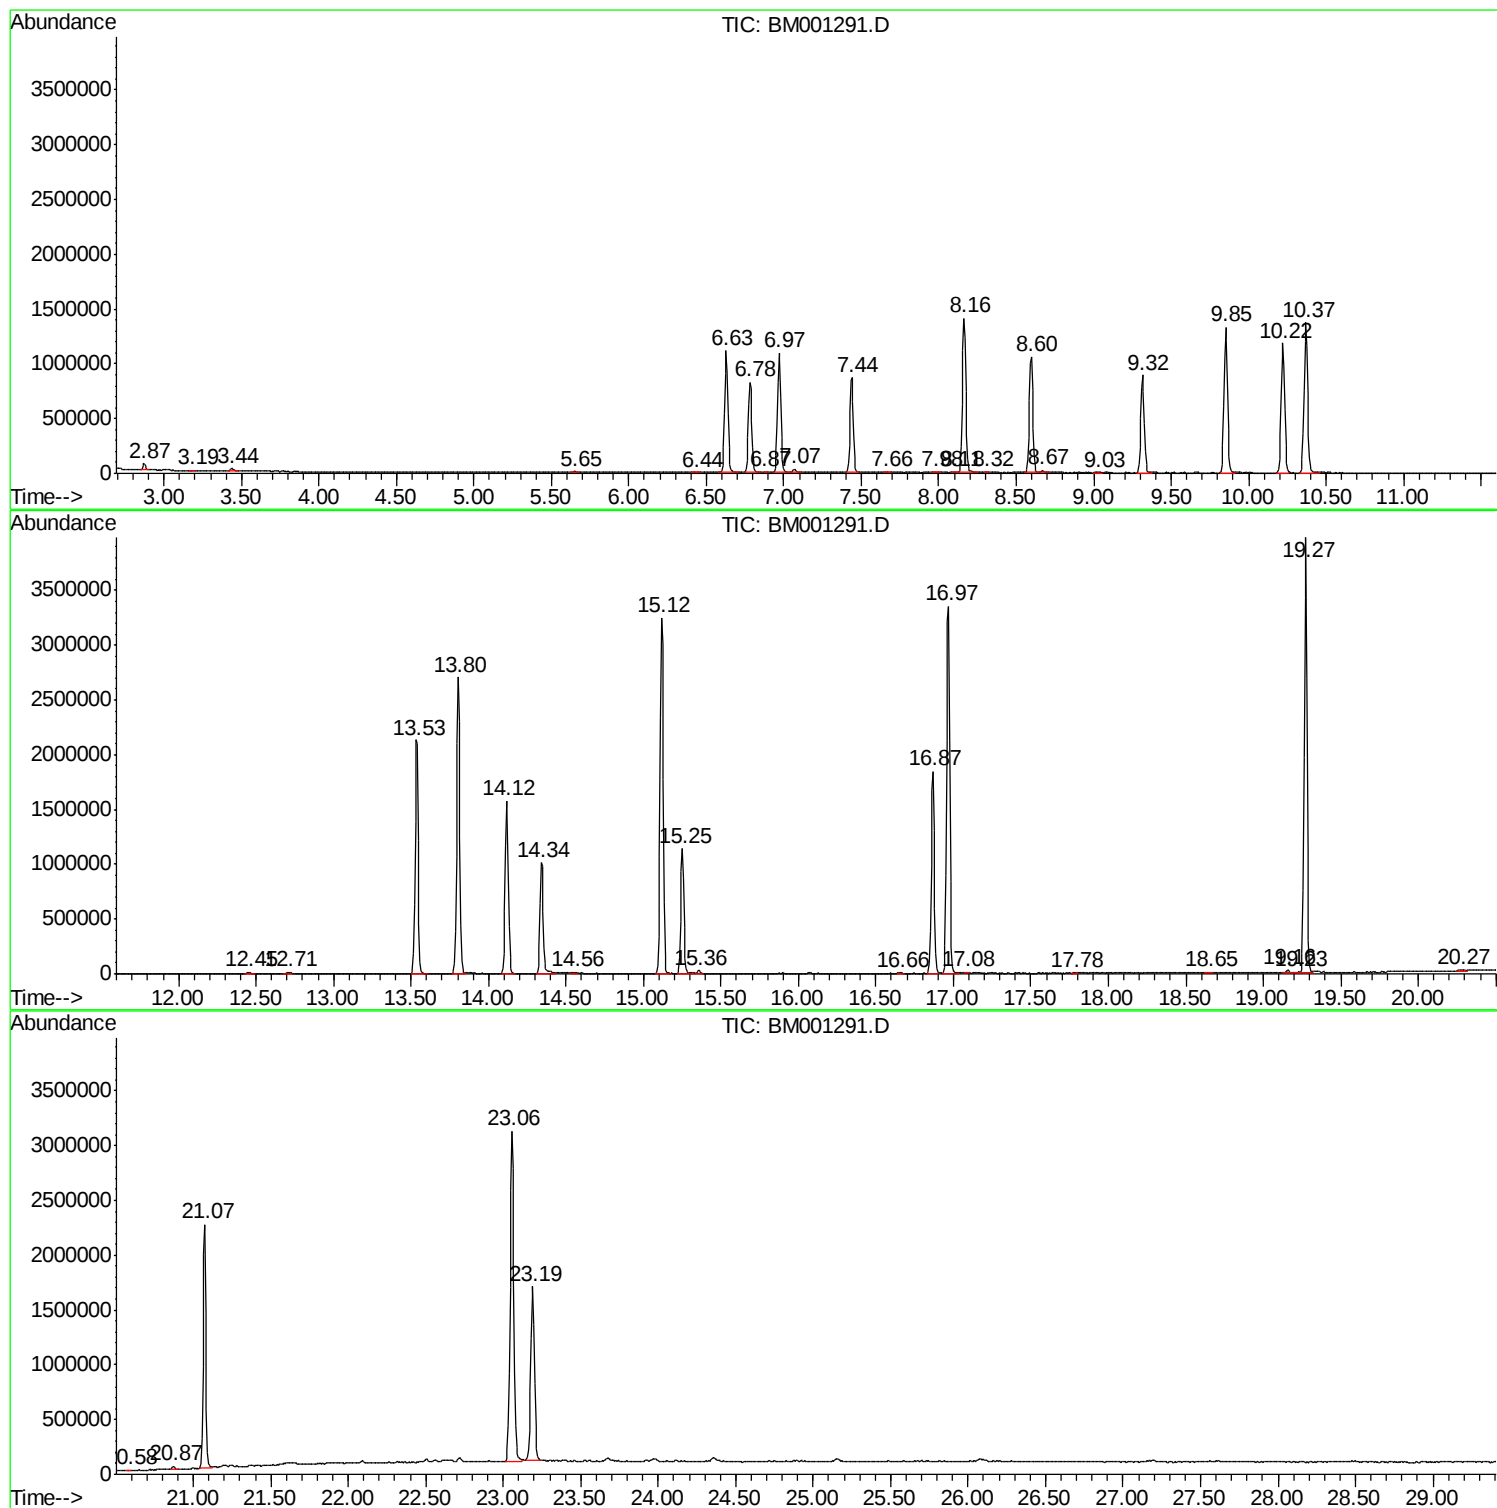

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM051515\
Data File : BM001291.D
Acq On : 14 May 2015 13:38
Operator : TP/IZ
Sample : PB83265BL
Misc : SBLK60
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK60

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM051515.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM051515\
Data File : BM001291.D
Acq On : 14 May 2015 13:38
Operator : TP/IZ
Sample : PB83265BL
Misc : SBLK60
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK60

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM051515.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc