
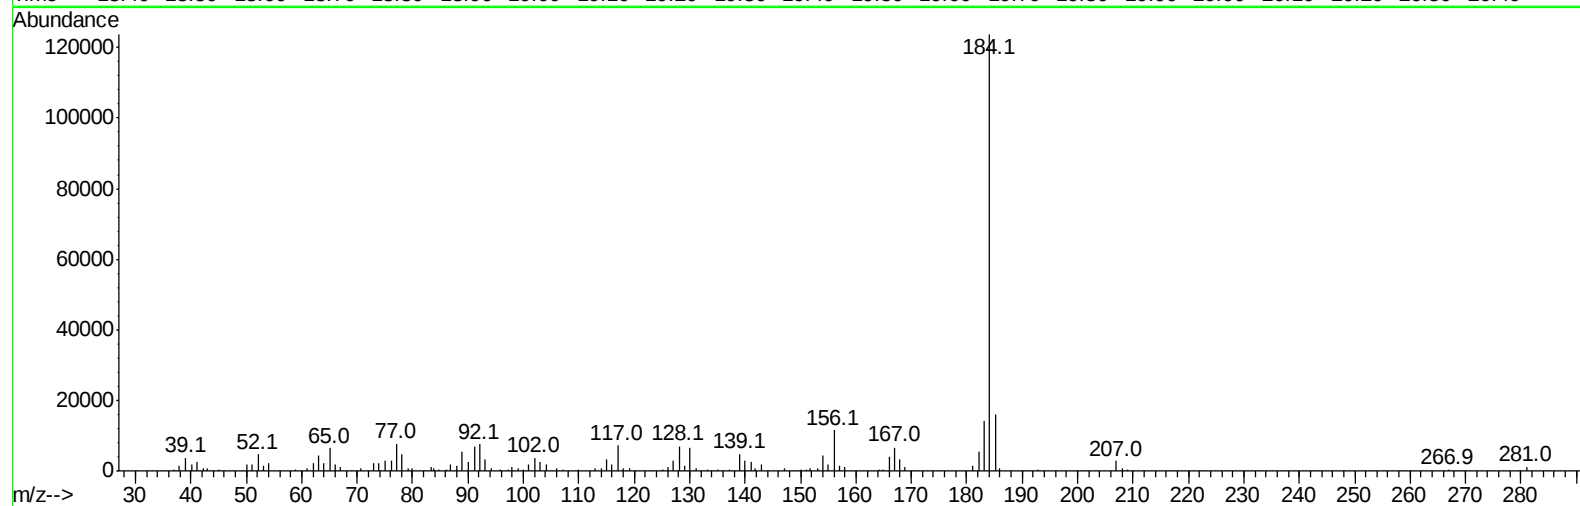


Data Path : Z:\HPCHEM1\BNA M\DATA\BM051517\
Data File : BM010039.D
Acq On : 15 May 2017 14:03
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 16 05:11:16 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM051117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 11 19:50:16 2017
Response via : Initial Calibration

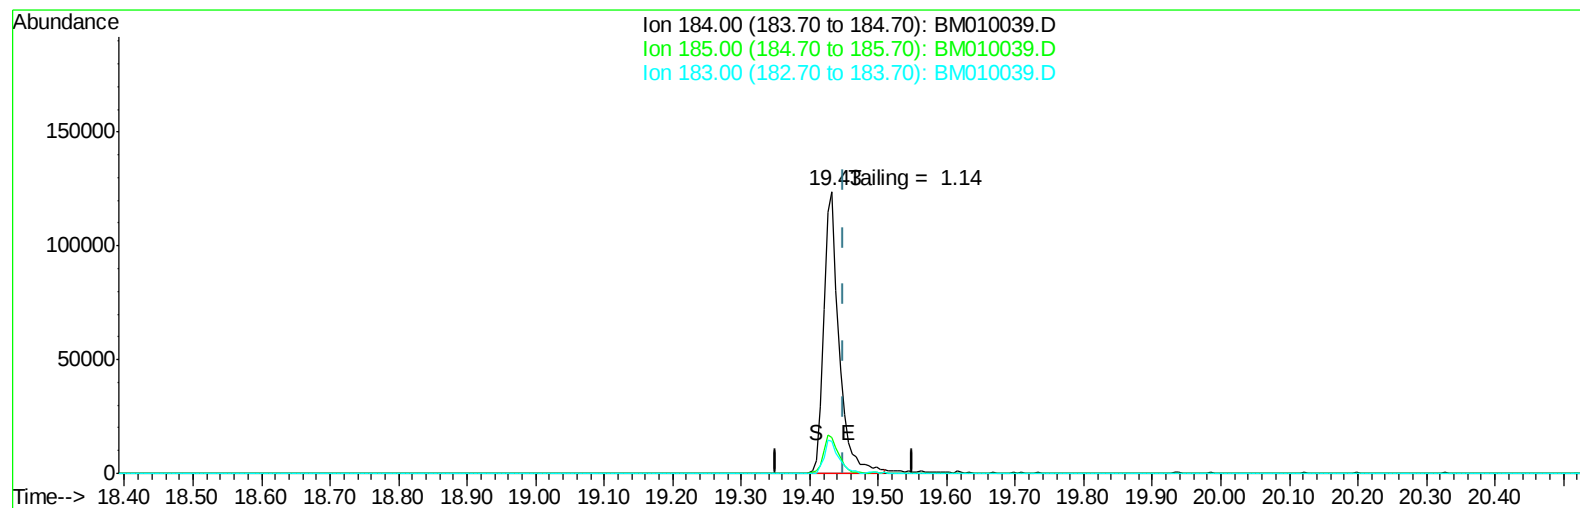

TIC: BM010039.D

(76) Benzidine



19.433min (-0.018) 0.00ng

response 194265

Ion	Exp%	Act%
184.00	100	100
185.00	14.10	12.77
183.00	11.10	11.35
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA M\DATA\BM051517\
Data File : BM010039.D
Acq On : 15 May 2017 14:03
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 16 05:11:16 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM051117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 11 19:50:16 2017
Response via : Initial Calibration

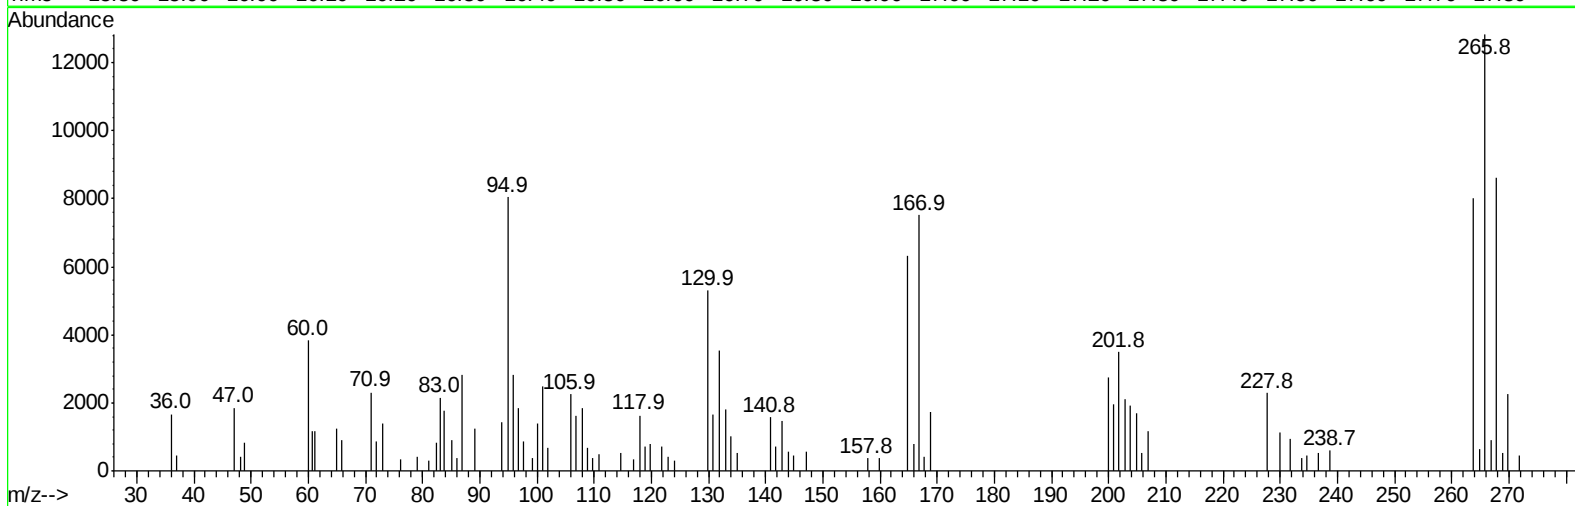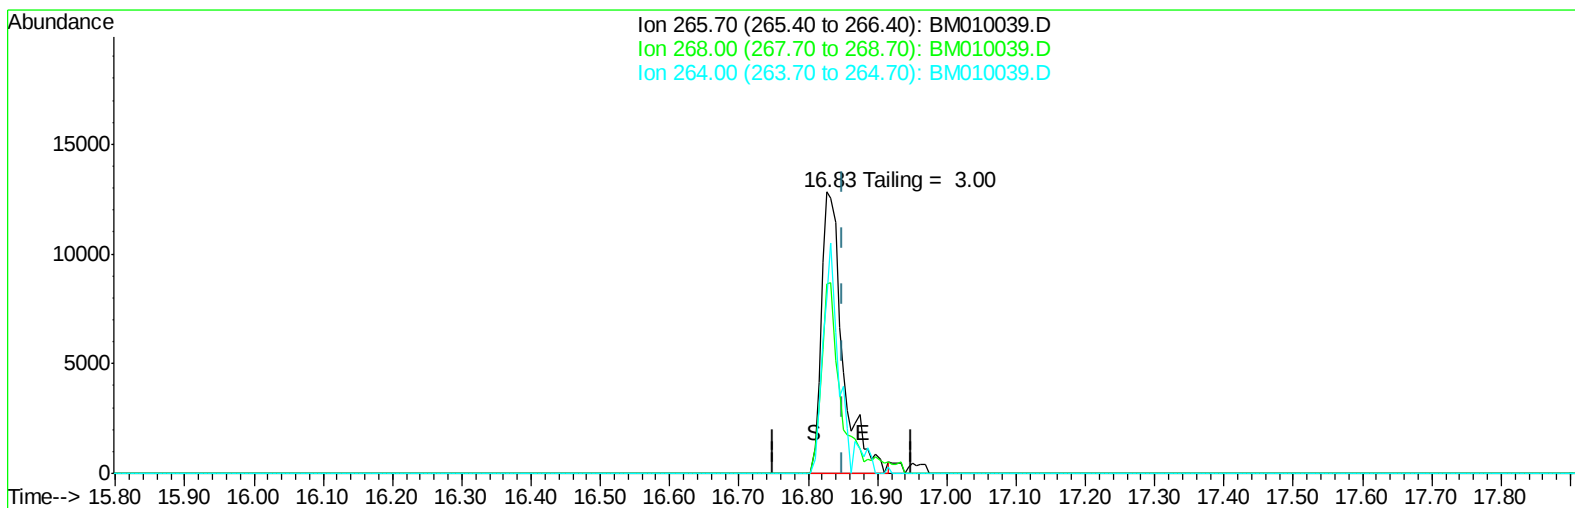

TIC: BM010039.D

(69) Pentachlorophenol (C)

16.827min (-0.023) 0.00ng

response 27200

Ion	Exp%	Act%
265.70	100	100
268.00	65.00	67.08
264.00	61.20	62.50
0.00	0.00	0.00