


Data Path : Z:\HPCHEM1\BNA_M\Data\BM051517\
 Data File : BM010039.D
 Acq On : 15 May 2017 14:03
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM051117.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu May 11 19:50:16 2017

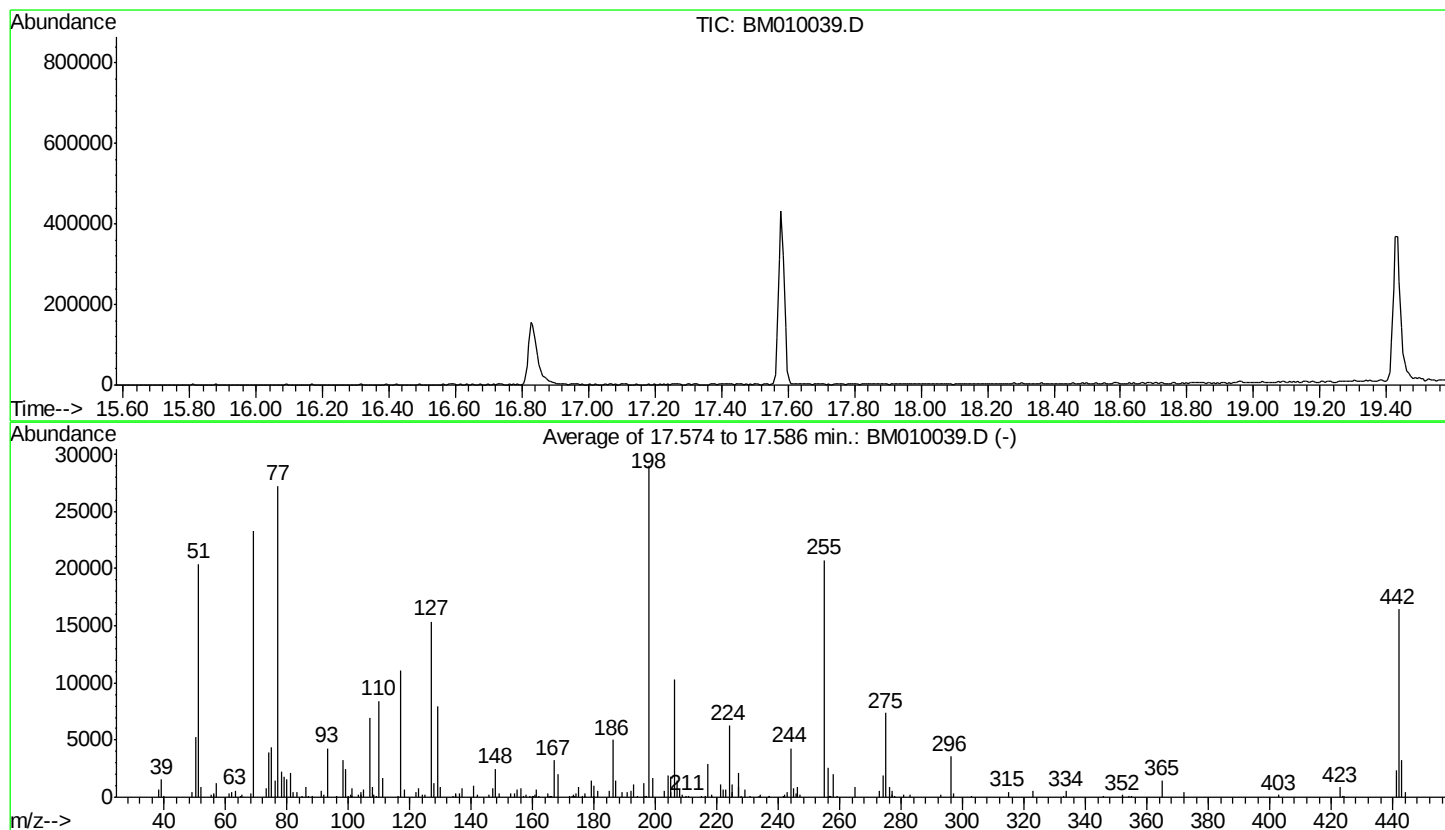

AutoFind: Scans 2463, 2464, 2465; Background Corrected with Scan 2458

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	70.4	20408	PASS
68	69	0.00	2	1.5	348	PASS
69	198	0.00	100	80.3	23290	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	53.0	15387	PASS
197	198	0.00	2	0.5	155	PASS
198	198	100	100	100.0	29008	PASS
199	198	5	9	5.9	1714	PASS
275	198	10	60	25.4	7368	PASS
365	198	1	100	5.0	1439	PASS
441	442	0.01	24	14.0	2306	PASS
442	198	50	100	56.7	16454	PASS
443	442	15	24	19.4	3196	PASS