

Quantitation Report (LSC Reviewed)


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM051520\
 Data File : BM025999.D
 Acq On : 15 May 2020 23:25
 Operator : MA/SJ
 Sample : L2634-02
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 COAH0

Manual Integrations
 APPROVED

Sohil
 5/18/2020 10:00:27 AM

Quant Time: May 16 06:10:04 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 15 12:17:41 2020
 Response via : Initial Calibration

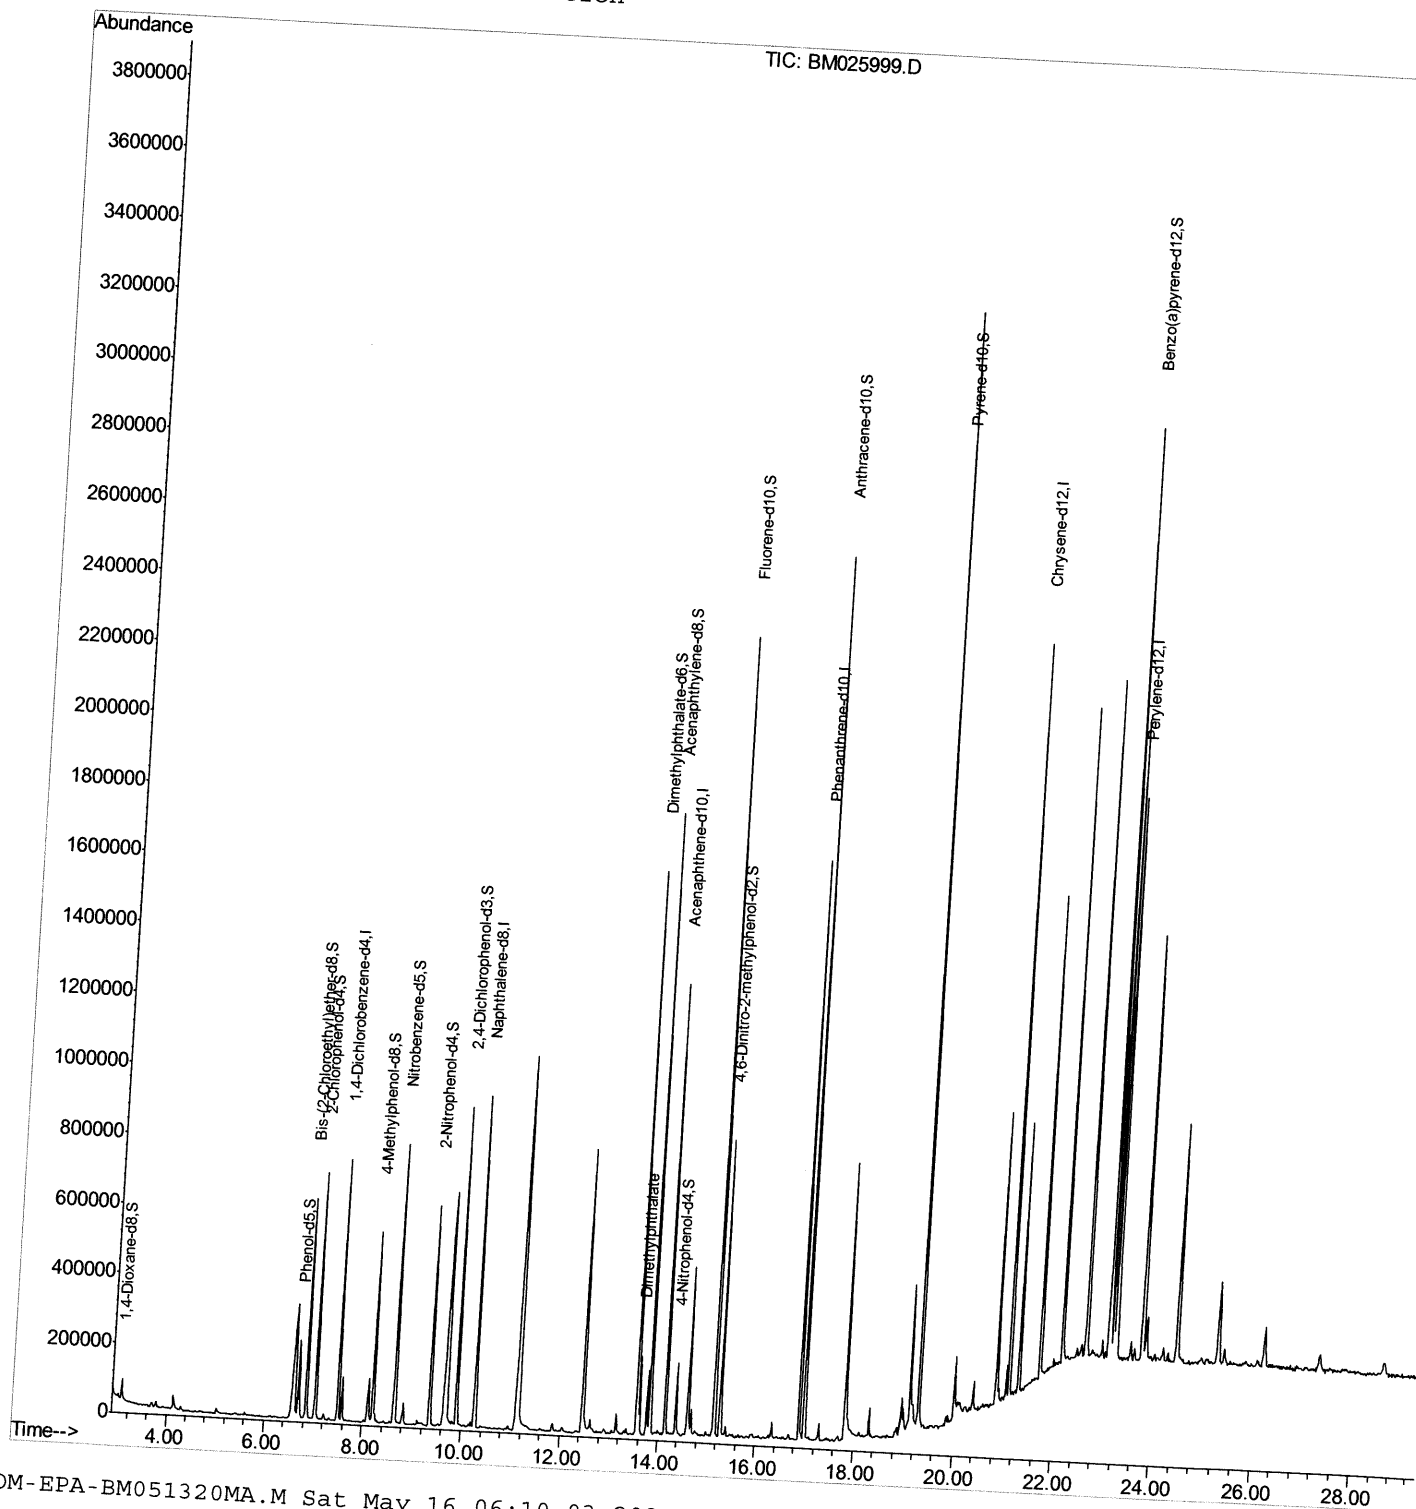

Quantitation Report (Qedit)


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM051520\
 Data File : BM025999.D
 Acq On : 15 May 2020 23:25
 Operator : MA/SJ
 Sample : L2634-02
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 COAH0

Manual Integrations
 APPROVED

Sohil
 5/18/2020 10:00:27 AM

Quant Time: May 16 01:41:31 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 15 12:17:41 2020
 Response via : Initial Calibration

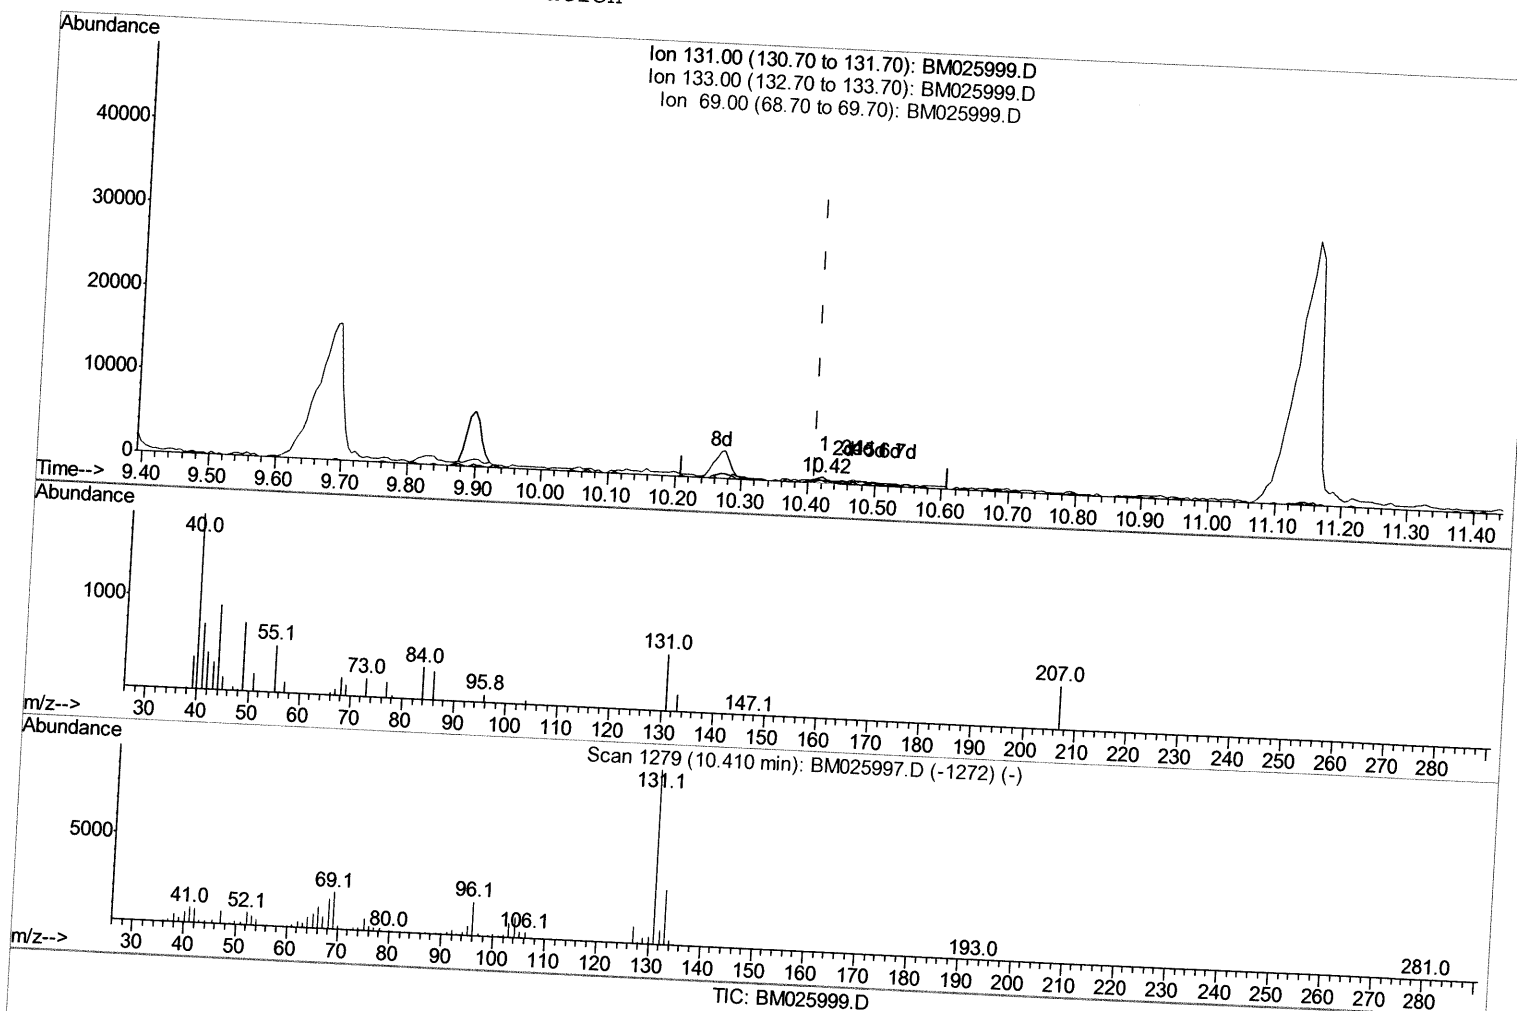

(29) 4-Chloroaniline-d4 (S)

10.422min (+0.012) 0.11ng/ul

response 1182

Ion	Exp%	Act%
131.00	100	100
133.00	34.00	44.87#
69.00	21.90	37.59#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM051520\
 Data File : BM025999.D
 Acq On : 15 May 2020 23:25
 Operator : MA/SJ
 Sample : L2634-02
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AH0

Manual Integrations
 APPROVED

Sohil
 5/18/2020 10:00:27 AM

Quant Time: May 16 01:41:31 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 15 12:17:41 2020
 Response via : Initial Calibration

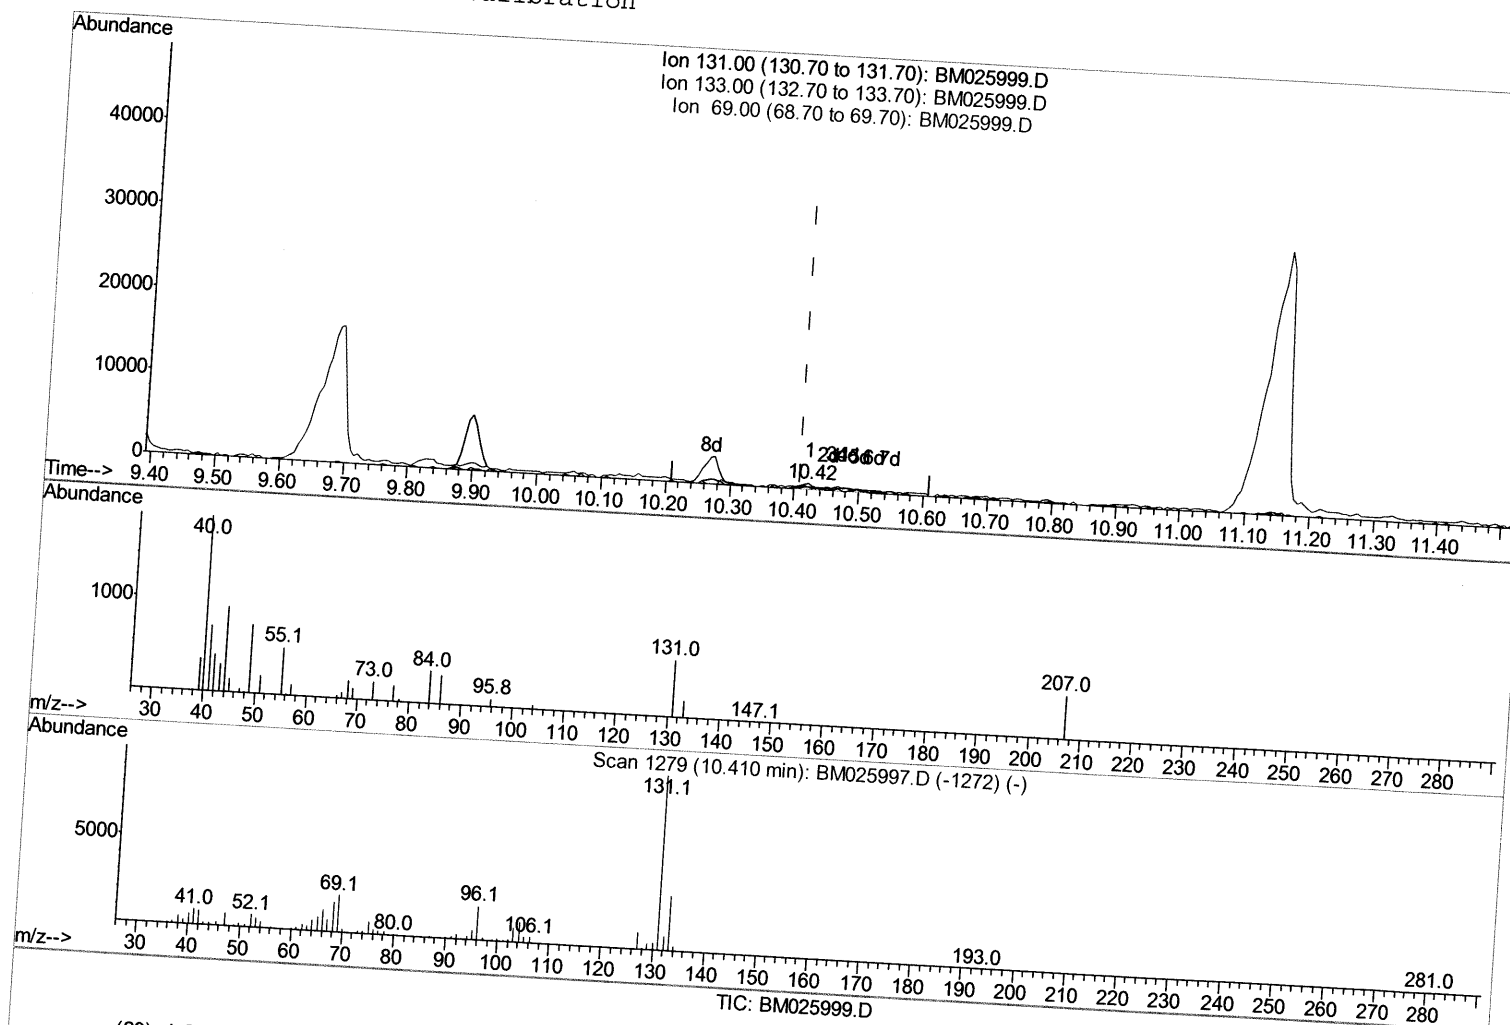

(29) 4-Chloroaniline-d4 (S)

10.422min (+0.012) 0.21ng/ul m 05/18/20 AP

response 2328

Ion	Exp%	Act%
131.00	100	100
133.00	34.00	44.87#
69.00	21.90	37.59#
0.00	0.00	0.00

Quantitation Report (LSC Reviewed)

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM051520\
 Data File : BM025999.D
 Acq On : 15 May 2020 23:25
 Operator : MA/SJ
 Sample : L2634-02
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 COAH0

Manual Integrations
 APPROVED

Sohil
 5/18/2020 10:00:27 AM

Quant Time: May 16 06:10:04 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 15 12:17:41 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.50	152	169988	20.00	ng/ul	0.00
18) Naphthalene-d8	10.27	136	679358	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.15	164	393944	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.90	188	846072	20.00	ng/ul	0.00
78) Chrysene-d12	21.09	240	912667	20.00	ng/ul	0.00
86) Perylene-d12	23.22	264	980198	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.08	96	29826	5.29	ng/uL	0.00
5) Phenol-d5	6.69	99	100188	6.50	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.85	67	287353	26.94	ng/ul	0.00
9) 2-Chlorophenol-d4	7.05	132	257457	21.33	ng/ul	0.00
13) 4-Methylphenol-d8	8.22	113	177078	15.24	ng/ul	0.00
19) Nitrobenzene-d5	8.65	128	152724	27.58	ng/ul	0.00
22) 2-Nitrophenol-d4	9.36	143	156858	28.63	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.90	165	276759	25.16	ng/ul	0.00
29) 4-Chloroaniline-d4	10.42	131	2328m	0.21	ng/ul	0.01
44) Dimethylphthalate-d6	13.57	166	913633	28.92	ng/ul	0.00
47) Acenaphthylene-d8	13.83	160	1066856	28.51	ng/ul	0.00
52) 4-Nitrophenol-d4	14.36	143	39311	7.03	ng/ul	0.00
58) Fluorene-d10	15.15	176	793486	28.88	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.27	200	133814	27.13	ng/ul	0.00
71) Anthracene-d10	16.99	188	1256521	30.14	ng/ul	0.00
79) Pyrene-d10	19.30	212	1465403	31.26	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.09	264	1651759	31.66	ng/ul	0.00
Target Compounds						
45) Dimethylphthalate	13.62	163	115978	3.497	ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed