

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM051520\
 Data File : BM026002.D
 Acq On : 16 May 2020 01:15
 Operator : MA/SJ
 Sample : L2655-02
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0F20

Quant Time: May 16 03:24:55 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 15 12:17:41 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.50	152	175004	20.00	ng/ul	0.00
18) Naphthalene-d8	10.27	136	712787	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.15	164	409362	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.90	188	874296	20.00	ng/ul	0.00
78) Chrysene-d12	21.09	240	901327	20.00	ng/ul	0.00
86) Perylene-d12	23.21	264	963488	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.07	96	28867	4.98	ng/uL	0.00
5) Phenol-d5	6.69	99	100876	6.35	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.85	67	301907	27.49	ng/ul	0.00
9) 2-Chlorophenol-d4	7.05	132	261909	21.08	ng/ul	0.00
13) 4-Methylphenol-d8	8.22	113	179424	15.00	ng/ul	0.00
19) Nitrobenzene-d5	8.65	128	161927	27.87	ng/ul	0.00
22) 2-Nitrophenol-d4	9.36	143	163130	28.38	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.90	165	282058	24.44	ng/ul	0.00
29) 4-Chloroaniline-d4	10.42	131	25800	2.20	ng/ul	0.00
44) Dimethylphthalate-d6	13.57	166	1027725	31.31	ng/ul	0.00
47) Acenaphthylene-d8	13.84	160	1161261	29.86	ng/ul	0.00
52) 4-Nitrophenol-d4	14.36	143	29425	5.06	ng/ul	0.00
58) Fluorene-d10	15.15	176	884233	30.97	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.27	200	141281	27.71	ng/ul	0.00
71) Anthracene-d10	17.00	188	1441358	33.45	ng/ul	0.00
79) Pyrene-d10	19.30	212	1618463	34.96	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.09	264	1752342	34.17	ng/ul	0.00


Target Compounds					Ovalue	
45) Dimethylphthalate	13.62	163	136025	3.947	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM051520\
Data File : BM026002.D
Acq On : 16 May 2020 01:15
Operator : MA/SJ
Sample : L2655-02
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0F20

Quant Time: May 16 03:24:55 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri May 15 12:17:41 2020
Response via : Initial Calibration

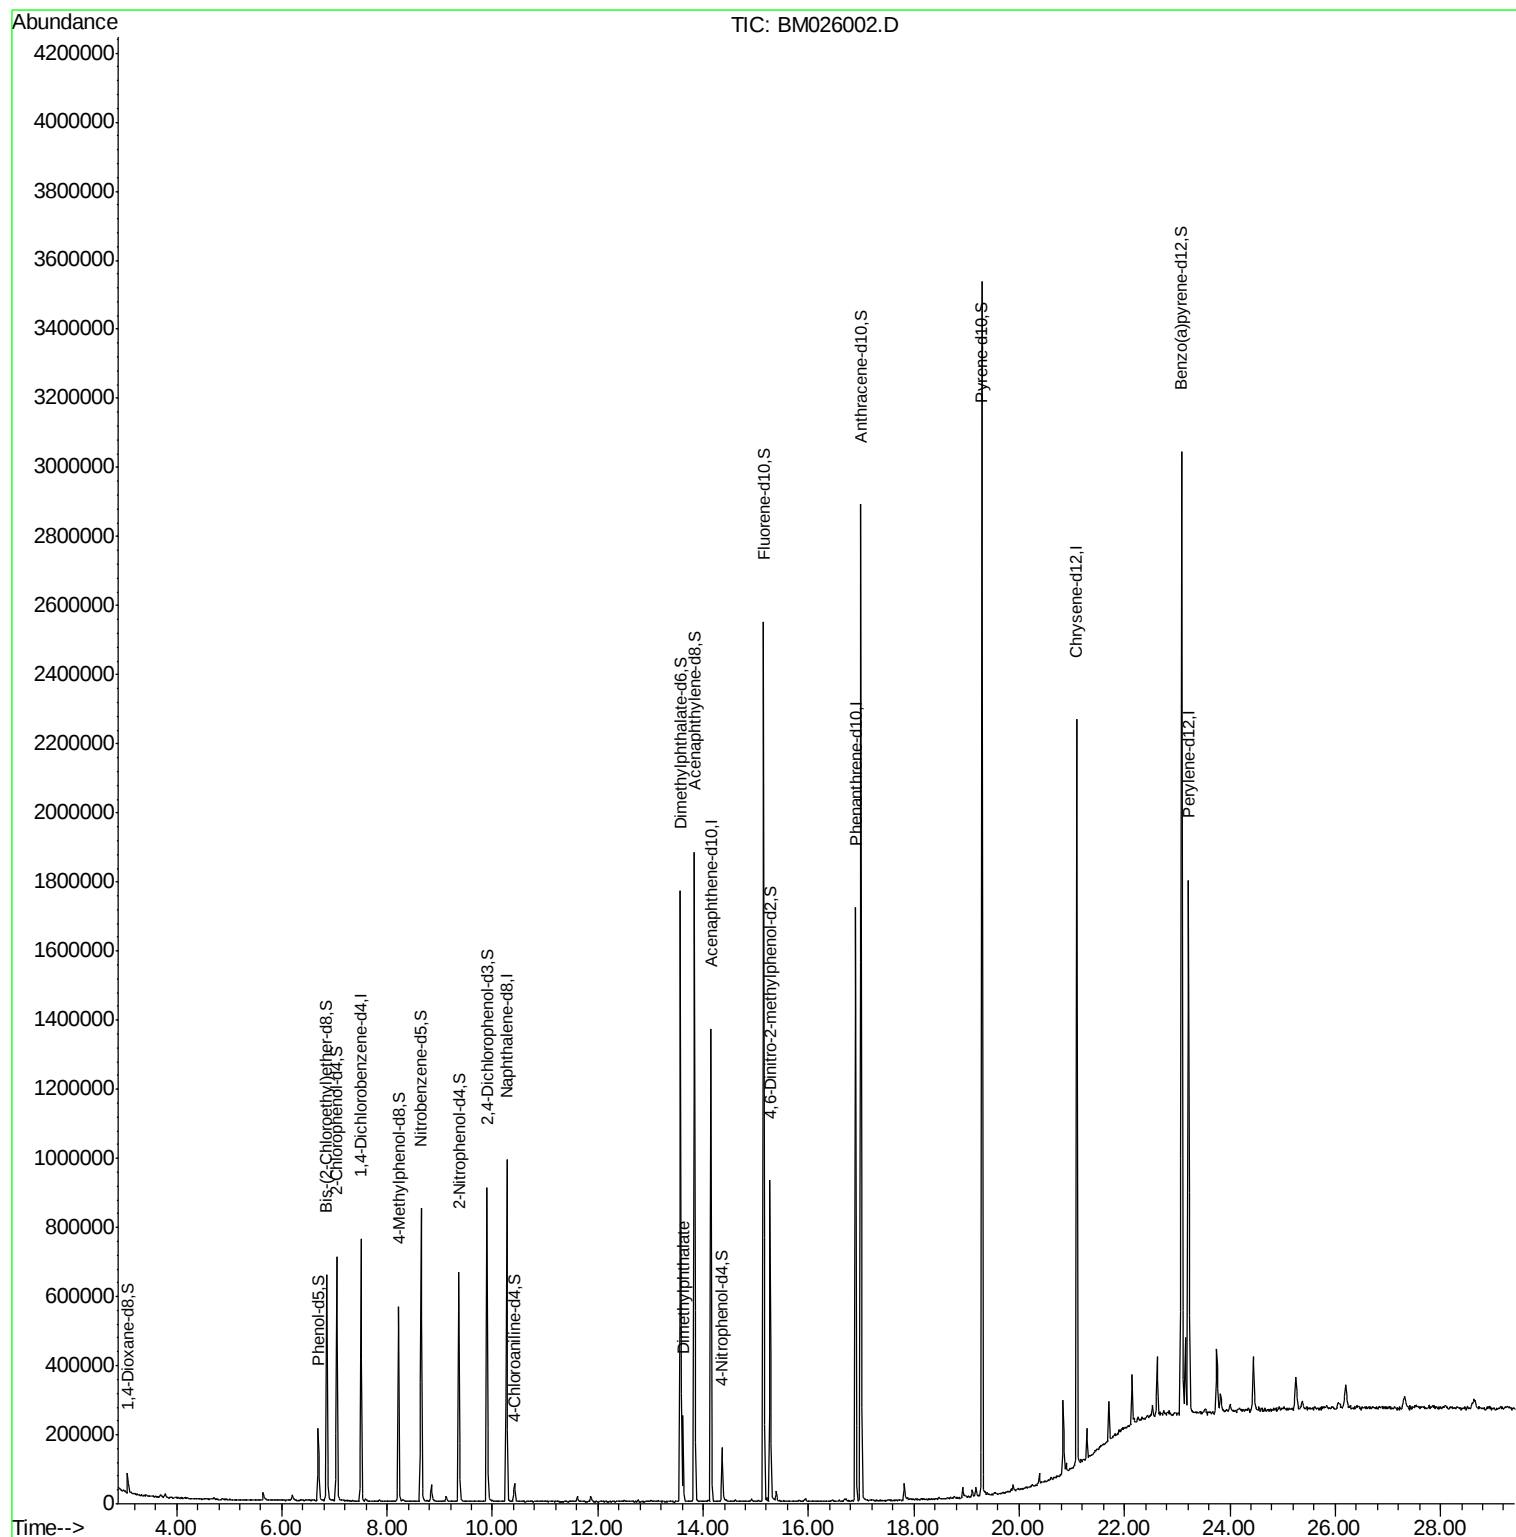

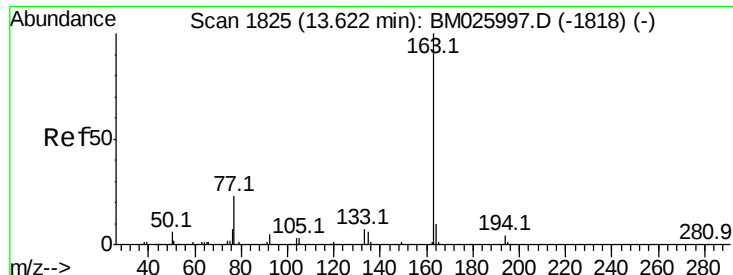

#45

Dimethylphthalate

Concen: 3.947 ng/ul

RT: 13.62 min Scan# 1824

Delta R.T. -0.00 min

Lab File: BM026002.D

Acq: 16 May 2020 01:15

Instrument :

BNA_M

ClientSampleId :

C0F20


Tot Ion:163 Resp: 136025

Ion Ratio Lower Upper

163 100

194 4.2 3.2 4.8

164 10.3 8.0 12.0

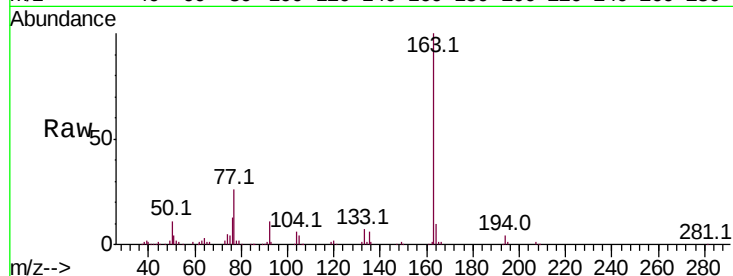

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

