

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM051520\
 Data File : BM026003.D
 Acq On : 16 May 2020 01:52
 Operator : MA/SJ
 Sample : L2655-03
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0F21

Quant Time: May 16 03:33:48 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 15 12:17:41 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.50	152	157620	20.00	ng/ul	0.00
18) Naphthalene-d8	10.27	136	645300	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.15	164	372746	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.90	188	786287	20.00	ng/ul	0.00
78) Chrysene-d12	21.09	240	808171	20.00	ng/ul	0.00
86) Perylene-d12	23.21	264	858795	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.08	96	30460	5.83	ng/uL	0.00
5) Phenol-d5	6.69	99	114030	7.97	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.85	67	402598	40.70	ng/ul	0.00
9) 2-Chlorophenol-d4	7.05	132	331815	29.65	ng/ul	0.00
13) 4-Methylphenol-d8	8.22	113	151741	14.08	ng/ul	0.00
19) Nitrobenzene-d5	8.65	128	213664	40.62	ng/ul	0.00
22) 2-Nitrophenol-d4	9.36	143	225595	43.35	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.90	165	354249	33.90	ng/ul	0.00
29) 4-Chloroaniline-d4	10.41	131	41502	3.92	ng/ul	0.00
44) Dimethylphthalate-d6	13.57	166	1295328	43.33	ng/ul	0.00
47) Acenaphthylene-d8	13.84	160	1488617	42.04	ng/ul	0.00
52) 4-Nitrophenol-d4	14.36	143	41789	7.89	ng/ul	0.00
58) Fluorene-d10	15.15	176	1154006	44.39	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.27	200	216085	47.13	ng/ul	0.00
71) Anthracene-d10	17.00	188	1762148	45.48	ng/ul	0.00
79) Pyrene-d10	19.30	212	2108328	50.79	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.09	264	2238779	48.98	ng/ul	0.00

Target Compounds


					Ovalue
20) Nitrobenzene	8.69	77	104777	6.485	ng/ul 98
37) 1,2,4,5-Tetrachlorobenzene	12.32	216	14406	1.078	ng/ul 94
45) Dimethylphthalate	13.62	163	123488	3.935	ng/ul 99
73) 1,2,3,4-Tetrachlorobenzene	12.93	216	49318	3.755	ng/uL 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM051520\
Data File : BM026003.D
Acq On : 16 May 2020 01:52
Operator : MA/SJ
Sample : L2655-03
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0F21

Quant Time: May 16 03:33:48 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri May 15 12:17:41 2020
Response via : Initial Calibration

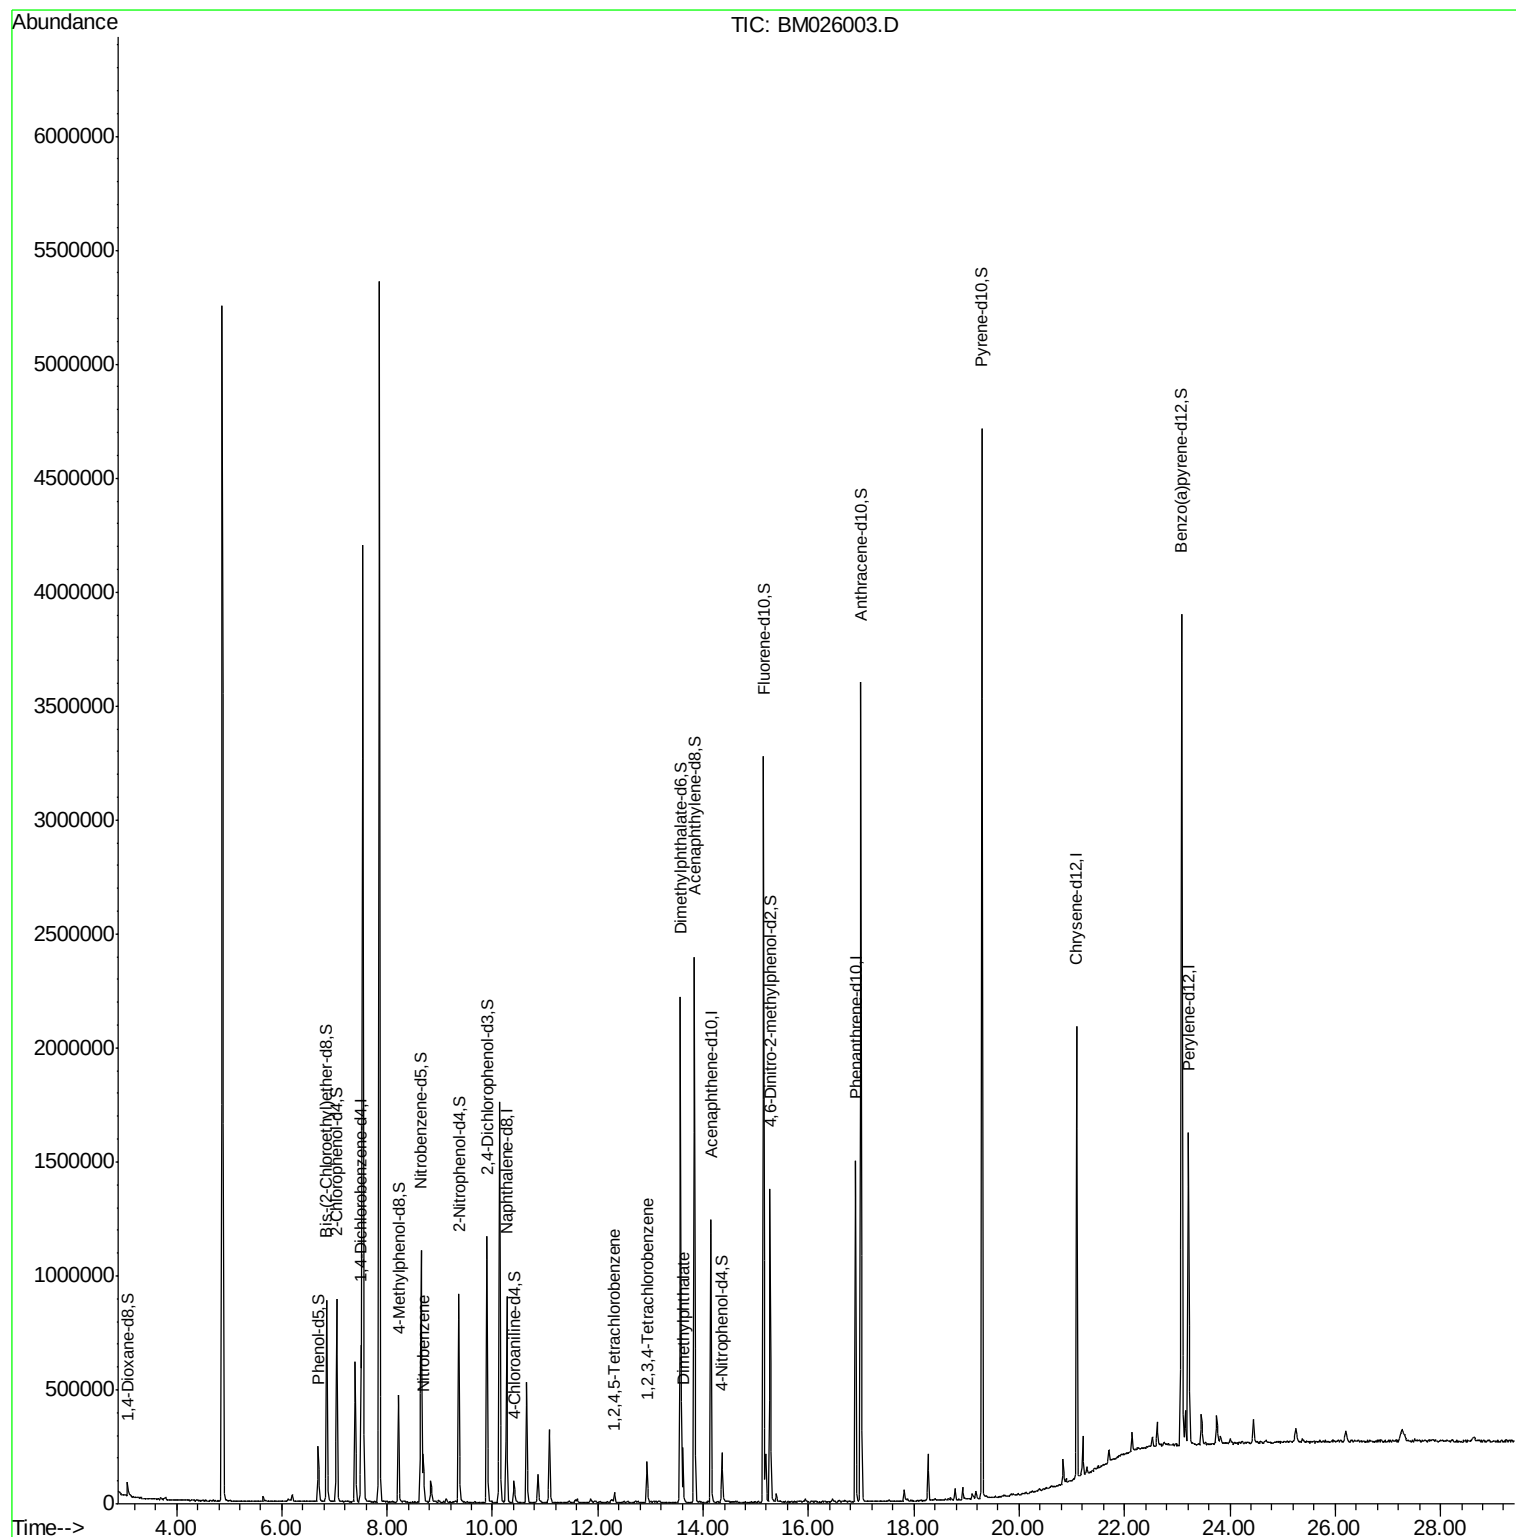

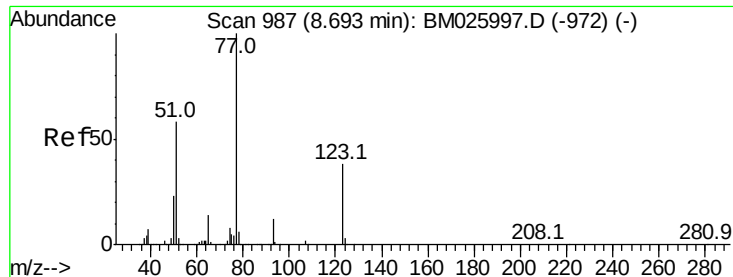

#20

Nitrobenzene

Concen: 6.485 ng/ul

RT: 8.69 min Scan# 986

Delta R.T. -0.01 min

Lab File: BM026003.D

Acq: 16 May 2020 01:52

Instrument :

BNA_M

ClientSampleId :

C0F21





Tot Ion: 77 Resp: 104777

Ion Ratio Lower Upper

77 100

123 38.7 29.5 44.3

65 13.9 11.0 16.4

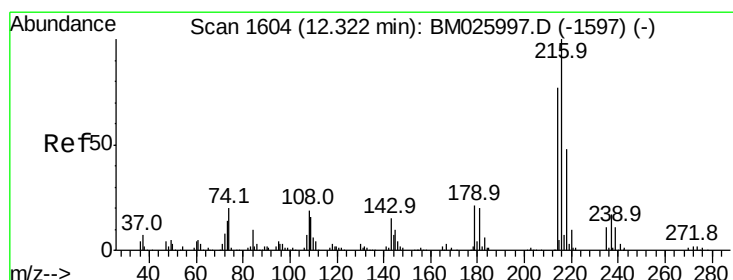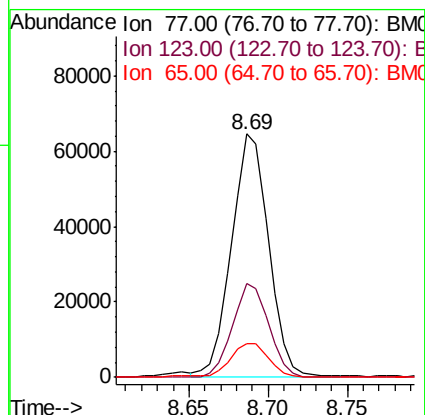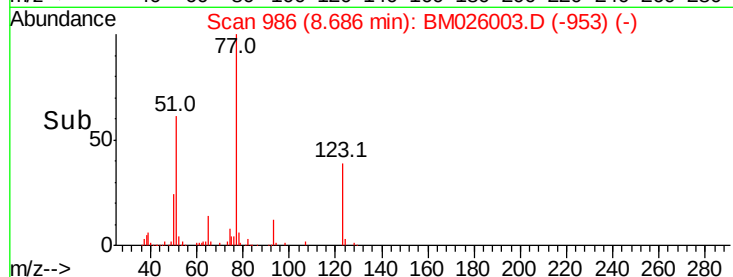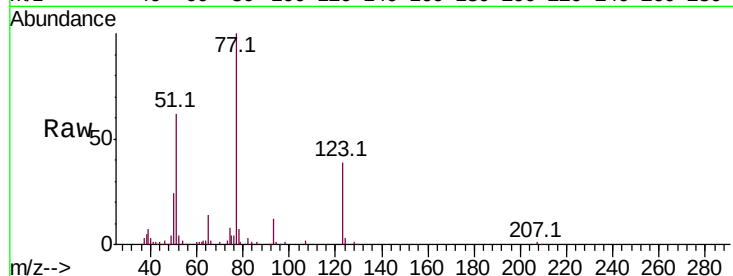

#37

1,2,4,5-Tetrachlorobenzene

Concen: 1.078 ng/ul

RT: 12.32 min Scan# 1604

Delta R.T. -0.00 min

Lab File: BM026003.D

Acq: 16 May 2020 01:52

Tgt Ion: 216 Resp: 14406




Ion Ratio Lower Upper


216 100

214 73.5 62.7 94.1

179 24.6 17.0 25.6

108 21.3 15.1 22.7


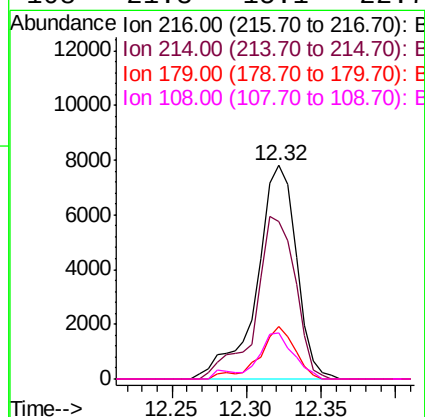
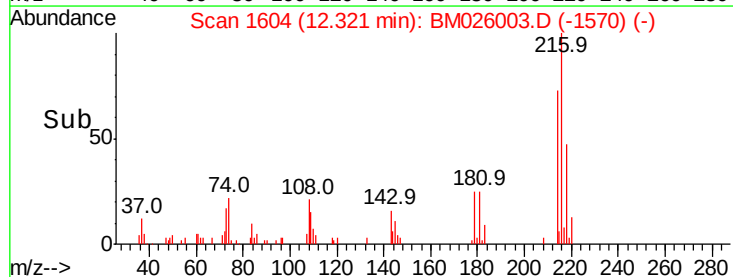
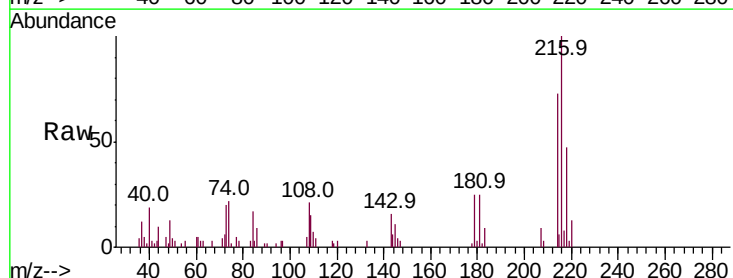


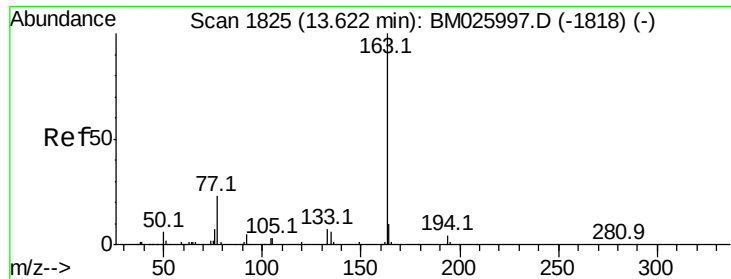

#45
 Dimethylphthalate
 Concen: 3.935 ng/uL
 RT: 13.62 min Scan# 1824
 Delta R.T. -0.00 min
 Lab File: BM026003.D
 Acq: 16 May 2020 01:52

Instrument :
 BNA_M
 ClientSampleId :
 C0F21

Tot Ion	Ratio	Lower	Upper
163	100		
194	4.7	3.2	4.8
164	9.7	8.0	12.0

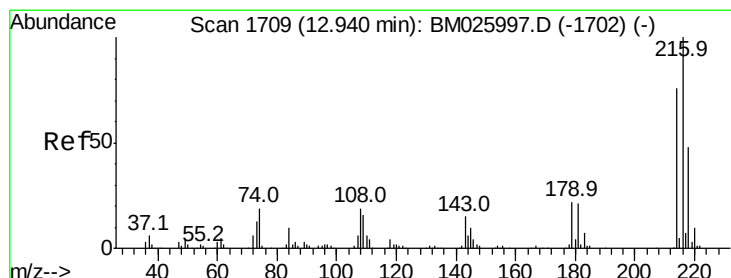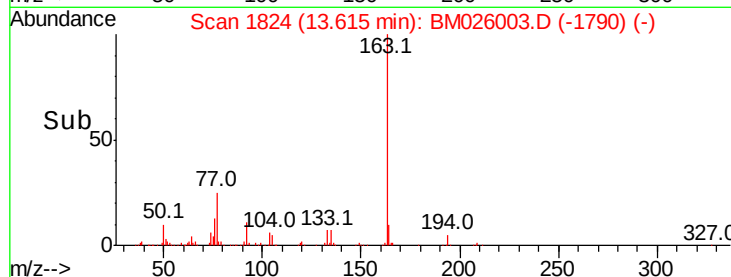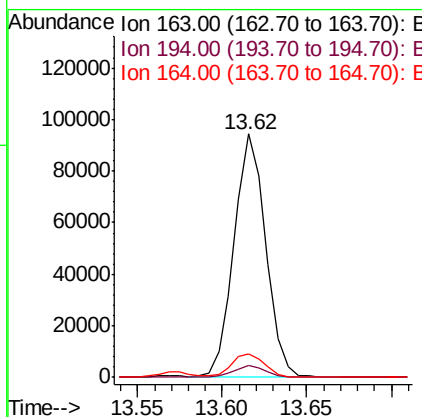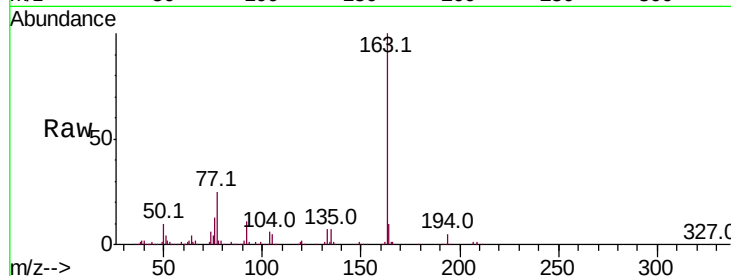

#73
 1,2,3,4-Tetrachlorobenzene
 Concen: 3.755 ng/uL
 RT: 12.93 min Scan# 1708
 Delta R.T. -0.01 min
 Lab File: BM026003.D
 Acq: 16 May 2020 01:52

Tgt Ion	Ratio	Lower	Upper
216	100		
214	76.2	61.7	92.5
218	49.2	38.4	57.6

