

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM051521\
 Data File : BM030046.D
 Acq On : 15 May 2021 13:02
 Operator : CG/JU
 Sample : M2397-04
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BG1Y5

Manual Integrations
 APPROVED

mohammad
 5/17/2021 11:21:46 AM

Quant Time: May 16 01:12:54 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat May 15 09:59:28 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.53	152	127515	20.00	ng/ul	0.00
20) Naphthalene-d8	10.30	136	503815	20.00	ng/ul	0.00
38) Acenaphthene-d10	14.18	164	286168	20.00	ng/ul	0.00
64) Phenanthrene-d10	16.93	188	542043	20.00	ng/ul	0.00
79) Chrysene-d12	21.12	240	509494	20.00	ng/ul	0.00
88) Perylene-d12	23.27	264	560523	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.06	96	4079	1.28	ng/uL	0.01
4) Pyridine-d5	0.00	84	0d	0.00	ng/ul	
7) Phenol-d5	6.73	99	53241	4.49	ng/ul	0.01
9) Bis-(2-Chloroethyl)ether-d	6.88	67	164574	22.38	ng/ul	0.00
11) 2-Chlorophenol-d4	7.07	132	185146	20.23	ng/ul	0.00
15) 4-Methylphenol-d8	8.25	113	101126	10.31	ng/ul	0.00
21) Nitrobenzene-d5	8.69	128	94004	27.08	ng/ul	0.00
24) 2-Nitrophenol-d4	9.40	143	106748	27.24	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	9.95	165	163328	20.79	ng/ul	0.01
31) 4-Chloroaniline-d4	10.54	131	6475m	0.54	ng/ul	0.09
46) Dimethylphthalate-d6	13.60	166	592442	26.71	ng/ul	0.00
49) Acenaphthylene-d8	13.87	160	743723	26.46	ng/ul	0.00
54) 4-Nitrophenol-d4	14.49	143	8320m	2.30	ng/ul	0.08
60) Fluorene-d10	15.18	176	519288	27.58	ng/ul	0.00
65) 4,6-Dinitro-2-methylphenol	15.32	200	77527	22.02	ng/ul	0.00
73) Anthracene-d10	17.03	188	820269	30.05	ng/ul	0.00
81) Pyrene-d10	19.33	212	904607	34.61	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.13	264	956584	30.11	ng/ul	0.00
Target Compounds						
47) Dimethylphthalate	13.65	163	34396	1.549	ng/ul	Ovalue 99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM051521\
Data File : BM030046.D
Acq On : 15 May 2021 13:02
Operator : CG/JU
Sample : M2397-04
Misc :
ALS Vial : 7 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
BG1Y5

Manual Integrations
APPROVED

mohammad
5/17/2021 11:21:46 AM

Quant Time: May 16 01:12:54 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat May 15 09:59:28 2021
Response via : Initial Calibration

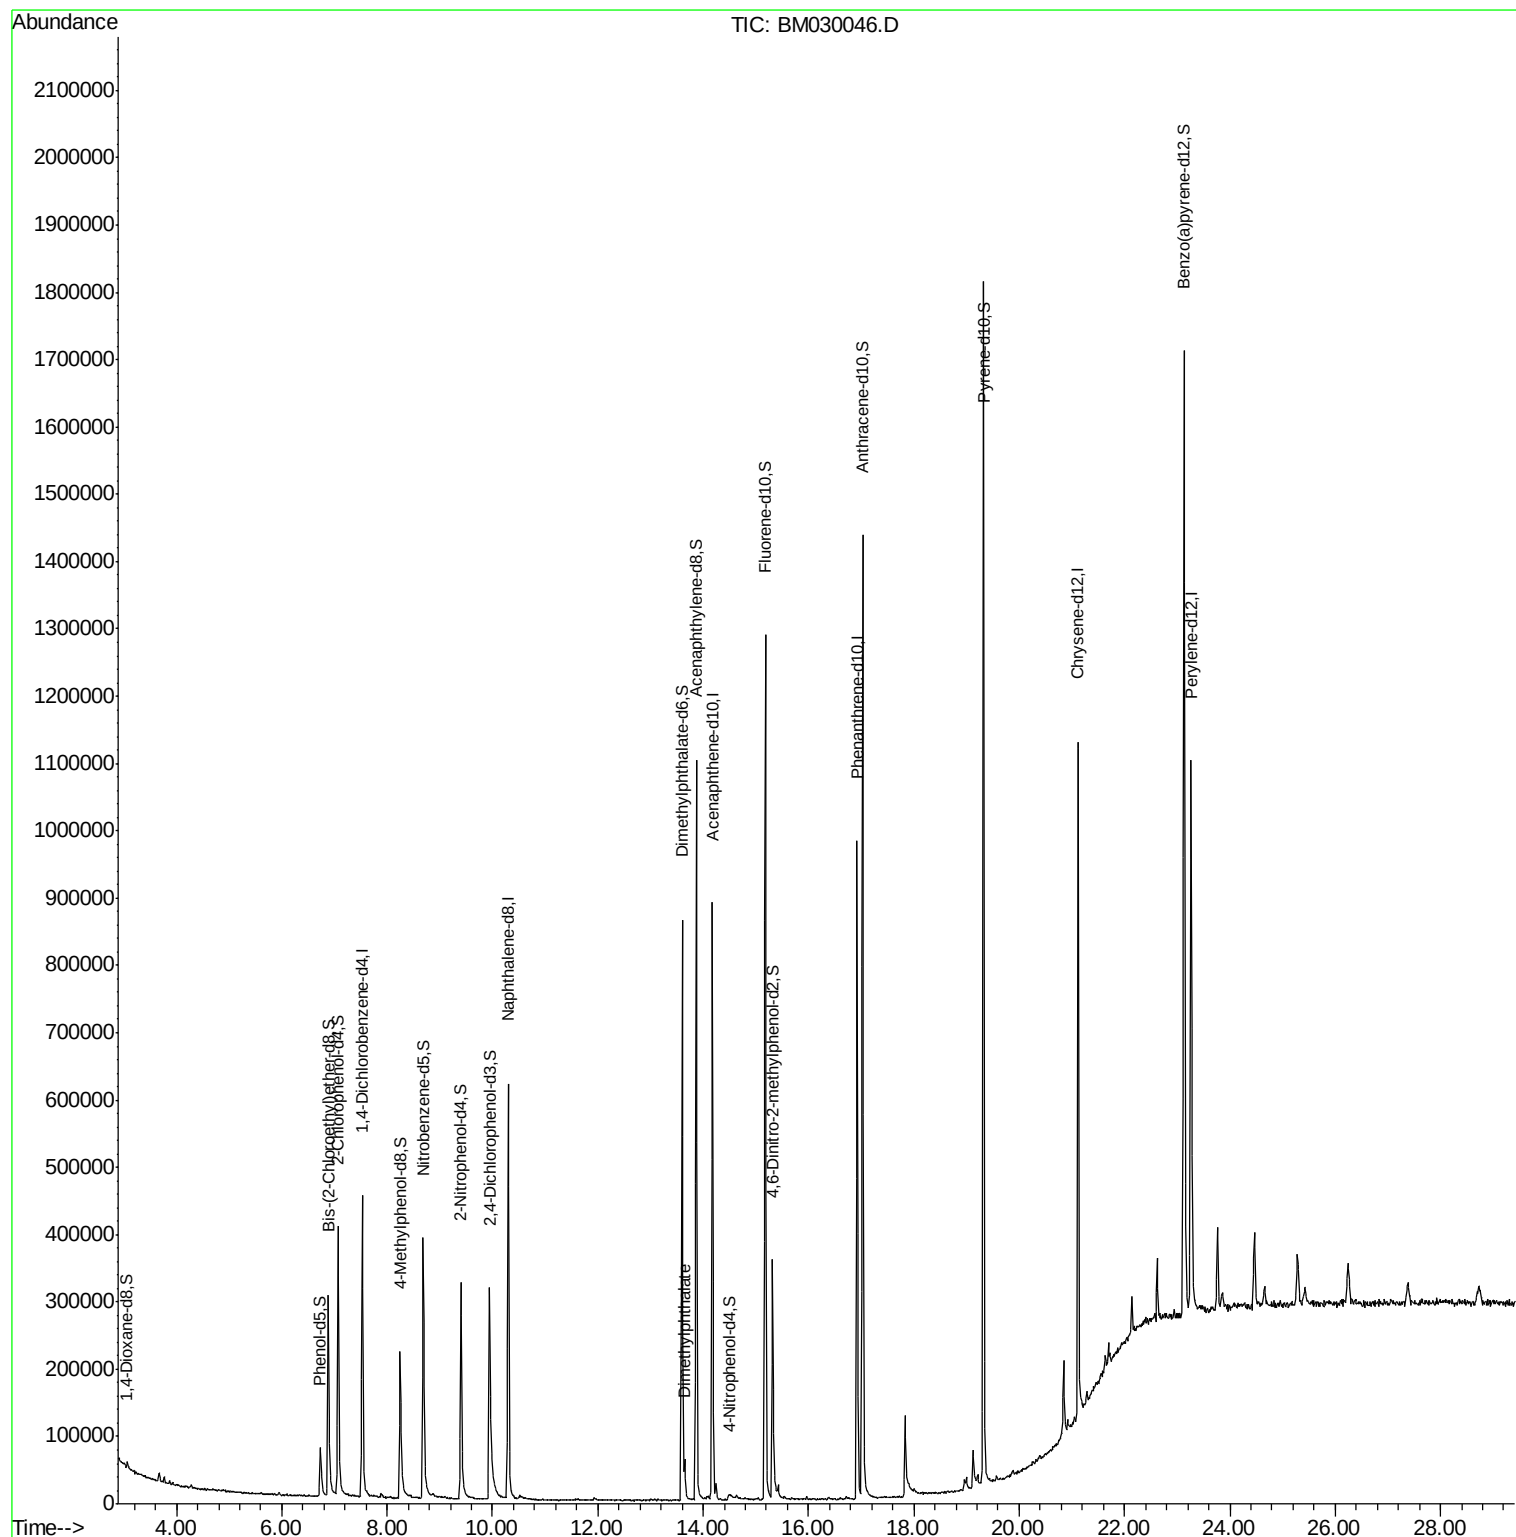

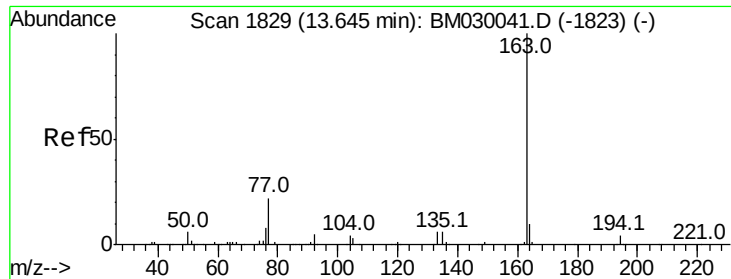

#47
 Dimethylphthalate
 Concen: 1.549 ng/ul
 RT: 13.65 min Scan# 1830
 Delta R.T. 0.01 min
 Lab File: BM030046.D
 Acq: 15 May 2021 13:02

Instrument :
 BNA_M
 ClientSampleId :
 BG1Y5

Tot Ion	Ratio	Resp Lower	Upper
163	100		
194	4.2	3.4	5.0
164	10.3	7.8	11.8

Manual Integrations
 APPROVED

mohammad
 5/17/2021 11:21:46 AM

