

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM051521\
 Data File : BM030050.D
 Acq On : 15 May 2021 15:27
 Operator : CG/JU
 Sample : M2397-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BG1Y6

Manual Integrations
 APPROVED

mohammad
 5/17/2021 11:21:58 AM

Quant Time: May 16 01:37:35 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat May 15 09:59:28 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.53	152	140590	20.00	ng/ul	0.00
20) Naphthalene-d8	10.30	136	617090	20.00	ng/ul	0.00
38) Acenaphthene-d10	14.18	164	394281	20.00	ng/ul	0.00
64) Phenanthrene-d10	16.93	188	782668	20.00	ng/ul	0.00
79) Chrysene-d12	21.12	240	692374	20.00	ng/ul	0.00
88) Perylene-d12	23.26	264	654619	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.06	96	3669m	1.04	ng/uL	0.01
4) Pyridine-d5	0.00	84	0d	0.00	ng/ul	
7) Phenol-d5	6.73	99	51919	3.97	ng/ul	0.01
9) Bis-(2-Chloroethyl)ether-d	6.88	67	186262	22.97	ng/ul	0.00
11) 2-Chlorophenol-d4	7.07	132	192963	19.12	ng/ul	0.00
15) 4-Methylphenol-d8	8.25	113	106250	9.83	ng/ul	0.00
21) Nitrobenzene-d5	8.69	128	111689	26.26	ng/ul	0.00
24) 2-Nitrophenol-d4	9.40	143	122439	25.51	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	9.95	165	179438	18.64	ng/ul	0.01
31) 4-Chloroaniline-d4	10.52	131	10085m	0.69	ng/ul	0.06
46) Dimethylphthalate-d6	13.60	166	757897	24.80	ng/ul	0.00
49) Acenaphthylene-d8	13.87	160	953944	24.63	ng/ul	0.00
54) 4-Nitrophenol-d4	14.47	143	9899m	1.99	ng/ul	0.06
60) Fluorene-d10	15.17	176	691579	26.66	ng/ul	0.00
65) 4,6-Dinitro-2-methylphenol	15.32	200	117289	23.07	ng/ul	0.00
73) Anthracene-d10	17.03	188	1098703	27.88	ng/ul	0.00
81) Pyrene-d10	19.32	212	1220742	34.37	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.13	264	1050048	28.30	ng/ul	0.00
Target Compounds						
47) Dimethylphthalate	13.65	163	37600	1.229	ng/ul	Ovalue 99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM051521\
Data File : BM030050.D
Acq On : 15 May 2021 15:27
Operator : CG/JU
Sample : M2397-01
Misc :
ALS Vial : 5 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
BG1Y6

Quant Time: May 16 01:37:35 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat May 15 09:59:28 2021
Response via : Initial Calibration

Manual Integrations
APPROVED

mohammad
5/17/2021 11:21:58 AM

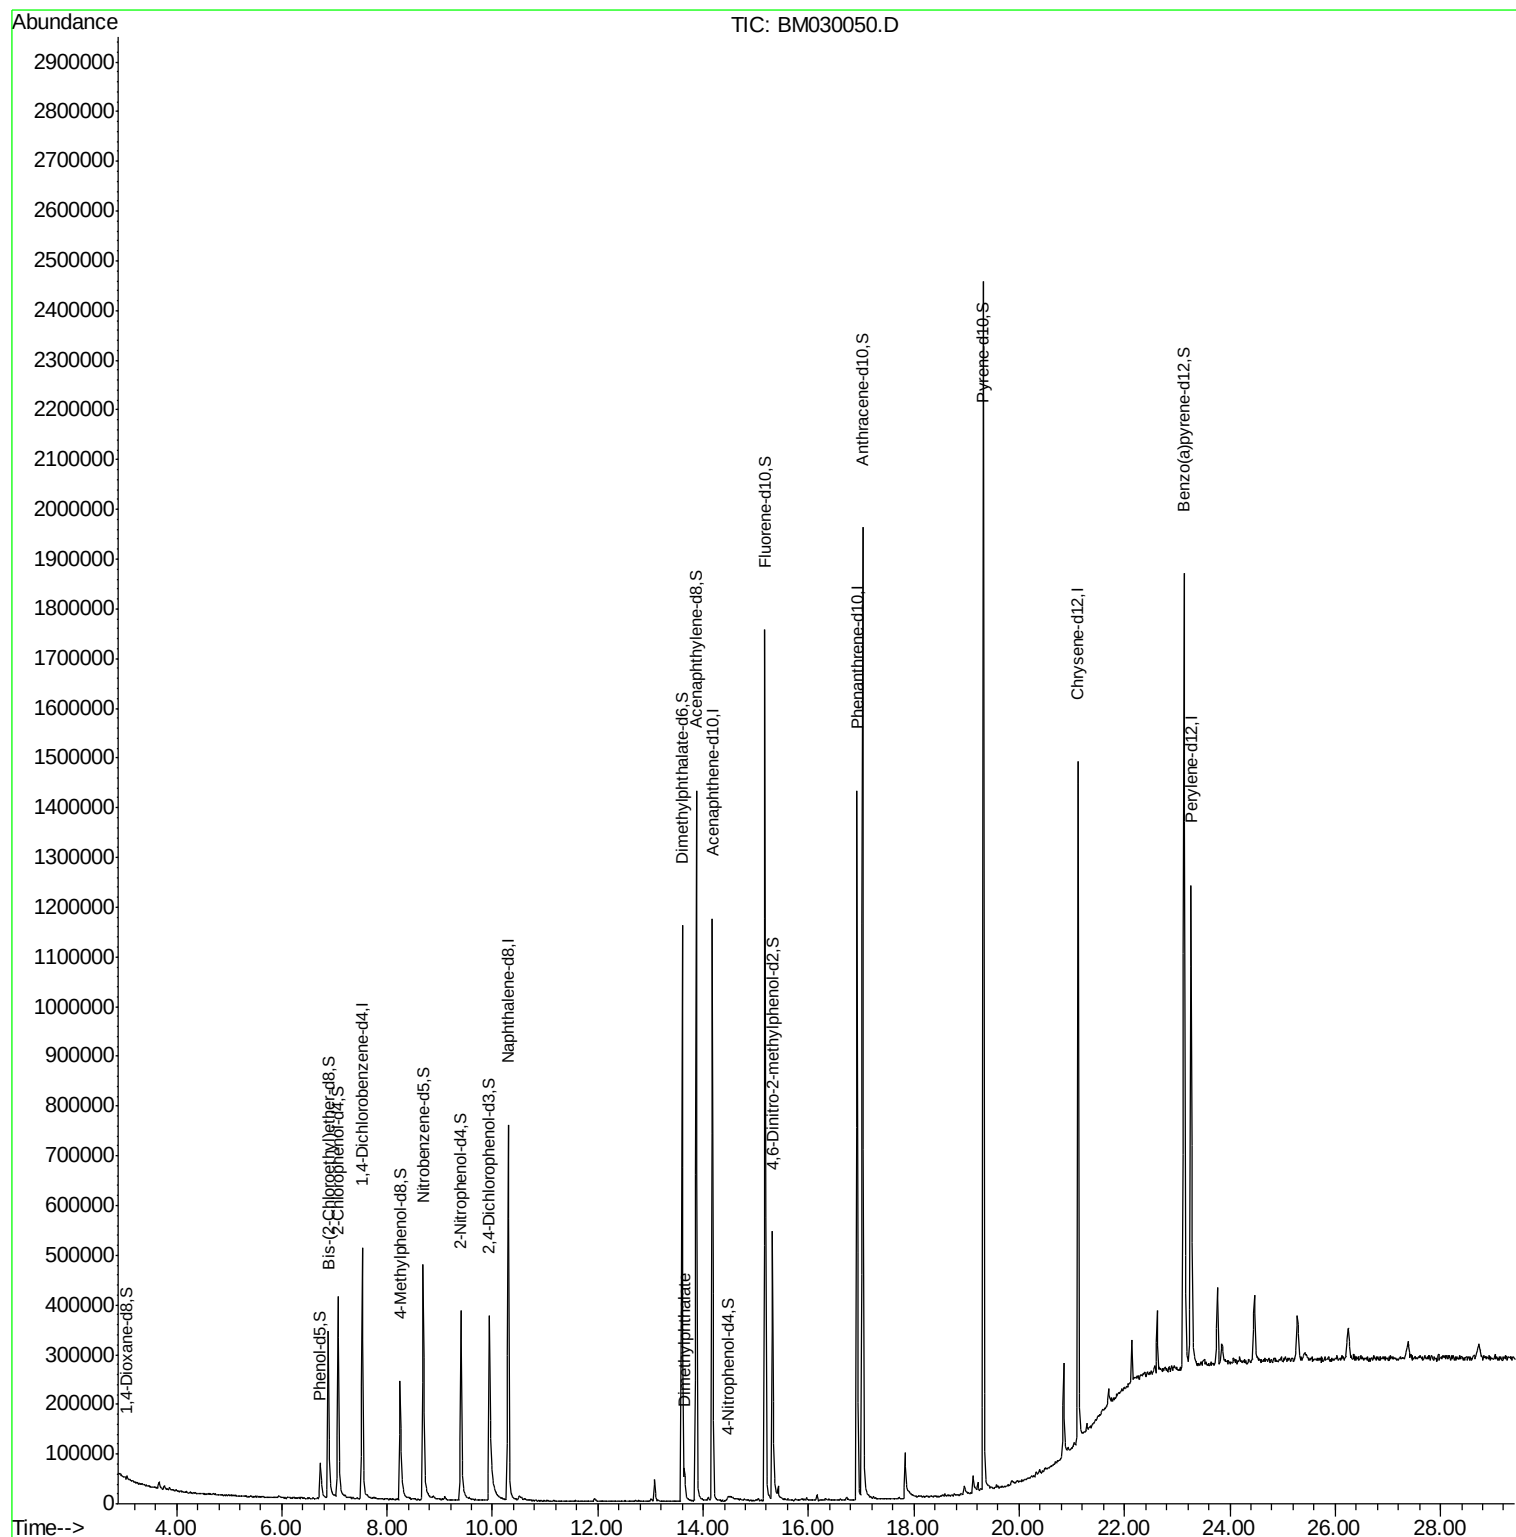

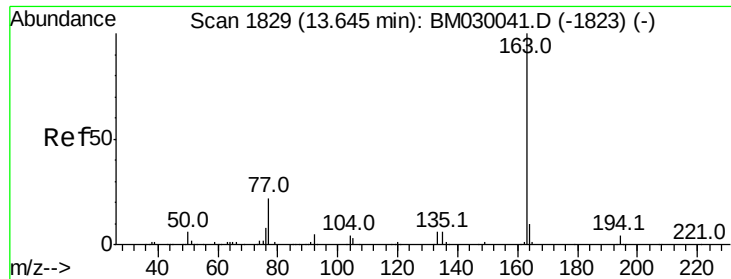


#47
 Dimethylphthalate
 Concen: 1.229 ng/ul
 RT: 13.65 min Scan# 1830
 Delta R.T. 0.01 min
 Lab File: BM030050.D
 Acq: 15 May 2021 15:27

Instrument :
 BNA_M
 ClientSampleId :
 BG1Y6

Tot Ion	Ratio	Resp Lower	Upper
163	100		
194	4.6	3.4	5.0
164	9.9	7.8	11.8

Manual Integrations
 APPROVED

mohammad
 5/17/2021 11:21:58 AM

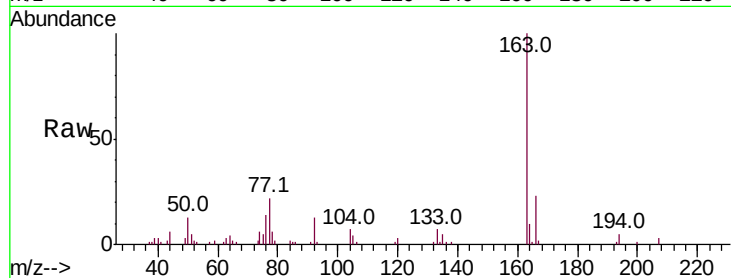

Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

