


Data Path : Z:\HPCHEM1\BNA M\Data\BM051615\
 Data File : BM001293.D
 Acq On : 14 May 2015 14:50
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\SIM-BM040315.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Apr 03 18:16:53 2015

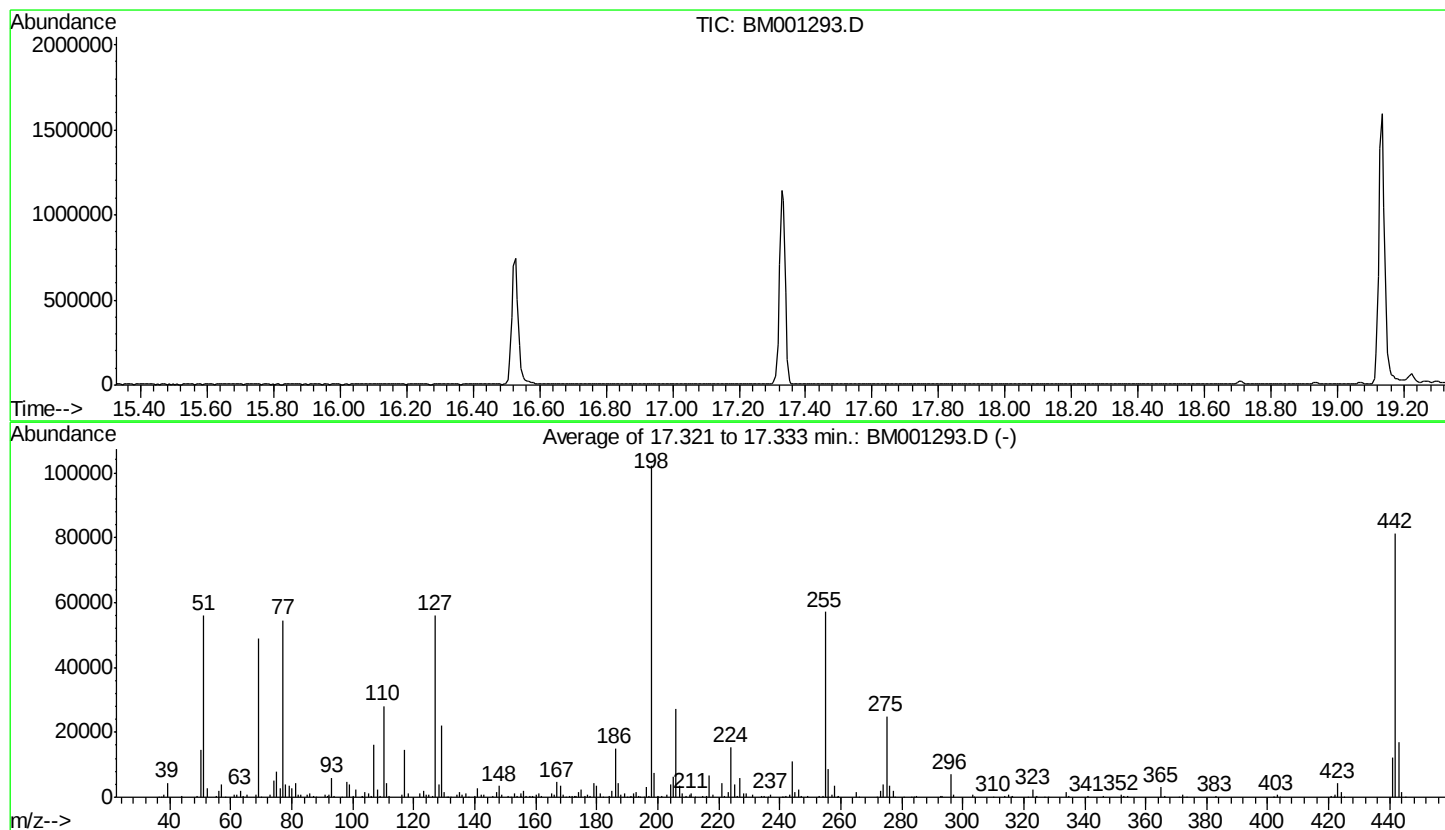

AutoFind: Scans 2488, 2489, 2490; Background Corrected with Scan 2482

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	54.8	55989	PASS
68	69	0.00	2	1.8	858	PASS
69	198	0.00	100	47.9	49002	PASS
70	69	0.00	2	0.2	109	PASS
127	198	10	80	54.8	55992	PASS
197	198	0.00	2	0.6	578	PASS
198	198	100	100	100.0	102210	PASS
199	198	5	9	7.3	7437	PASS
275	198	10	60	24.3	24840	PASS
365	198	1	100	3.0	3028	PASS
441	442	0.01	24	15.2	12321	PASS
442	198	50	100	79.4	81154	PASS
443	442	15	24	20.9	16947	PASS