


Data Path : Z:\HPCHEM1\BNA_M\Data\BM051617\
 Data File : BM010053.D
 Acq On : 16 May 2017 14:23
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM051117.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu May 11 19:50:16 2017

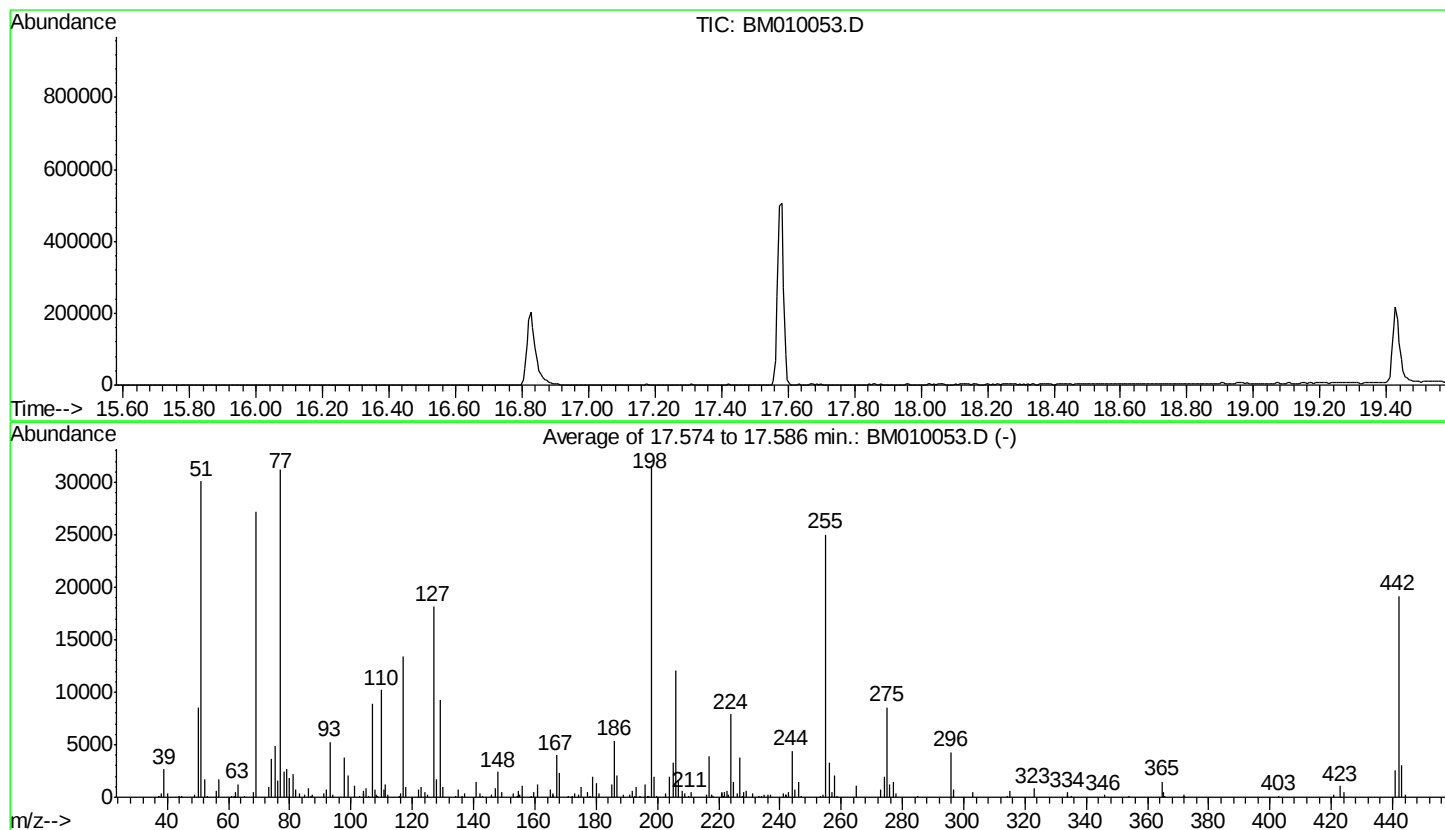

AutoFind: Scans 2463, 2464, 2465; Background Corrected with Scan 2457

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	95.2	30069	FAIL*
68	69	0.00	2	1.9	514	PASS
69	198	0.00	100	86.0	27174	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	57.4	18124	PASS
197	198	0.00	2	0.4	124	PASS
198	198	100	100	100.0	31592	PASS
199	198	5	9	6.1	1916	PASS
275	198	10	60	27.0	8540	PASS
365	198	1	100	4.8	1506	PASS
441	442	0.01	24	13.3	2558	PASS
442	198	50	100	60.8	19200	PASS
443	442	15	24	15.9	3052	PASS