


Data Path : Z:\HPCHEM1\BNA_M\Data\BM051617\
 Data File : BM010054.D
 Acq On : 16 May 2017 15:28
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM051117.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu May 11 19:50:16 2017

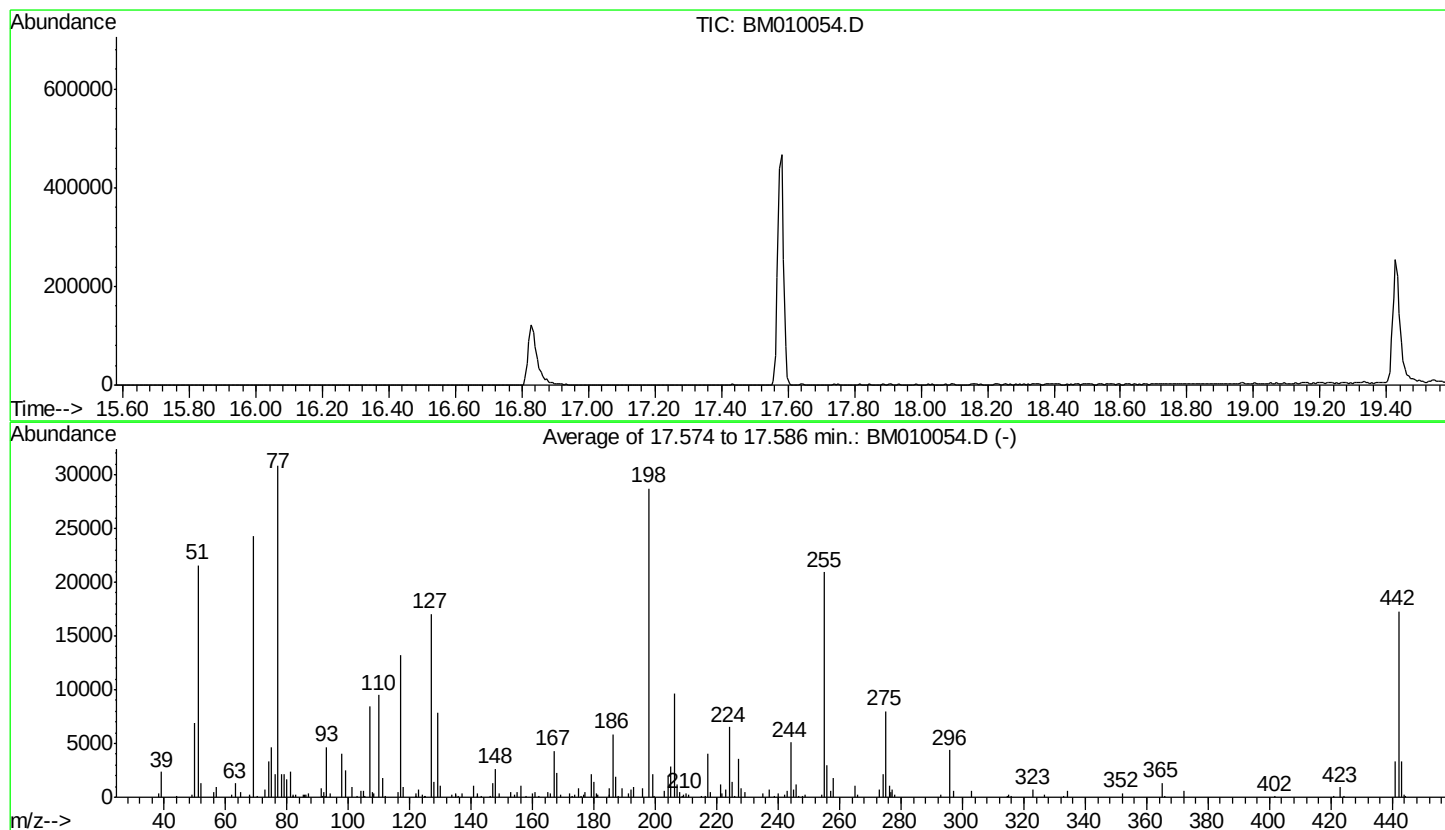

AutoFind: Scans 2463, 2464, 2465; Background Corrected with Scan 2457

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	75.1	21570	PASS
68	69	0.00	2	0.8	193	PASS
69	198	0.00	100	84.4	24240	PASS
70	69	0.00	2	0.5	113	PASS
127	198	10	80	59.5	17077	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	28706	PASS
199	198	5	9	7.3	2089	PASS
275	198	10	60	27.9	8009	PASS
365	198	1	100	4.8	1365	PASS
441	442	0.01	24	19.1	3306	PASS
442	198	50	100	60.2	17283	PASS
443	442	15	24	19.1	3308	PASS