

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM051622\
 Data File : BM035097.D
 Acq On : 16 May 2022 10:50
 Operator : CG/JU
 Sample : PB144680BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK680

Quant Time: May 17 00:50:45 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM051222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu May 12 18:15:39 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.917	152	3774	0.400	ng/ul	0.00
4) Naphthalene-d8	10.715	136	11880	0.400	ng/ul #	0.00
9) Acenaphthene-d10	14.552	164	7852	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.292	188	16043	0.400	ng/ul #	0.00
17) Chrysene-d12	21.476	240	10796	0.400	ng/ul	0.00
23) Perylene-d12	23.864	264	9612	0.400	ng/ul #	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.356	96	25860	5.720	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.305	152	6113	0.322	ng/ul	0.00
18) Fluoranthene-d10	19.322	212	12741	0.344	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.542	166	2392	0.061	ng/ul#	16
20) Pyrene	19.684	202	2205	0.036	ng/ul#	1
26) Benzo(a)pyrene	23.712	252	3261	0.071	ng/ul#	71


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM051622\
Data File : BM035097.D
Acq On : 16 May 2022 10:50
Operator : CG/JU
Sample : PB144680BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK680

Quant Time: May 17 00:50:45 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM051222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 12 18:15:39 2022
Response via : Initial Calibration




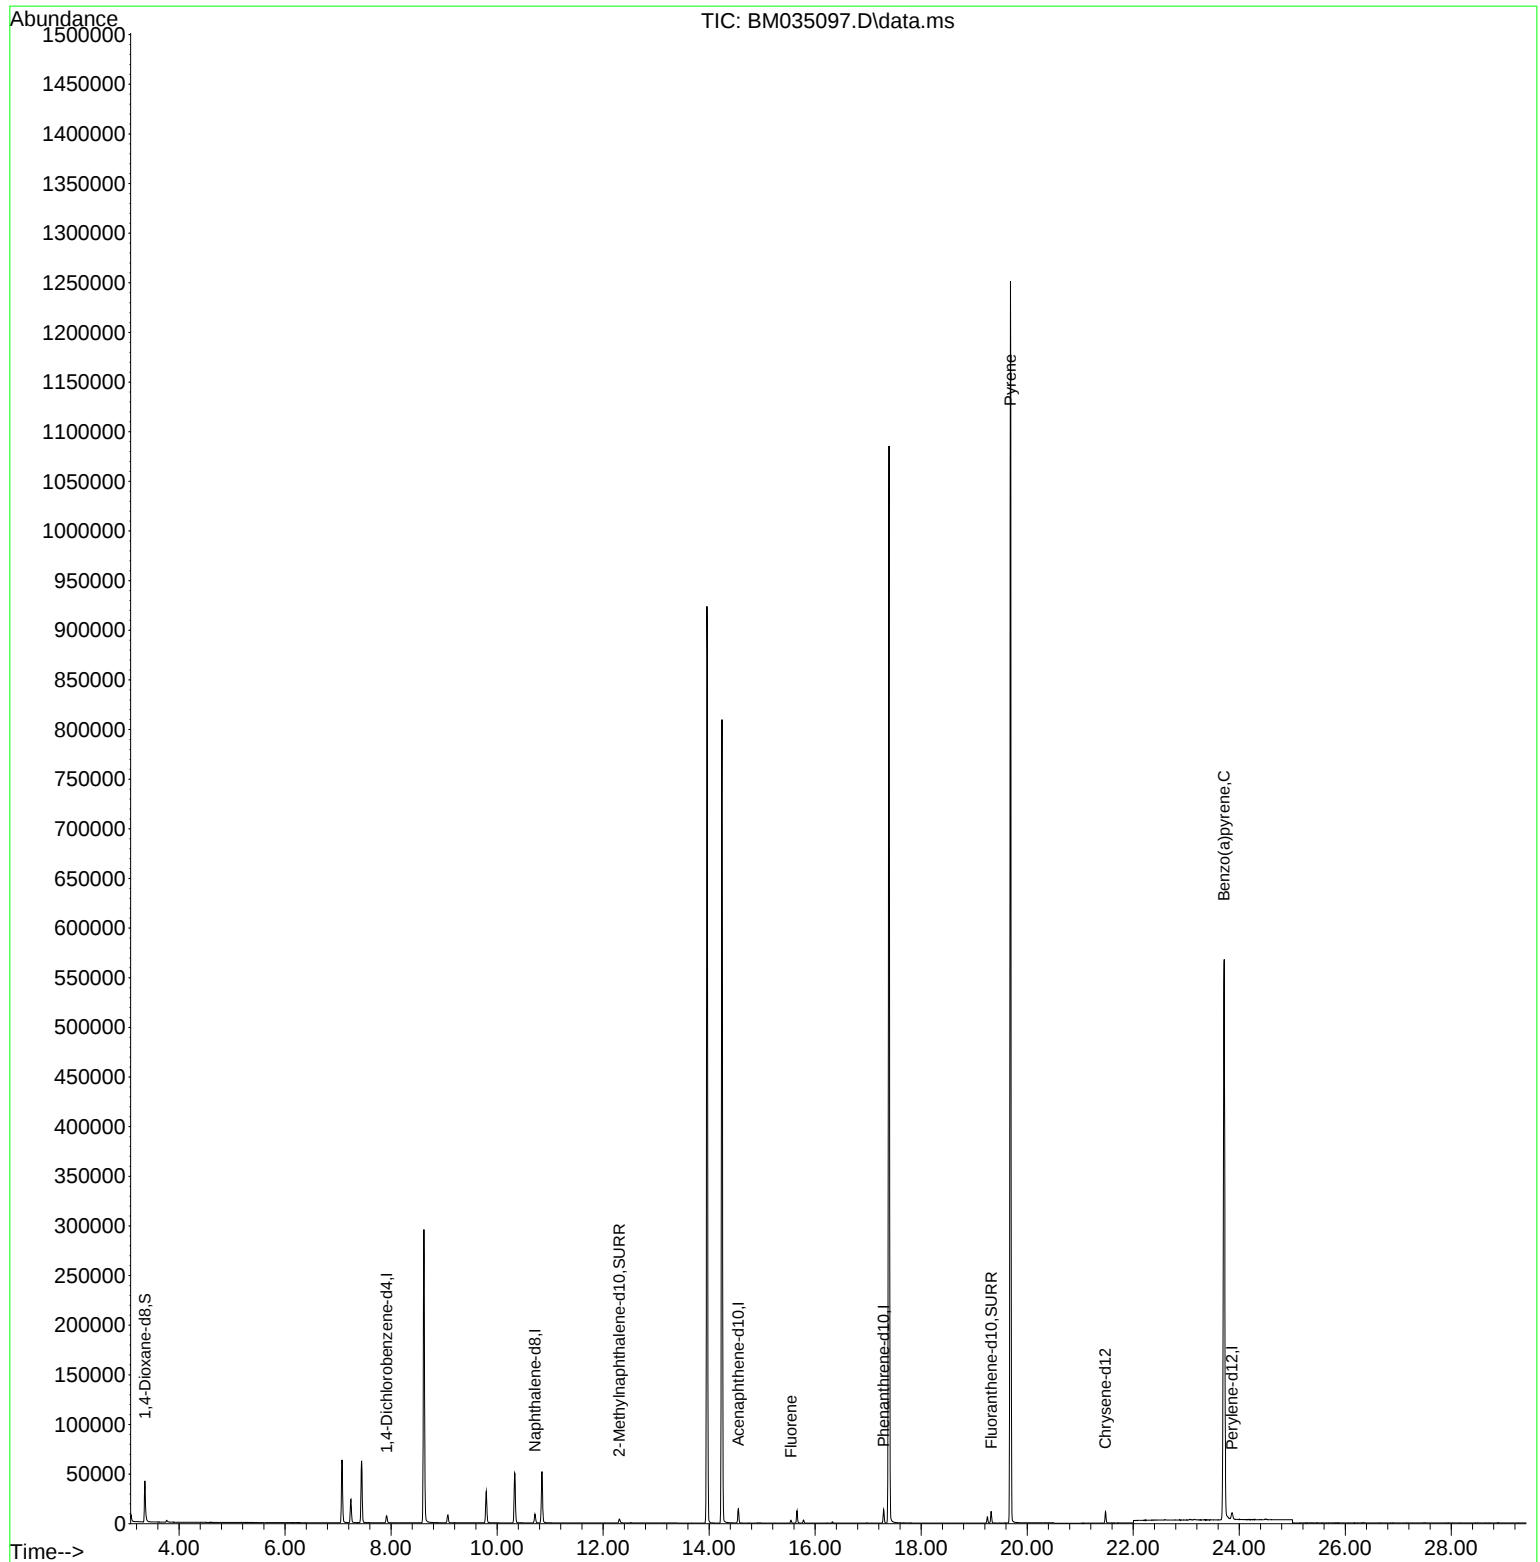


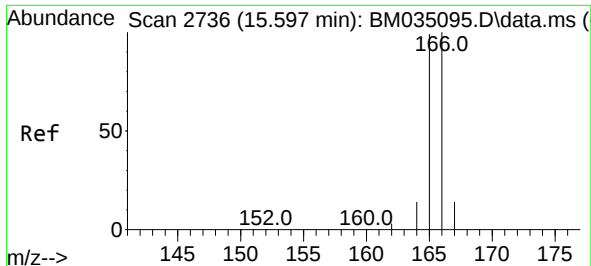

#12
Fluorene
Concen: 0.061 ng/ul
RT: 15.542 min Scan# 21
Delta R.T. -0.060 min
Lab File: BM035097.D
Acq: 16 May 2022 10:50




Instrument :
BNA_M
ClientSampleId :
SBLK680


Tgt Ion:166 Resp: 2392
Ion Ratio Lower Upper
166 100
165 7.5 81.1 121.7#
167 32.5 14.9 22.3#

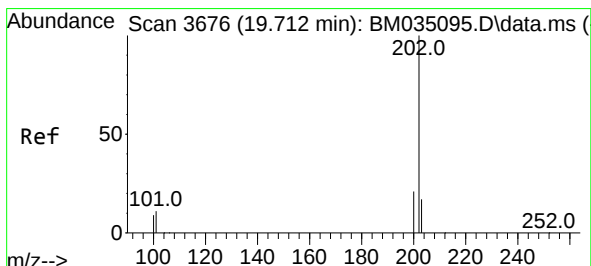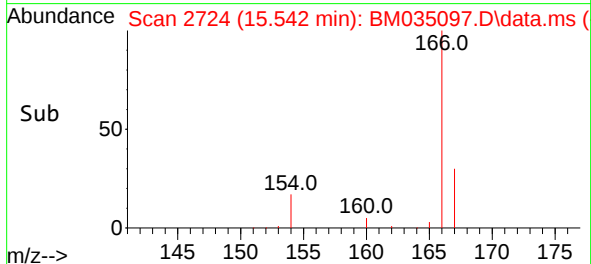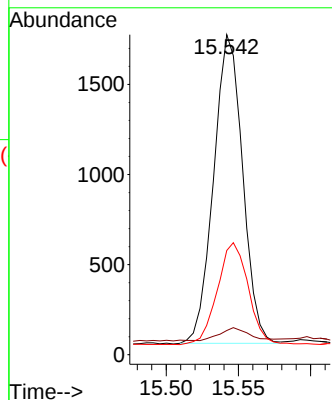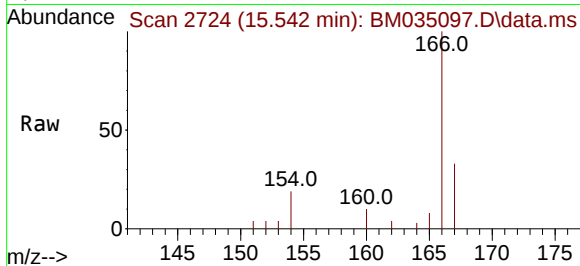

#20
Pyrene
Concen: 0.036 ng/ul
RT: 19.684 min Scan# 3670
Delta R.T. -0.028 min
Lab File: BM035097.D
Acq: 16 May 2022 10:50


Tgt Ion:202 Resp: 2205
Ion Ratio Lower Upper
202 100
101 170.4 9.3 13.9#
100 1329.8 7.8 11.6#

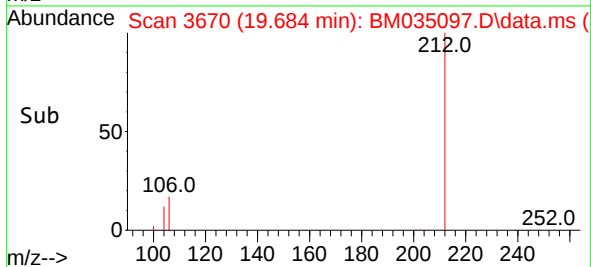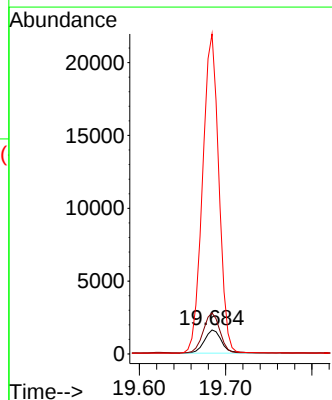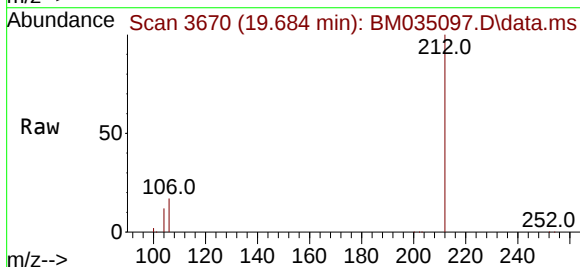

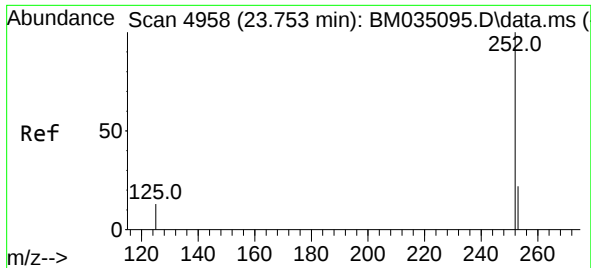

#26
Benzo(a)pyrene
Concen: 0.071 ng/ul
RT: 23.712 min Scan# 4944
Delta R.T. -0.038 min
Lab File: BM035097.D
Acq: 16 May 2022 10:50

Instrument :
BNA_M
ClientSampleId :
SBLK680

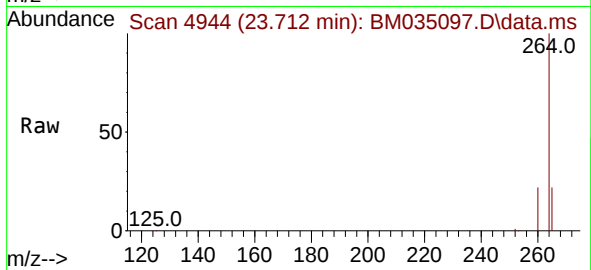

Tgt Ion:252 Resp: 3261
Ion Ratio Lower Upper
252 100
253 49.5 32.0 48.0#
125 44.9 14.5 21.7#

