

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM051622\
 Data File : BM035101.D
 Acq On : 16 May 2022 13:16
 Operator : CG/JU
 Sample : N2707-13
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EXLA4

Quant Time: May 17 00:51:02 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM051222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu May 12 18:15:39 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.918	152	4043	0.400	ng/ul	0.00
4) Naphthalene-d8	10.716	136	12919	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.548	164	8666	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.292	188	18676	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.477	240	13747	0.400	ng/ul	0.00
23) Perylene-d12	23.865	264	11818	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.357	96	19717	4.071	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.305	152	6522	0.316	ng/ul	0.00
18) Fluoranthene-d10	19.322	212	18155	0.385	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.689	202	3336	0.043	ng/ul#	1
26) Benzo(a)pyrene	23.716	252	5095	0.090	ng/ul#	78


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM051622\
Data File : BM035101.D
Acq On : 16 May 2022 13:16
Operator : CG/JU
Sample : N2707-13
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EXLA4

Quant Time: May 17 00:51:02 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM051222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 12 18:15:39 2022
Response via : Initial Calibration

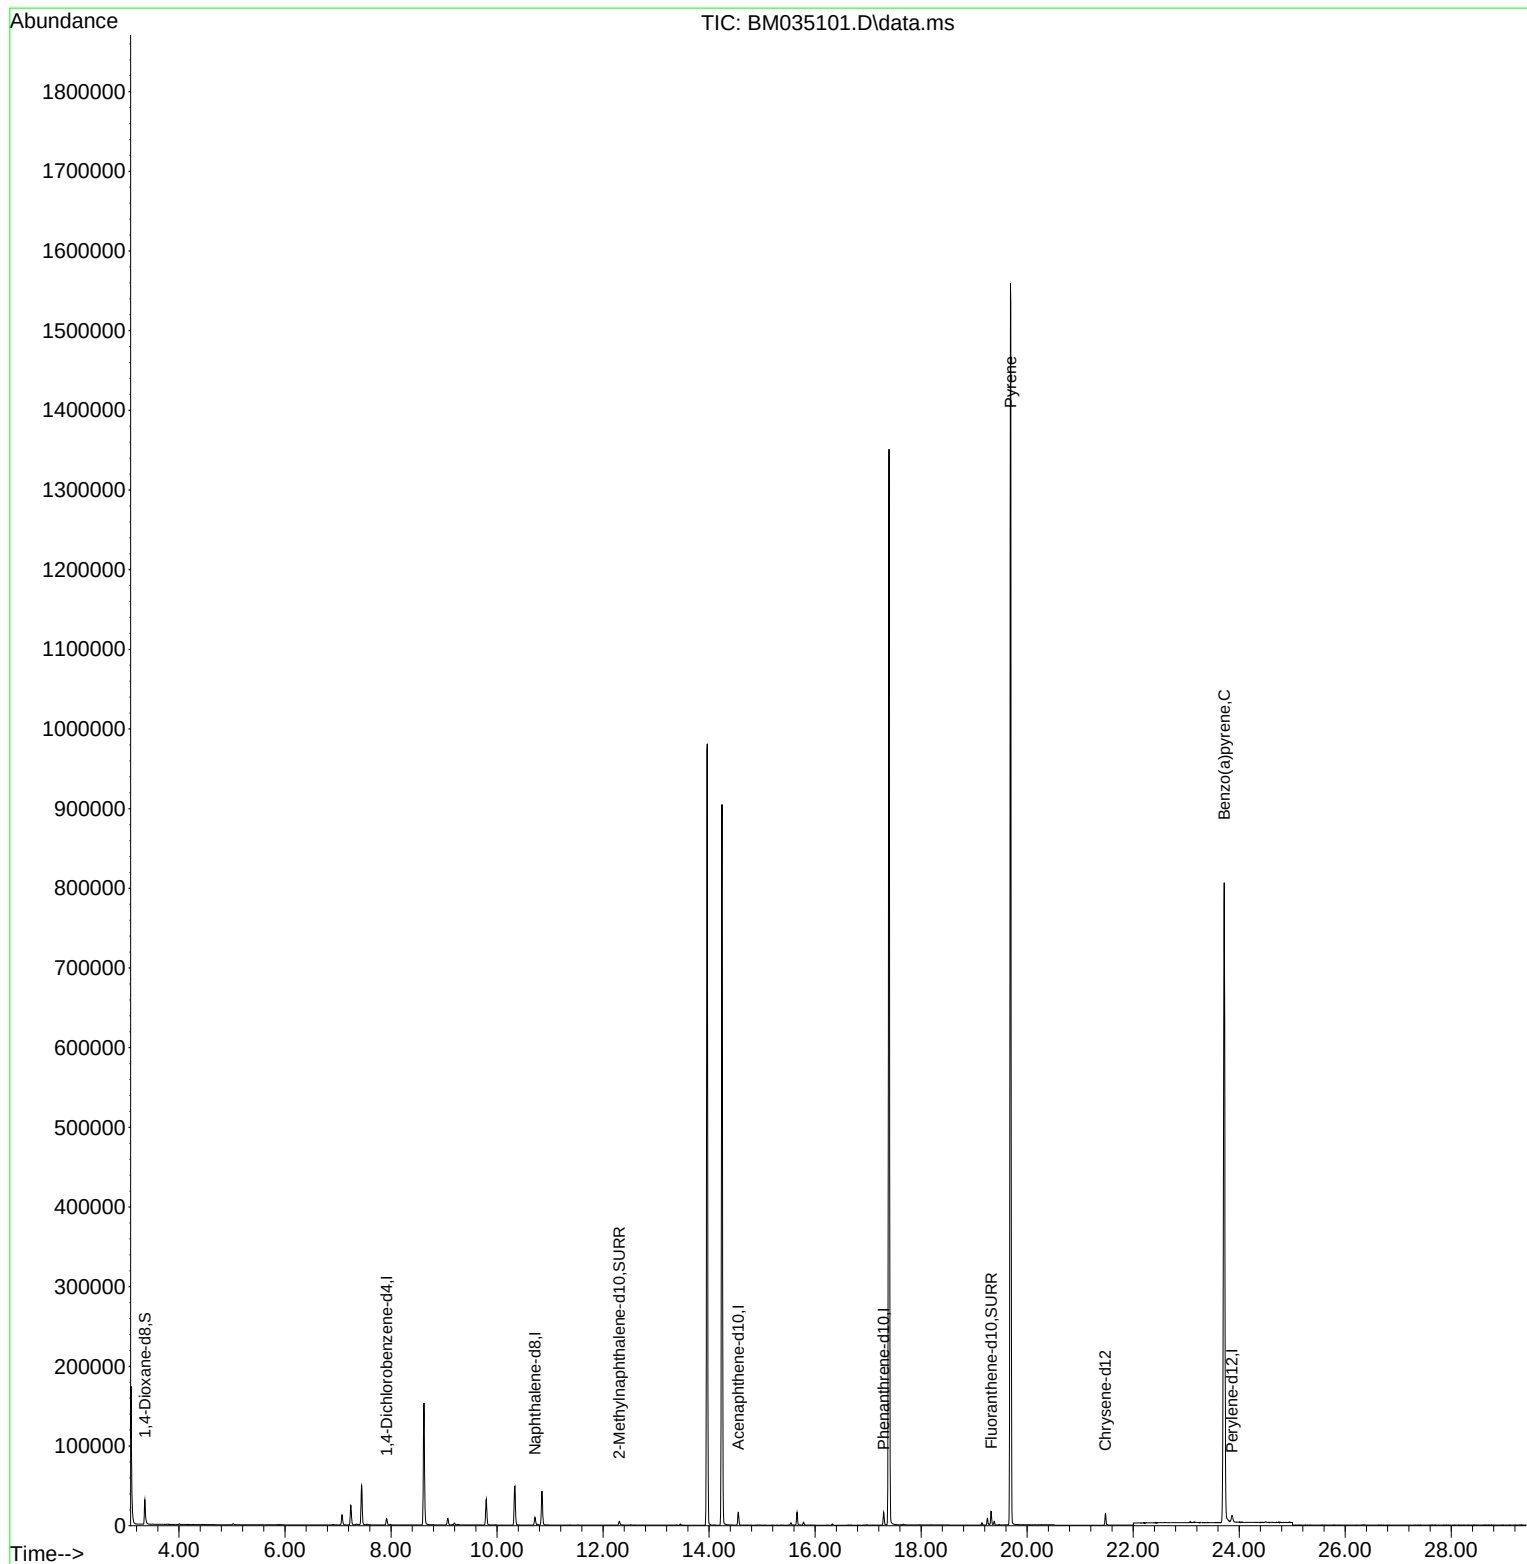

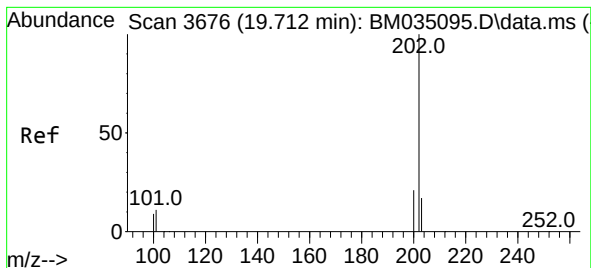

#20

Pyrene

Concen: 0.043 ng/ul

RT: 19.689 min Scan# 3

Delta R.T. -0.023 min

Lab File: BM035101.D

Acq: 16 May 2022 13:16

Instrument :

BNA_M

ClientSampleId :

EXLA4





Tgt Ion:202 Resp: 3336

Ion Ratio Lower Upper

202 100

101 156.3 9.3 13.9#

100 1143.4 7.8 11.6#

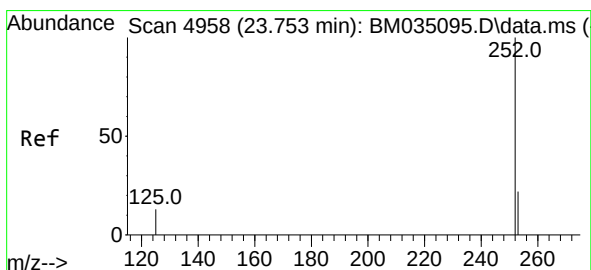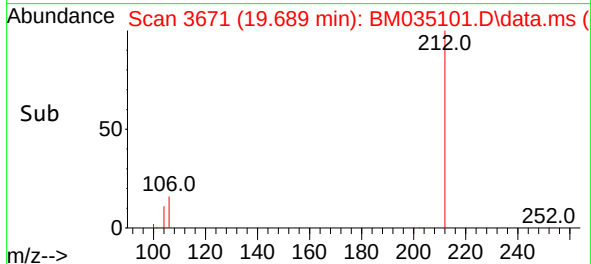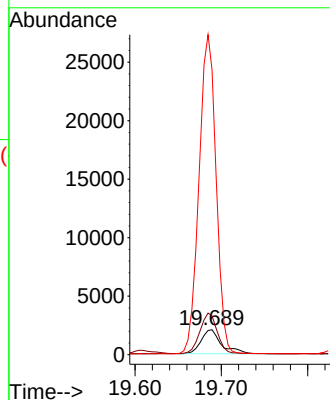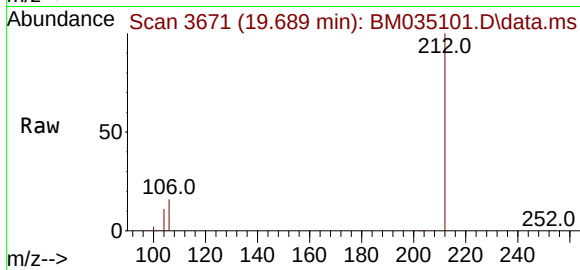

#26

Benzo(a)pyrene

Concen: 0.090 ng/ul

RT: 23.716 min Scan# 4945

Delta R.T. -0.035 min

Lab File: BM035101.D

Acq: 16 May 2022 13:16

Tgt Ion:252 Resp: 5095

Ion Ratio Lower Upper

252 100

253 45.0 32.0 48.0

125 41.4 14.5 21.7#

