

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM051622\
 Data File : BM035103.D
 Acq On : 16 May 2022 14:30
 Operator : CG/JU
 Sample : N2707-15
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EXLA6

Quant Time: May 17 00:51:08 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM051222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu May 12 18:15:39 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.917	152	3532	0.400	ng/ul	0.00
4) Naphthalene-d8	10.715	136	11553	0.400	ng/ul #	0.00
9) Acenaphthene-d10	14.552	164	7630	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.292	188	15864	0.400	ng/ul #	0.00
17) Chrysene-d12	21.476	240	11967	0.400	ng/ul	0.00
23) Perylene-d12	23.865	264	10500	0.400	ng/ul #	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.356	96	20192	4.772	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.310	152	7154	0.388	ng/ul	0.00
18) Fluoranthene-d10	19.322	212	18435	0.449	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.547	166	3022	0.079	ng/ul#	16
20) Pyrene	19.684	202	3431	0.050	ng/ul#	1
26) Benzo(a)pyrene	23.712	252	5400	0.108	ng/ul#	82


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM051622\
Data File : BM035103.D
Acq On : 16 May 2022 14:30
Operator : CG/JU
Sample : N2707-15
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EXLA6

Quant Time: May 17 00:51:08 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM051222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 12 18:15:39 2022
Response via : Initial Calibration




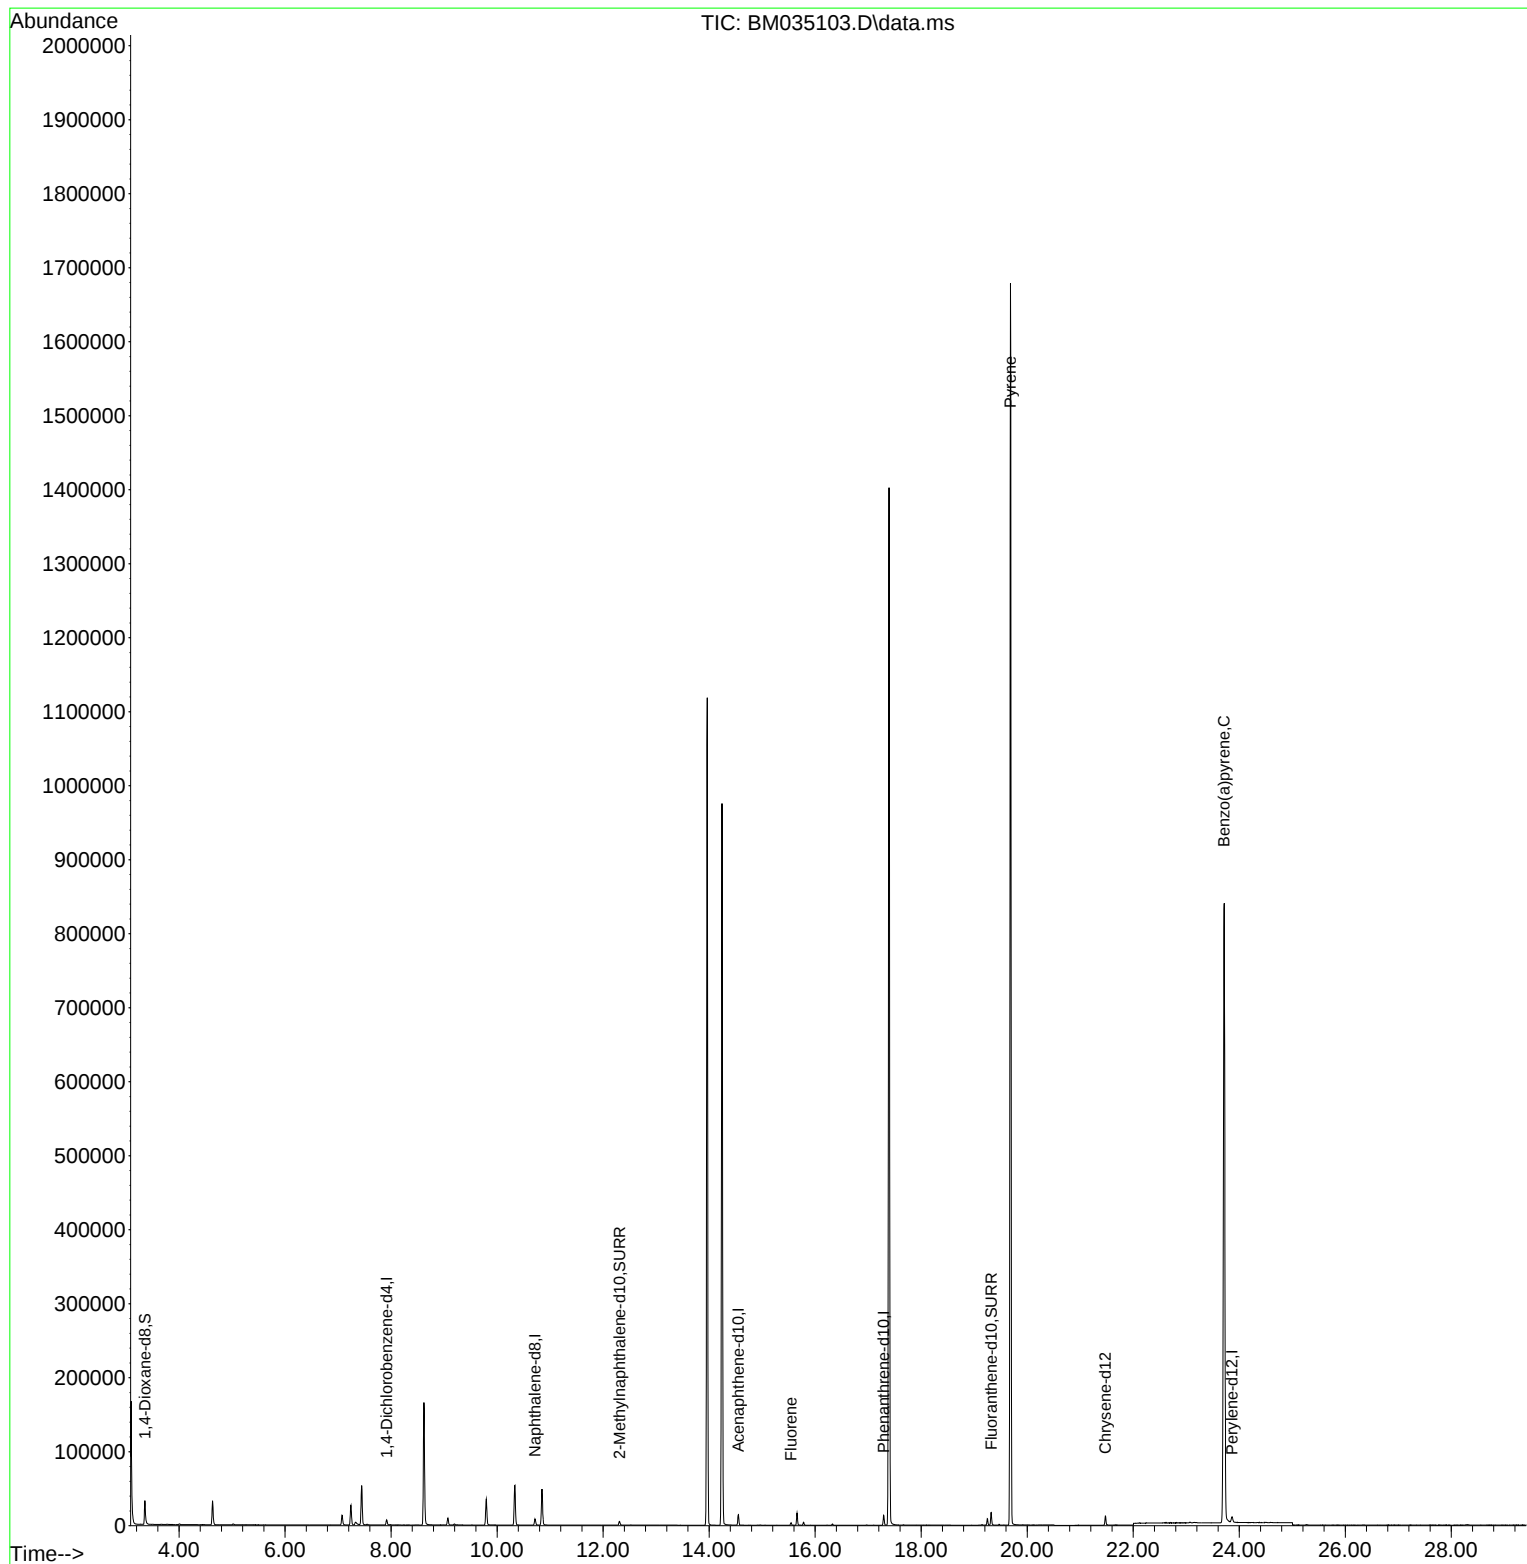


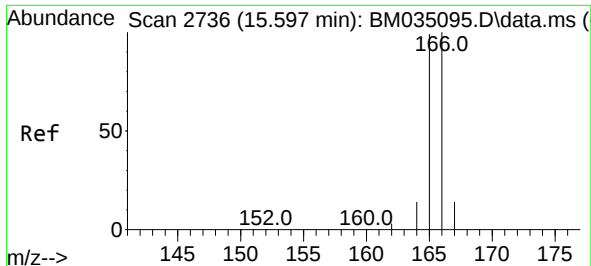

#12
Fluorene
Concen: 0.079 ng/ul
RT: 15.547 min Scan# 21
Delta R.T. -0.055 min
Lab File: BM035103.D
Acq: 16 May 2022 14:30




Instrument :
BNA_M
ClientSampleId :
EXLA6


Tgt Ion:166 Resp: 3022
Ion Ratio Lower Upper
166 100
165 7.5 81.1 121.7#
167 35.0 14.9 22.3#

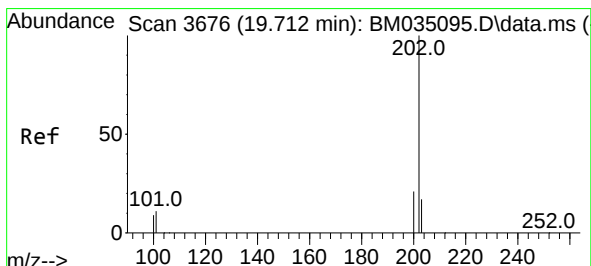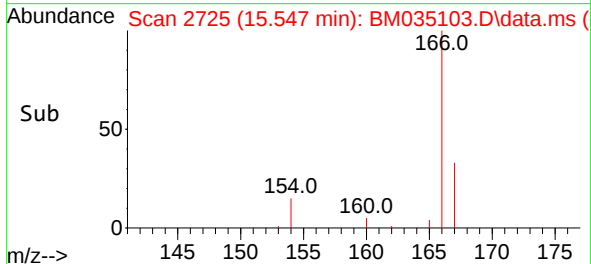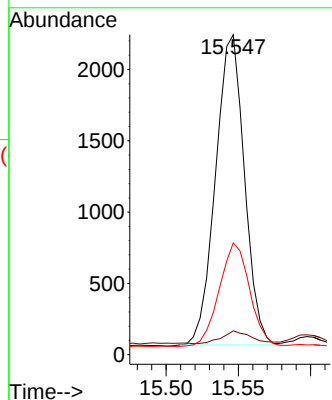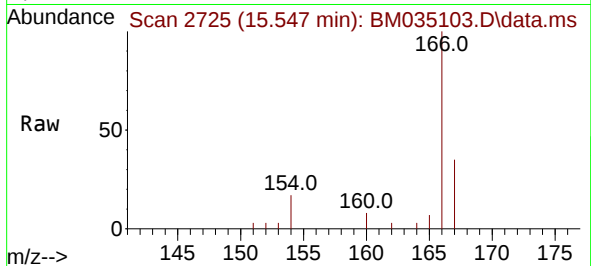

#20
Pyrene
Concen: 0.050 ng/ul
RT: 19.684 min Scan# 3670
Delta R.T. -0.028 min
Lab File: BM035103.D
Acq: 16 May 2022 14:30


Tgt Ion:202 Resp: 3431
Ion Ratio Lower Upper
202 100
101 174.1 9.3 13.9#
100 1347.0 7.8 11.6#

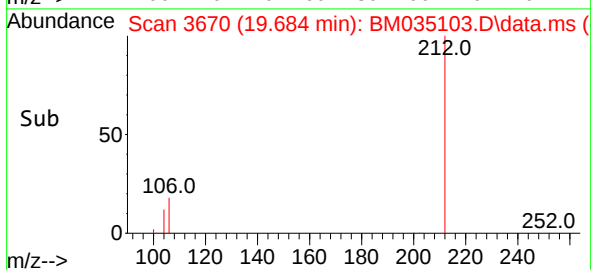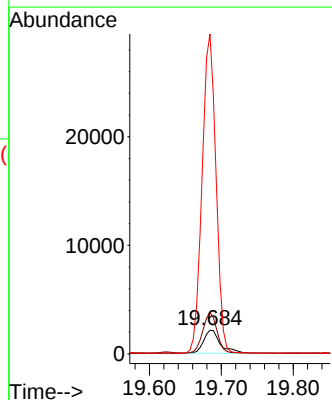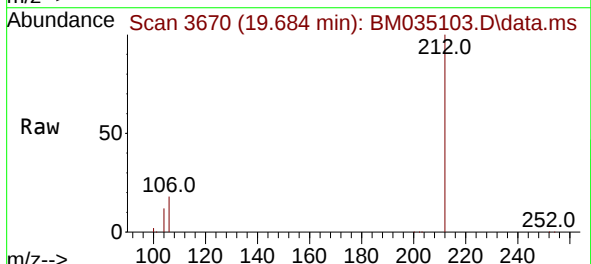

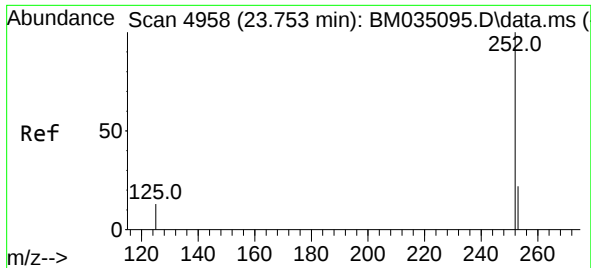

#26
 Benzo(a)pyrene
 Concen: 0.108 ng/ul
 RT: 23.712 min Scan# 4944
 Delta R.T. -0.038 min
 Lab File: BM035103.D
 Acq: 16 May 2022 14:30

Instrument :
 BNA_M
 ClientSampleId :
 EXLA6

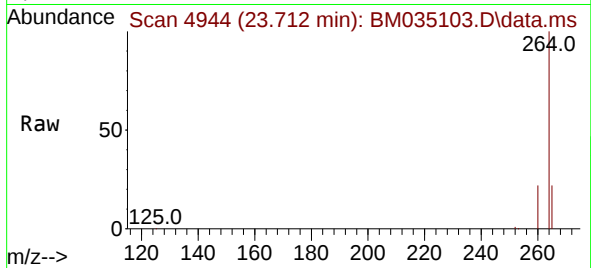

Tgt Ion:252	Resp:	5400
Ion Ratio	Lower	Upper
252	100	
253	42.9	32.0 48.0
125	39.5	14.5 21.7#

