

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM051622\
 Data File : BM035104.D
 Acq On : 16 May 2022 15:07
 Operator : CG/JU
 Sample : N2707-16
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EXLA7

Quant Time: May 17 00:51:12 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM051222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu May 12 18:15:39 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.917	152	3812	0.400	ng/ul	0.00
4) Naphthalene-d8	10.715	136	12373	0.400	ng/ul #	0.00
9) Acenaphthene-d10	14.553	164	8197	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.293	188	17213	0.400	ng/ul #	0.00
17) Chrysene-d12	21.476	240	13576	0.400	ng/ul	0.00
23) Perylene-d12	23.864	264	12081	0.400	ng/ul #	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.356	96	20586	4.508	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.305	152	6561	0.332	ng/ul	0.00
18) Fluoranthene-d10	19.323	212	16829	0.361	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.543	166	2801	0.068	ng/ul#	16
20) Pyrene	19.685	202	2877	0.037	ng/ul#	1
26) Benzo(a)pyrene	23.715	252	5076	0.088	ng/ul#	80


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM051622\
Data File : BM035104.D
Acq On : 16 May 2022 15:07
Operator : CG/JU
Sample : N2707-16
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EXLA7

Quant Time: May 17 00:51:12 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM051222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 12 18:15:39 2022
Response via : Initial Calibration




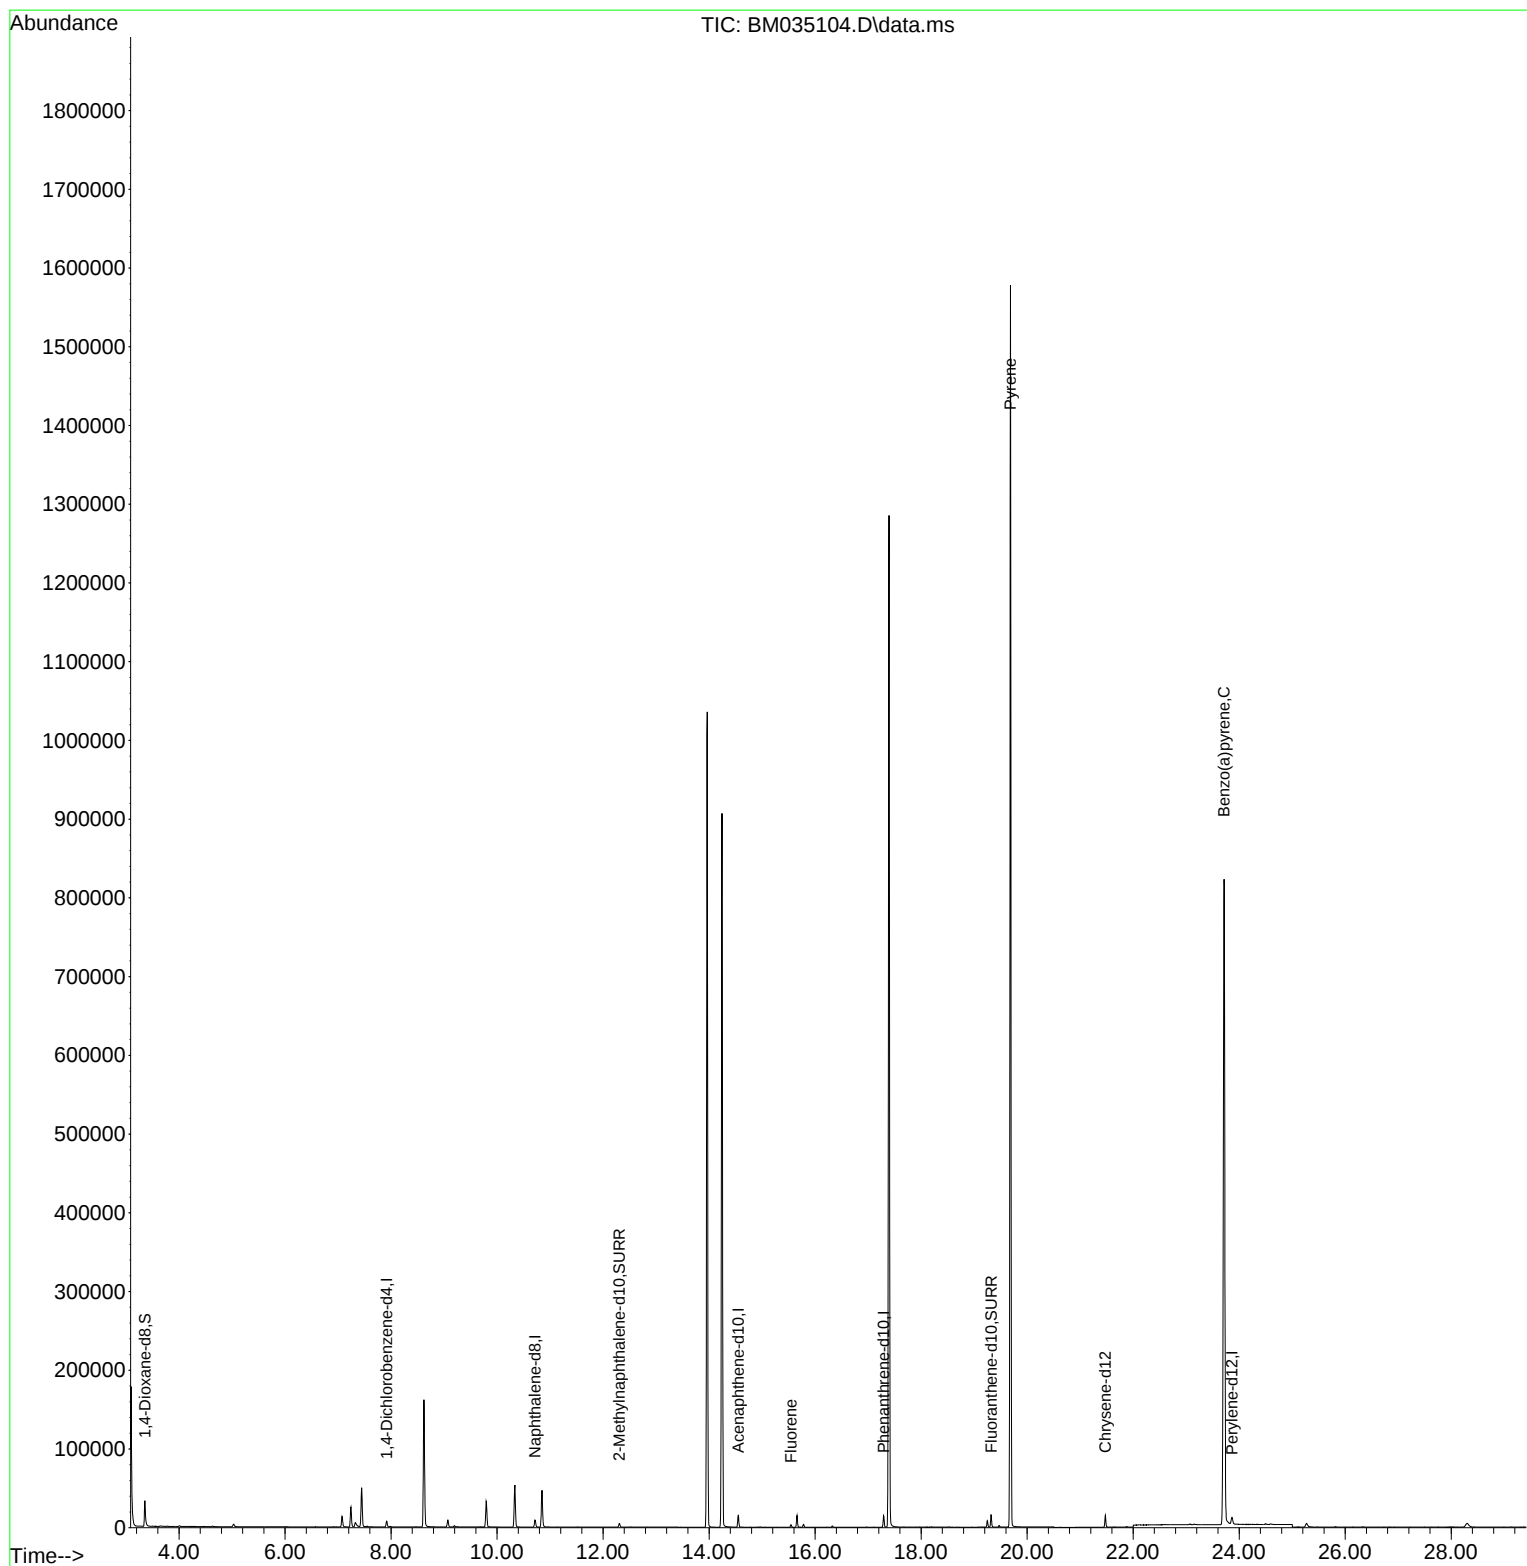


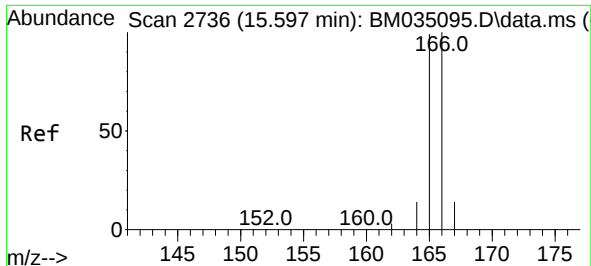

#12
Fluorene
Concen: 0.068 ng/ul
RT: 15.543 min Scan# 21
Delta R.T. -0.059 min
Lab File: BM035104.D
Acq: 16 May 2022 15:07




Instrument :
BNA_M
ClientSampleId :
EXLA7


Tgt Ion:166 Resp: 2801
Ion Ratio Lower Upper
166 100
165 7.1 81.1 121.7#
167 32.6 14.9 22.3#

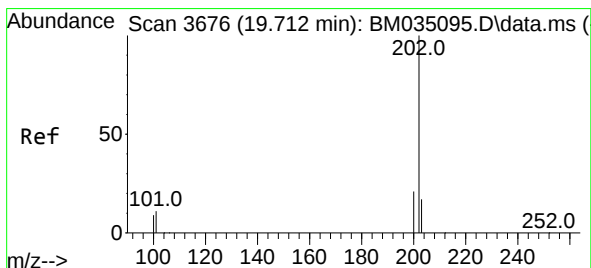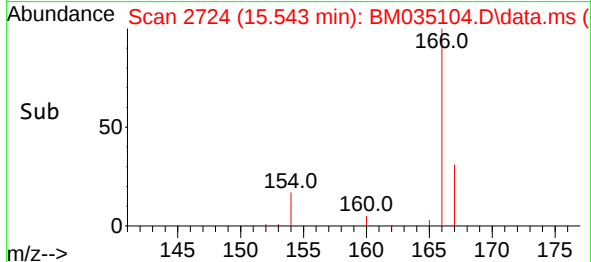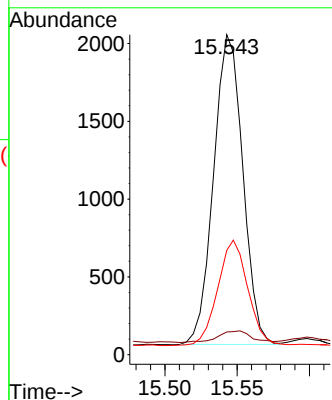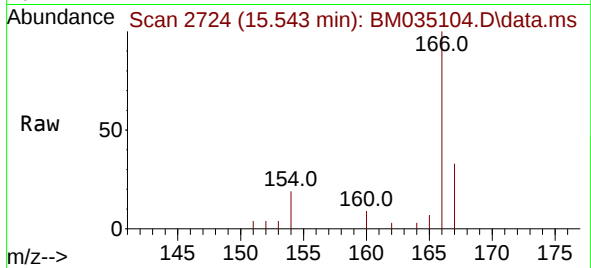

#20
Pyrene
Concen: 0.037 ng/ul
RT: 19.685 min Scan# 3670
Delta R.T. -0.027 min
Lab File: BM035104.D
Acq: 16 May 2022 15:07


Tgt Ion:202 Resp: 2877
Ion Ratio Lower Upper
202 100
101 168.4 9.3 13.9#
100 1297.2 7.8 11.6#

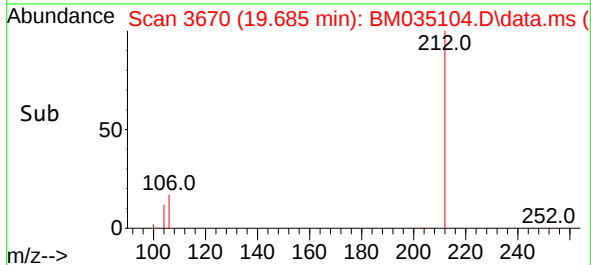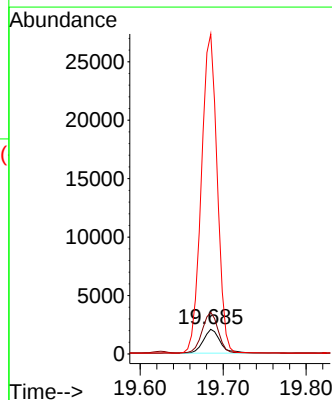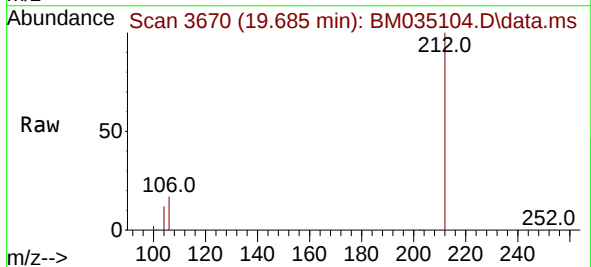

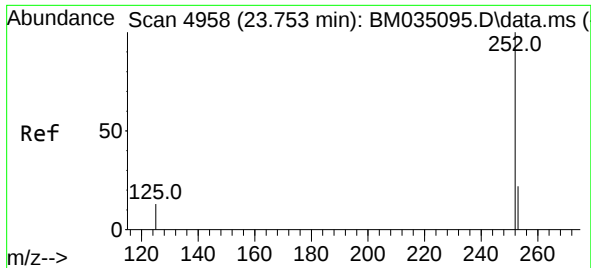

#26
Benzo(a)pyrene
Concen: 0.088 ng/ul
RT: 23.715 min Scan# 4945
Delta R.T. -0.036 min
Lab File: BM035104.D
Acq: 16 May 2022 15:07

Instrument :
BNA_M
ClientSampleId :
EXLA7

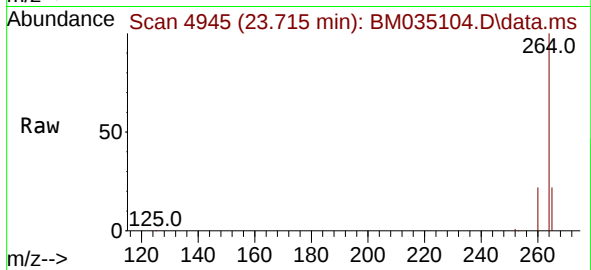

Tgt Ion:252 Resp: 5076
Ion Ratio Lower Upper
252 100
253 44.0 32.0 48.0
125 40.2 14.5 21.7#

