

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM051622\
 Data File : BM035115.D
 Acq On : 16 May 2022 22:30
 Operator : CG/JU
 Sample : N2707-18
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EXLB1

Quant Time: May 17 00:51:50 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM051222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu May 12 18:15:39 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.917	152	2444	0.400	ng/ul	0.00
4) Naphthalene-d8	10.715	136	8336	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.552	164	5767	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.292	188	12811	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.473	240	12182	0.400	ng/ul	0.00
23) Perylene-d12	23.855	264	12065	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.352	96	11858	4.050	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.305	152	4738	0.356	ng/ul	0.00
18) Fluoranthene-d10	19.317	212	14306	0.342	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.684	202	2537	0.037	ng/ul#	1
26) Benzo(a)pyrene	23.709	252	5544	0.096	ng/ul#	80


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM051622\
Data File : BM035115.D
Acq On : 16 May 2022 22:30
Operator : CG/JU
Sample : N2707-18
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EXLB1

Quant Time: May 17 00:51:50 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM051222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 12 18:15:39 2022
Response via : Initial Calibration




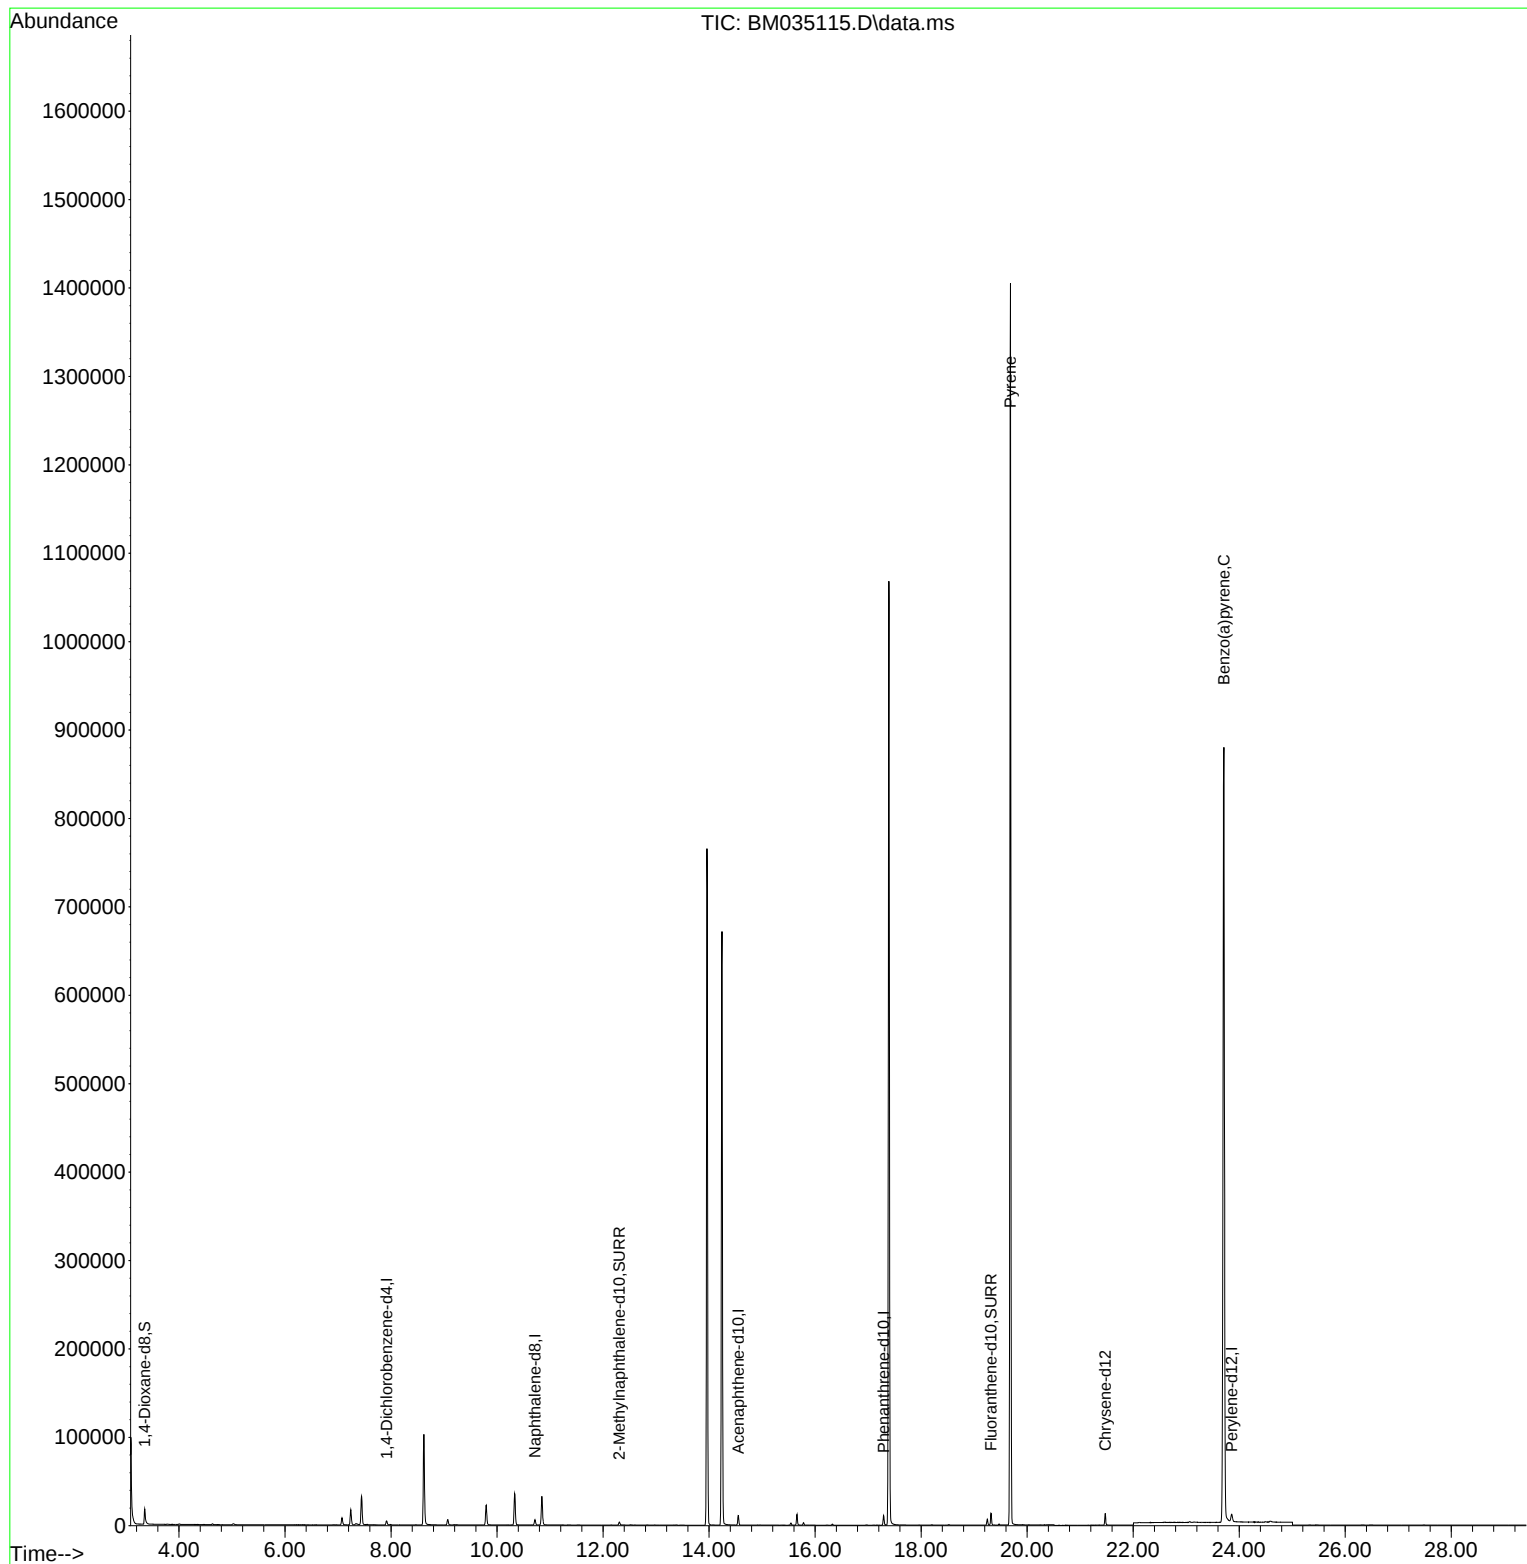


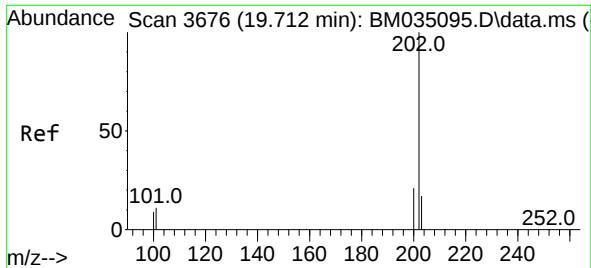

#20
Pyrene
Concen: 0.037 ng/ul
RT: 19.684 min Scan# 30
Delta R.T. -0.028 min
Lab File: BM035115.D
Acq: 16 May 2022 22:30

Instrument :
BNA_M
ClientSampleId :
EXLB1

Tgt Ion:202 Resp: 2537
Ion Ratio Lower Upper
202 100
101 169.6 9.3 13.9#
100 1266.1 7.8 11.6#

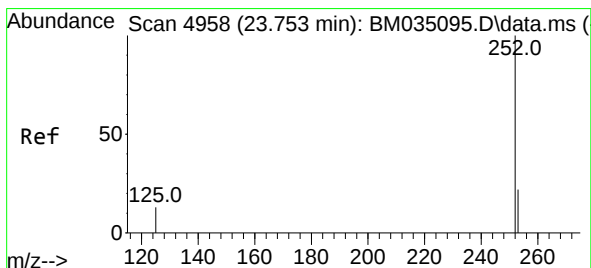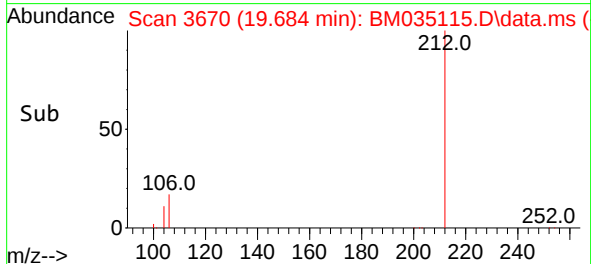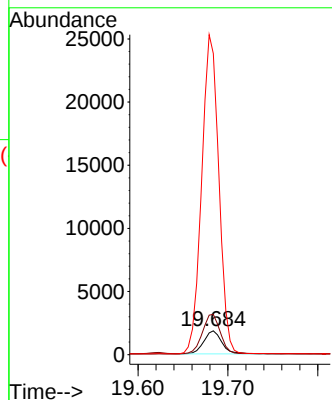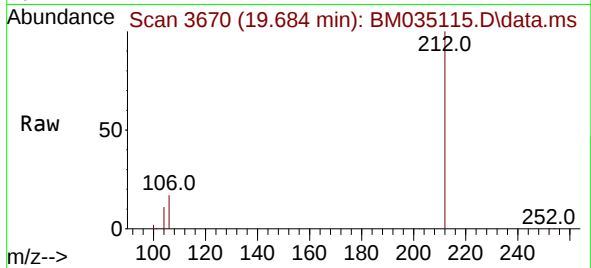

#26
Benzo(a)pyrene
Concen: 0.096 ng/ul
RT: 23.709 min Scan# 4943
Delta R.T. -0.041 min
Lab File: BM035115.D
Acq: 16 May 2022 22:30

Tgt Ion:252 Resp: 5544
Ion Ratio Lower Upper
252 100
253 44.2 32.0 48.0
125 40.4 14.5 21.7#

