

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM051622\
 Data File : BM035116.D
 Acq On : 16 May 2022 23:06
 Operator : CG/JU
 Sample : N2801-01
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EXLB4

Quant Time: May 17 00:51:53 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM051222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu May 12 18:15:39 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.913	152	3347	0.400	ng/ul	0.00
4) Naphthalene-d8	10.716	136	11089	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.547	164	7496	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.292	188	16271	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.471	240	14705	0.400	ng/ul	0.00
23) Perylene-d12	23.856	264	13506	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.357	96	16935	4.224	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.305	152	5295	0.299	ng/ul	0.00
18) Fluoranthene-d10	19.317	212	14759	0.293	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.684	202	3085	0.037	ng/ul#	1
26) Benzo(a)pyrene	23.707	252	5451	0.085	ng/ul#	80


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM051622\
Data File : BM035116.D
Acq On : 16 May 2022 23:06
Operator : CG/JU
Sample : N2801-01
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EXLB4

Quant Time: May 17 00:51:53 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM051222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 12 18:15:39 2022
Response via : Initial Calibration

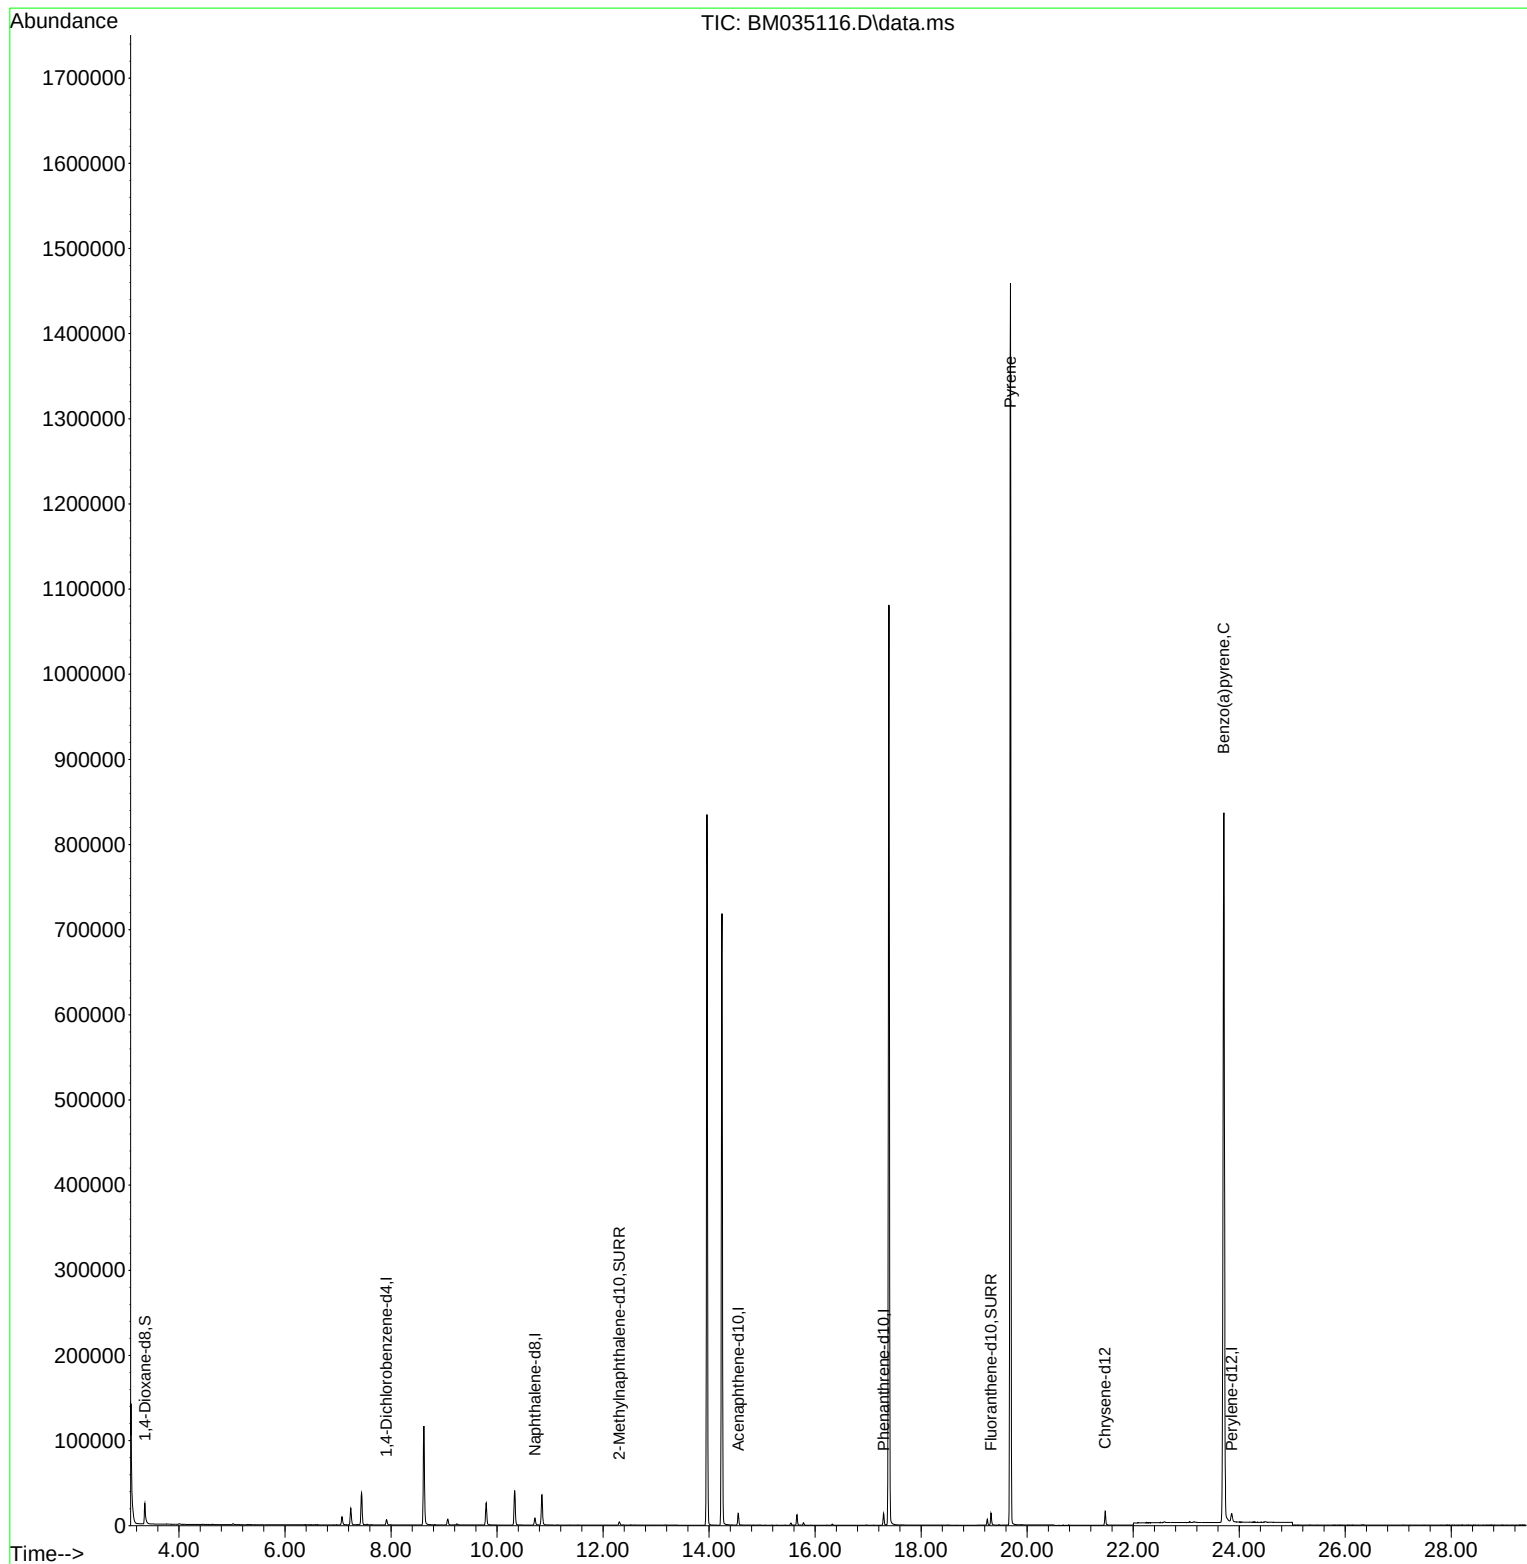

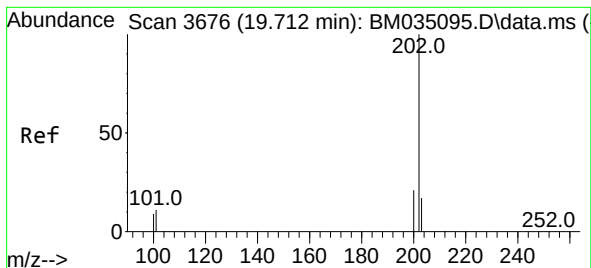

#20

Pyrene

Concen: 0.037 ng/ul

RT: 19.684 min Scan# 3

Delta R.T. -0.028 min

Lab File: BM035116.D

Acq: 16 May 2022 23:06

Instrument :





BNA_M

ClientSampleId :

EXLB4

Tgt Ion:202 Resp: 3085

Ion	Ratio	Lower	Upper
202	100		
101	170.0	9.3	13.9#
100	1273.5	7.8	11.6#

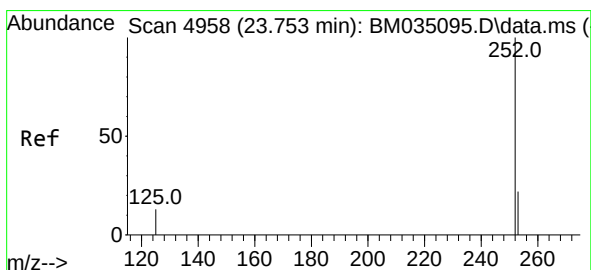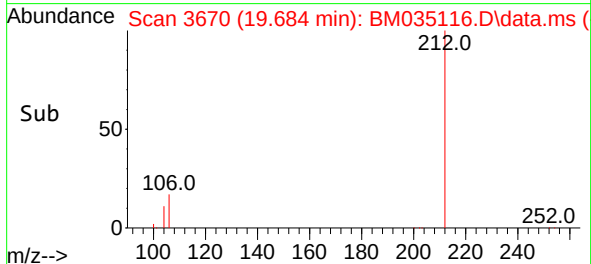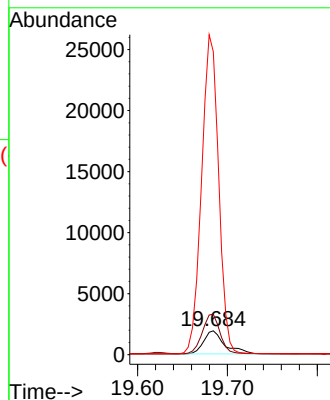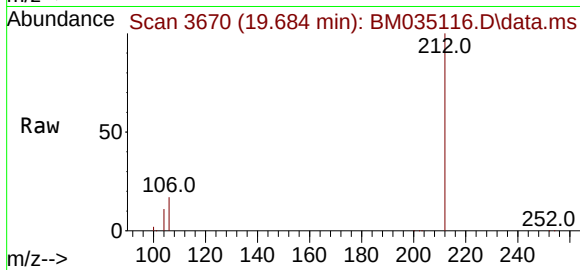

#26

Benzo(a)pyrene

Concen: 0.085 ng/ul

RT: 23.707 min Scan# 4942

Delta R.T. -0.044 min

Lab File: BM035116.D

Acq: 16 May 2022 23:06

Tgt Ion:252 Resp: 5451

Ion	Ratio	Lower	Upper
252	100		
253	43.4	32.0	48.0
125	41.1	14.5	21.7#

