

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM051622\
 Data File : BM035122.D
 Acq On : 17 May 2022 02:45
 Operator : CG/JU
 Sample : N2801-08
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EXLE1

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 05/17/2022
 Supervised By :mohammad ahmed 05/18/2022

Quant Time: May 17 04:05:05 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM051222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu May 12 18:15:39 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.913	152	2494	0.400	ng/ul	0.00
4) Naphthalene-d8	10.710	136	8088	0.400	ng/ul	#-0.01
9) Acenaphthene-d10	14.547	164	5652	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.288	188	12624	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.471	240	10818	0.400	ng/ul	# 0.00
23) Perylene-d12	23.856	264	10032	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.352	96	13038m	4.364	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.305	152	4462	0.346	ng/ul	0.00
18) Fluoranthene-d10	19.317	212	11920	0.321	ng/ul	0.00
Target Compounds						
					Qvalue	
5) Naphthalene	10.765	128	1300	0.049	ng/ul#	79

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM051622\
Data File : BM035122.D
Acq On : 17 May 2022 02:45
Operator : CG/JU
Sample : N2801-08
Misc :
ALS Vial : 29 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
EXLE1

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 05/17/2022
Supervised By :mohammad ahmed 05/18/2022


Quant Time: May 17 04:05:05 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM051222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 12 18:15:39 2022
Response via : Initial Calibration

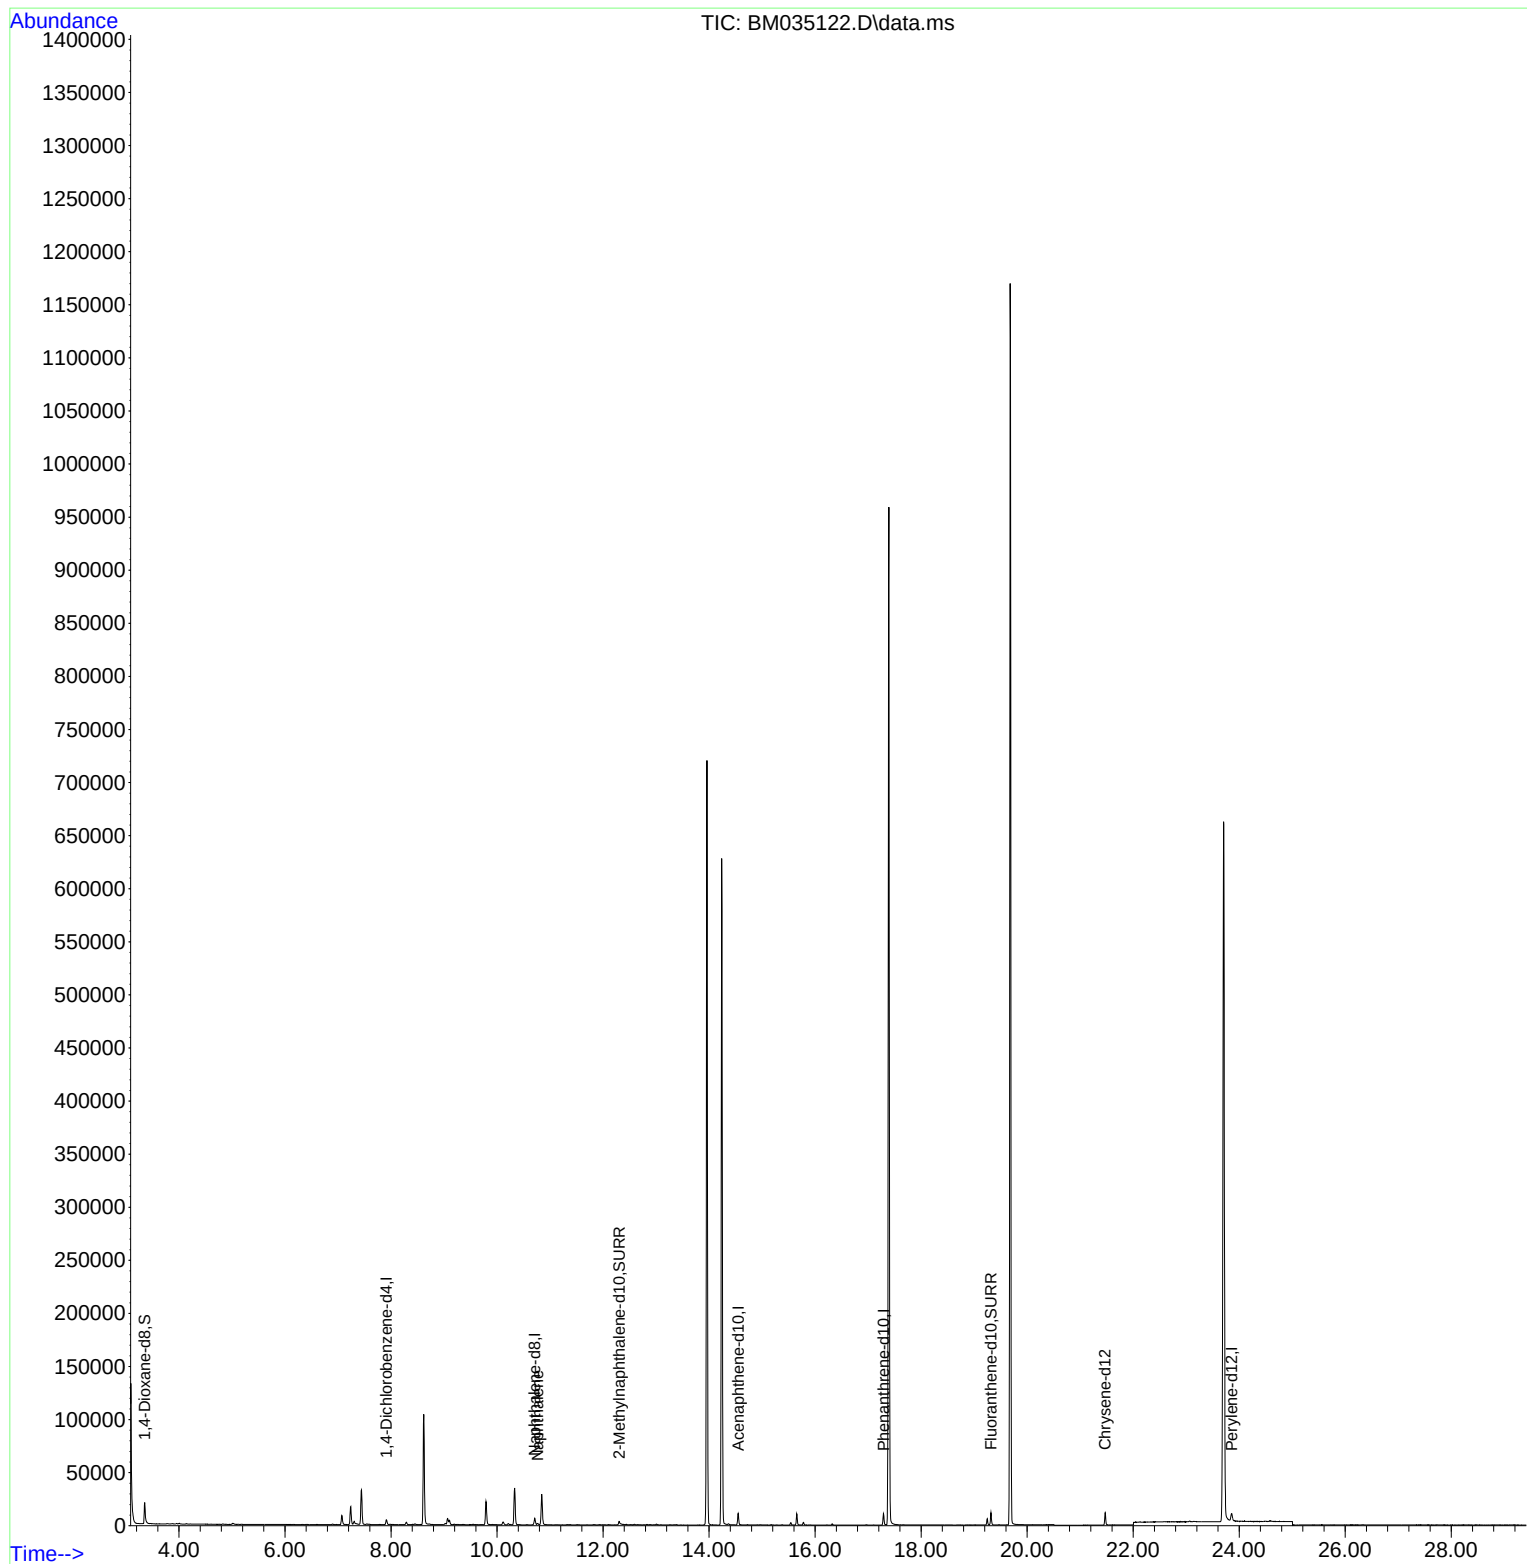

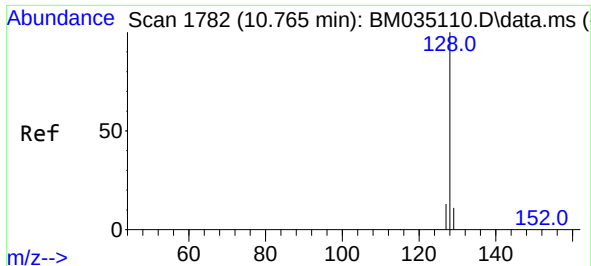

#5
Naphthalene
Concen: 0.049 ng/ul
RT: 10.765 min Scan# 11
Delta R.T. -0.005 min
Lab File: BM035122.D
Acq: 17 May 2022 02:45

Instrument :
BNA_M
ClientSampleId :
EXLE1

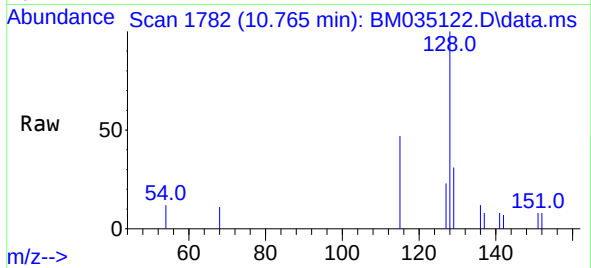

Tgt Ion:	128	Resp:	1300
Ion	Ratio	Lower	Upper
128	100		
129	31.3	13.4	20.2
127	23.1	15.2	22.8

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 05/17/2022
Supervised By :mohammad ahmed 05/18/2022

