


Data Path : Z:\HPCHEM1\BNA_M\Data\BM051715\
 Data File : BM001321.D
 Acq On : 15 May 2015 08:56
 Operator : TP/IZ
 Sample : DFTPP60
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP60

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF043015.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri May 15 01:57:52 2015

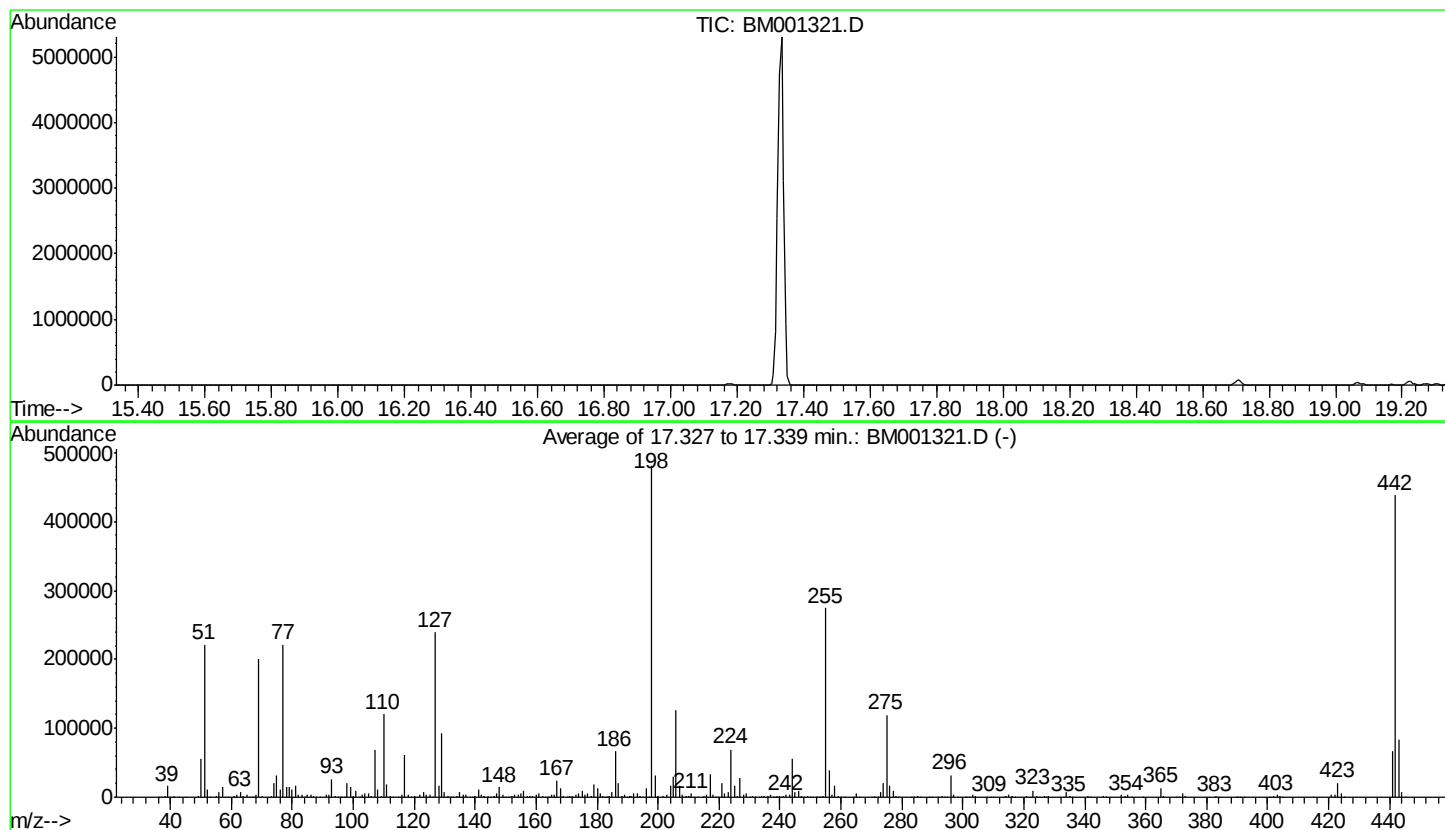

AutoFind: Scans 2489, 2490, 2491; Background Corrected with Scan 2482

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.1	221954	PASS
68	69	0.00	2	1.6	3221	PASS
69	198	0.00	100	41.8	201290	PASS
70	69	0.00	2	0.5	1091	PASS
127	198	10	80	49.7	239381	PASS
197	198	0.00	2	0.2	909	PASS
198	198	100	100	100.0	481237	PASS
199	198	5	9	6.8	32488	PASS
275	198	10	60	24.7	119058	PASS
365	198	1	100	2.8	13502	PASS
441	442	0.01	24	15.3	67208	PASS
442	198	50	100	91.0	437888	PASS
443	442	15	24	18.9	82826	PASS