


Data Path : Z:\HPCHEM1\BNA_M\Data\BM051815\
 Data File : BM001326.D
 Acq On : 15 May 2015 13:50
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF043015.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri May 15 01:57:52 2015

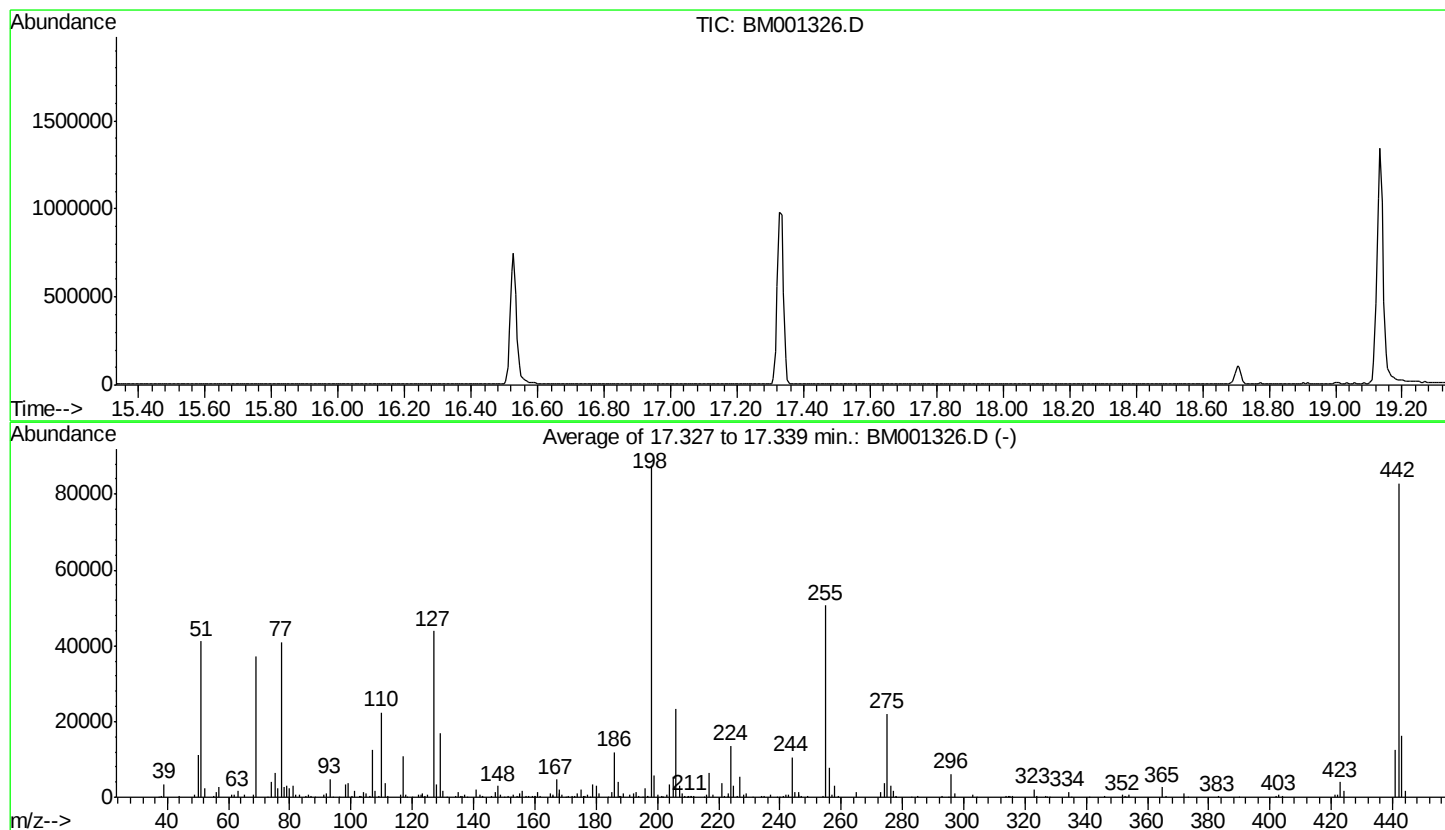

AutoFind: Scans 2489, 2490, 2491; Background Corrected with Scan 2482

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	47.1	41216	PASS
68	69	0.00	2	1.9	690	PASS
69	198	0.00	100	42.3	37077	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	50.2	43925	PASS
197	198	0.00	2	0.3	280	PASS
198	198	100	100	100.0	87557	PASS
199	198	5	9	6.6	5749	PASS
275	198	10	60	25.1	22002	PASS
365	198	1	100	3.0	2649	PASS
441	442	0.01	24	15.2	12619	PASS
442	198	50	100	94.8	82970	PASS
443	442	15	24	19.4	16130	PASS