

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM051815\
 Data File : BM001328.D
 Acq On : 15 May 2015 15:19
 Operator : TP/IZ
 Sample : G2182-02
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 S32-0483

Quant Time: May 18 11:19:18 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SIMPAH-BM051315.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat May 16 01:36:33 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.45	152	14104	5.00	ng	0.02
6) Naphthalene-d8	10.22	136	48974	5.00	ng	0.00
12) Acenaphthene-d10	14.12	164	25198	5.00	ng	0.00
18) Phenanthrene-d10	16.85	188	73067	5.00	ng	0.00
24) Chrysene-d12	21.08	240	47192	5.00	ng	0.01
30) Perylene-d12	23.18	264	45502	5.00	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.02	112	10990	4.00	ng	0.00
5) Phenol-d6	6.63	99	7511	2.42	ng	0.00
7) Nitrobenzene-d5	8.60	82	18575	5.99	ng	0.00
13) 2,4,6-Tribromophenol	15.63	330	7373	8.53	ng	0.03
14) 2-Fluorobiphenyl	12.73	172	56526	7.23	ng	0.00
26) Terphenyl-d14	19.51	244	54085	8.53	ng	0.00


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM051815\
Data File : BM001328.D
Acq On : 15 May 2015 15:19
Operator : TP/IZ
Sample : G2182-02
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
S32-0483

Quant Time: May 18 11:19:18 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SIMPAH-BM051315.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat May 16 01:36:33 2015
Response via : Initial Calibration

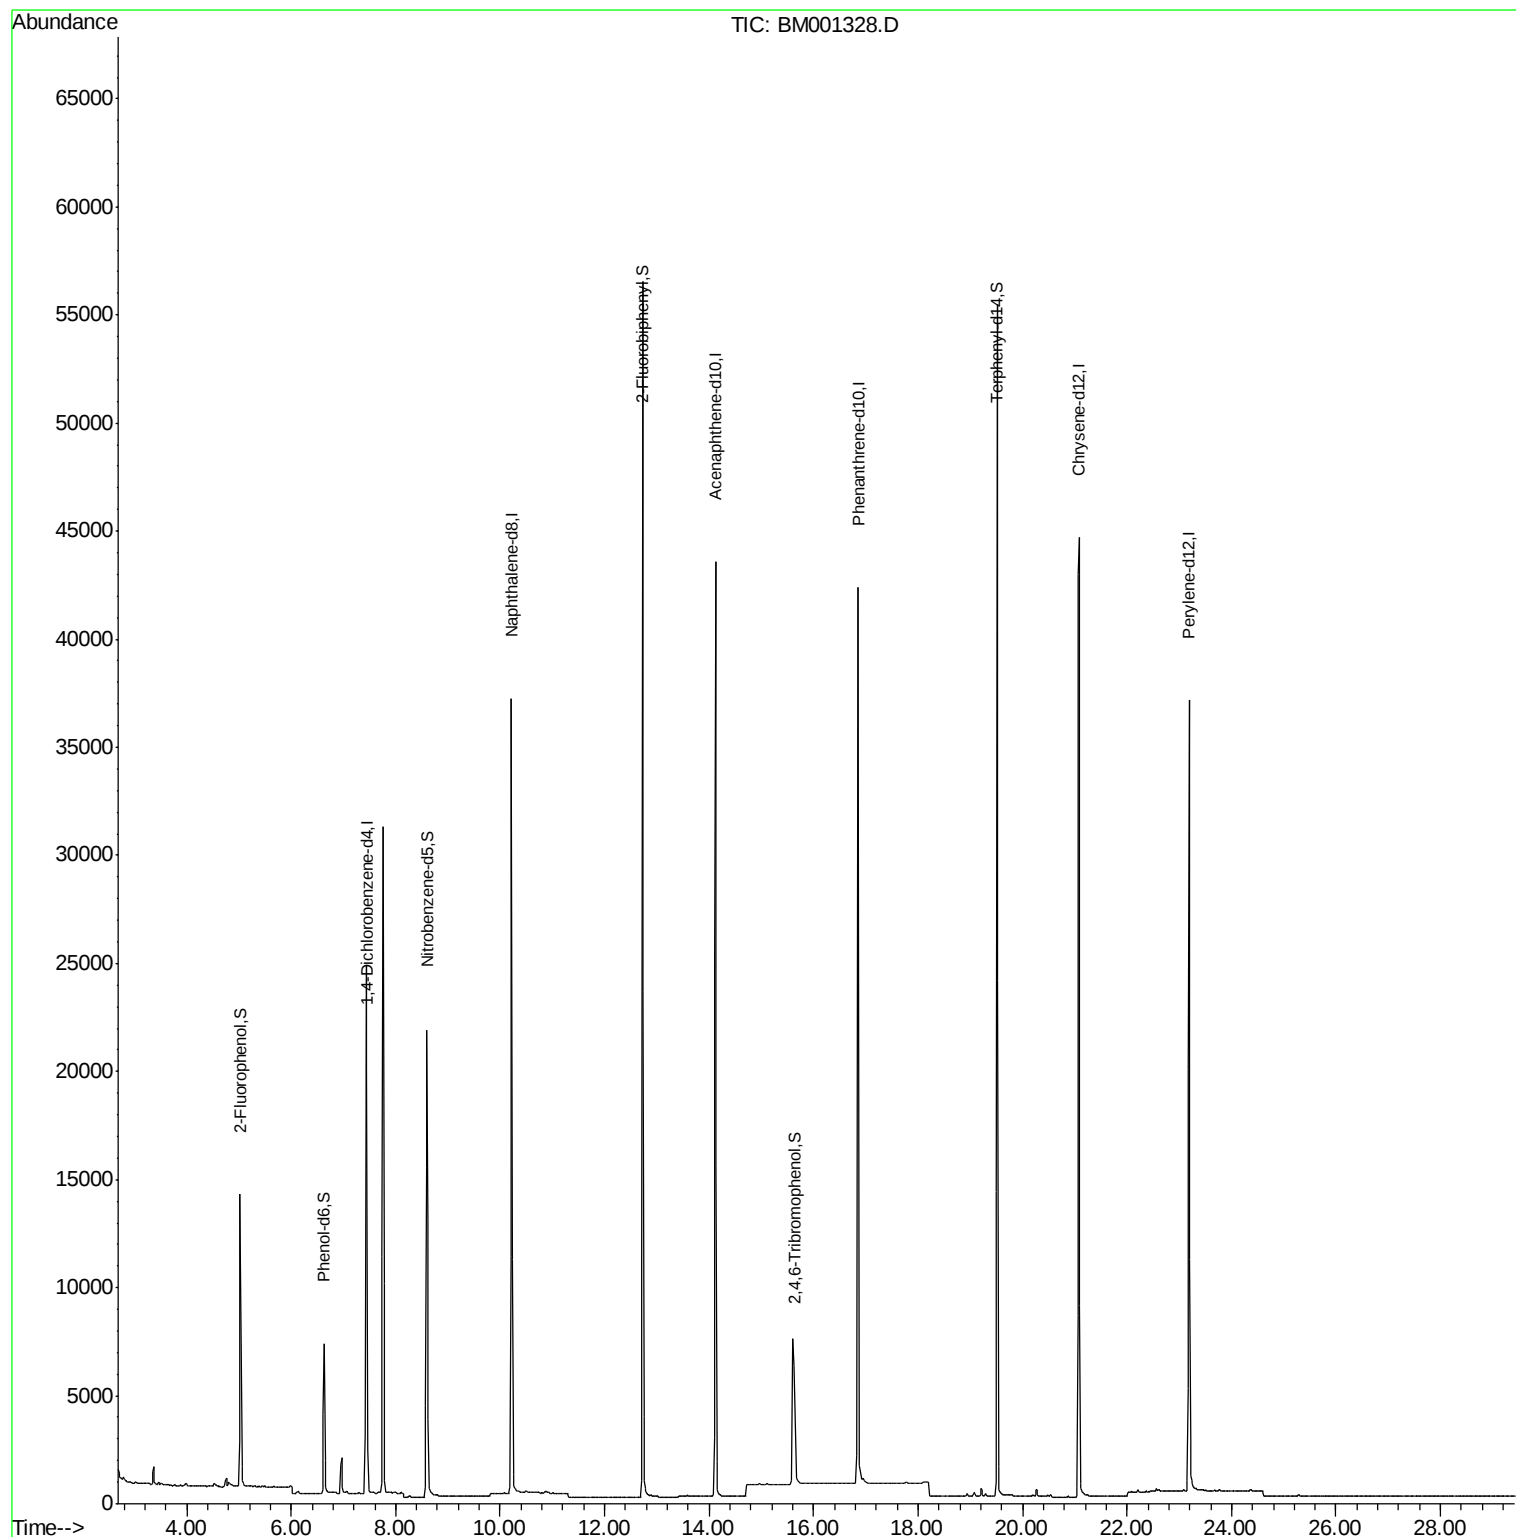

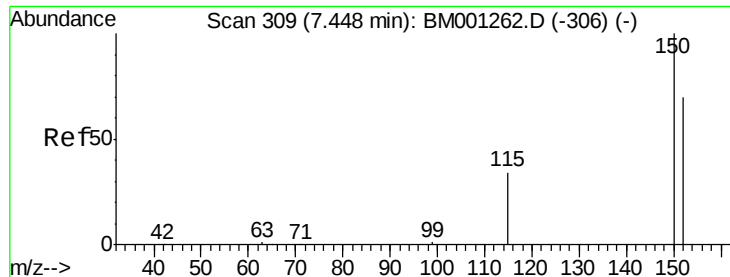

#1

1,4-Dichlorobenzene-d4

Concen: 5.00 ng

RT: 7.45 min Scan# 309

Delta R.T. 0.02 min

Lab File: BM001328.D

Acq: 15 May 2015 15:19

Instrument :

BNA_M

ClientSampleId :

S32-0483





Tgt Ion:152 Resp: 14104

Ion Ratio Lower Upper

152 100

150 133.5 114.6 172.0

115 42.9 39.3 58.9

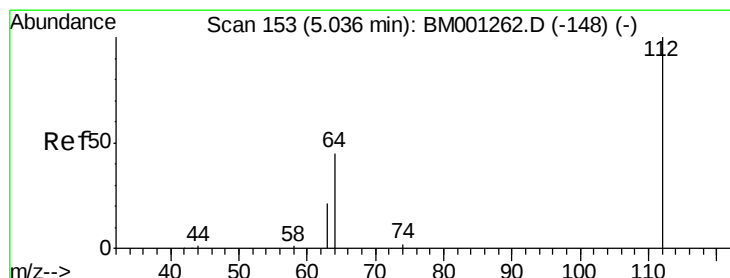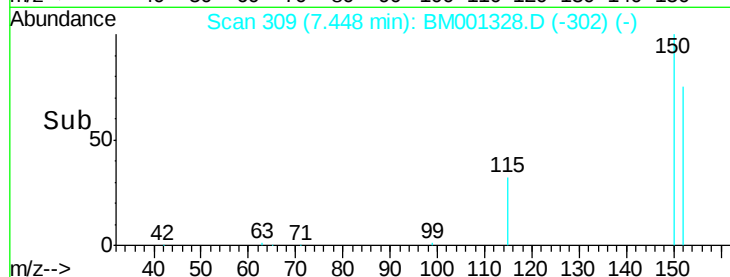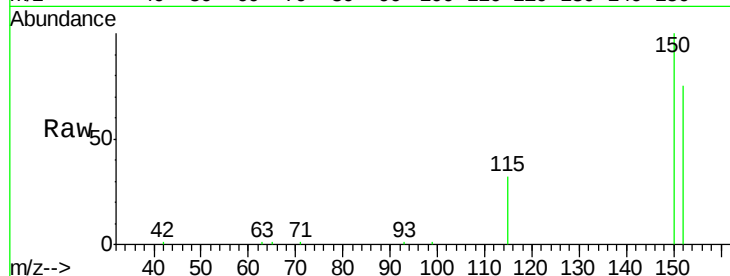

#4

2-Fluorophenol

Concen: 4.00 ng

RT: 5.02 min Scan# 152

Delta R.T. 0.00 min

Lab File: BM001328.D

Acq: 15 May 2015 15:19




Tgt Ion:112 Resp: 10990


Ion Ratio Lower Upper

112 100

64 64.8 50.8 76.2

63 36.0 28.2 42.4

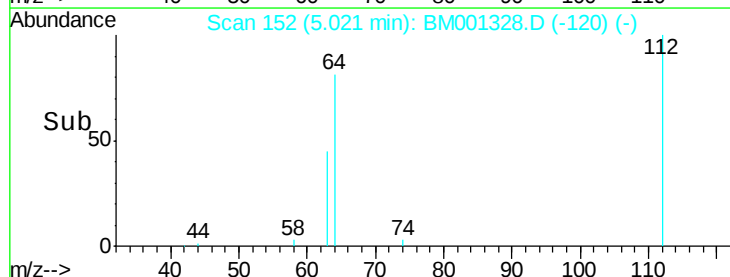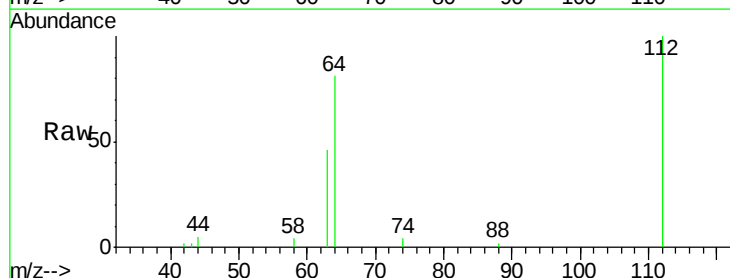

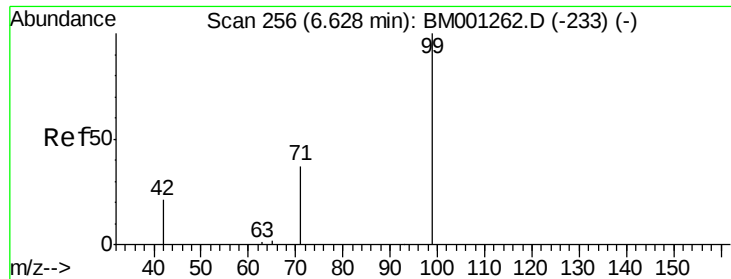

#5

Phenol-d6

Concen: 2.42 ng

RT: 6.63 min Scan# 256

Delta R.T. 0.00 min

Lab File: BM001328.D

Acq: 15 May 2015 15:19

Instrument :

BNA_M

ClientSampleId :

S32-0483


Tgt Ion: 99 Resp: 7511

Ion Ratio Lower Upper




99 100

42 24.6 19.9 29.9

71 35.3 28.0 42.0

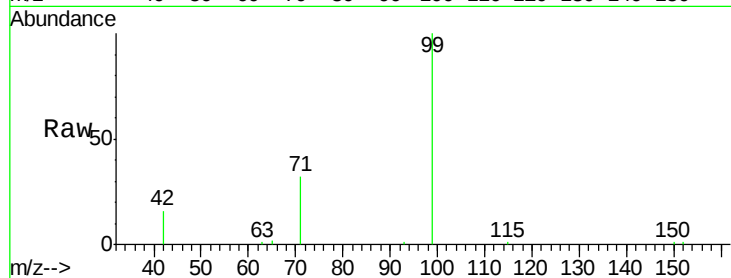

Abundance Ion 99.00 (98.70 to 99.70): BM001328.D (-224) (-)

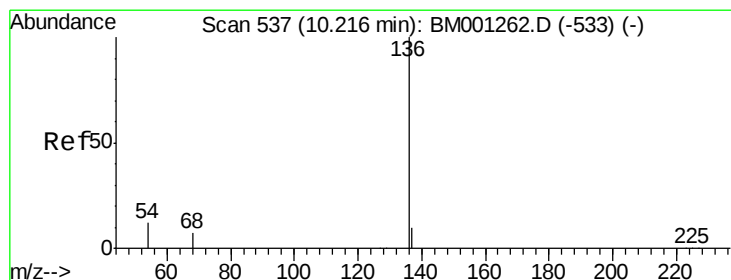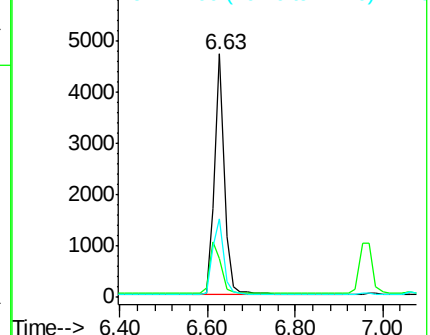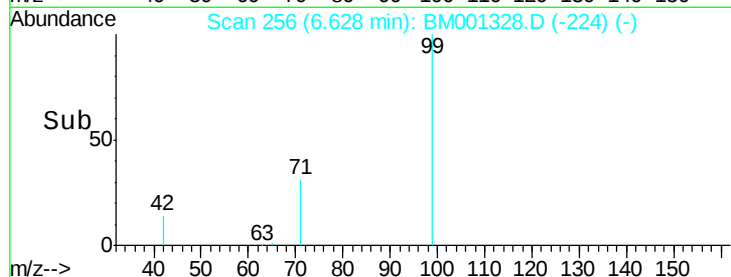

#6

Naphthalene-d8

Concen: 5.00 ng

RT: 10.22 min Scan# 537

Delta R.T. 0.00 min

Lab File: BM001328.D

Acq: 15 May 2015 15:19

Tgt Ion: 136 Resp: 48974


Ion Ratio Lower Upper

136 100



137 10.7 8.2 12.4


54 8.7 9.5 14.3#

68 5.3 5.5 8.3#

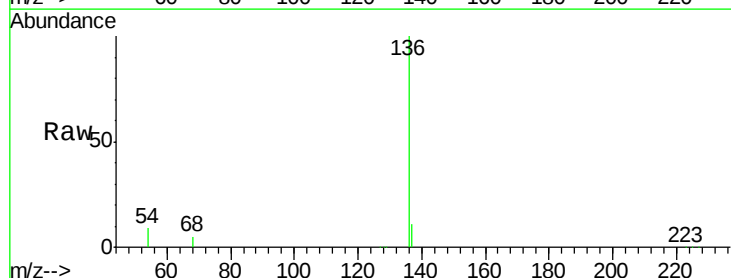

Abundance Ion 136.00 (135.70 to 136.70): BM001328.D (-520) (-)

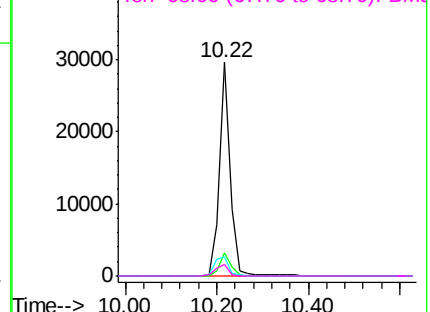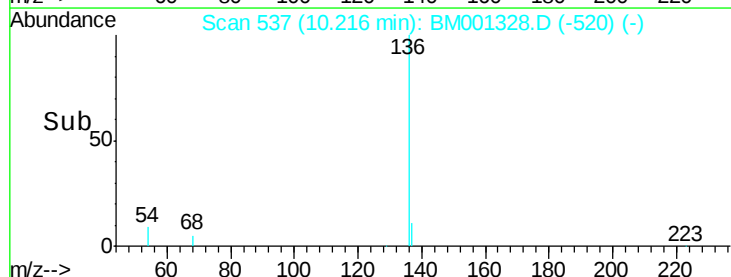

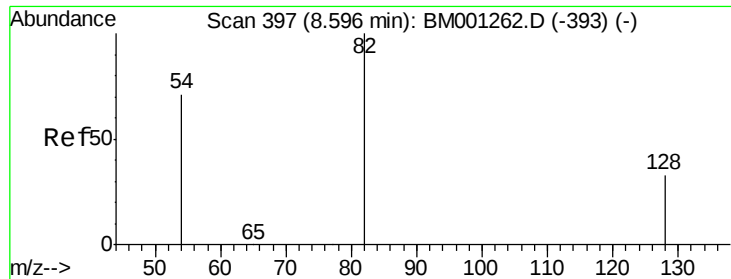

#7

Nitrobenzene-d5

Concen: 5.99 ng

RT: 8.60 min Scan# 397

Delta R.T. 0.00 min

Lab File: BM001328.D

Acq: 15 May 2015 15:19

Instrument :

BNA_M

ClientSampleId :

S32-0483


Tgt Ion: 82 Resp: 18575

Ion Ratio Lower Upper

82 100

128 39.4 28.0 42.0




54 58.0 57.3 85.9

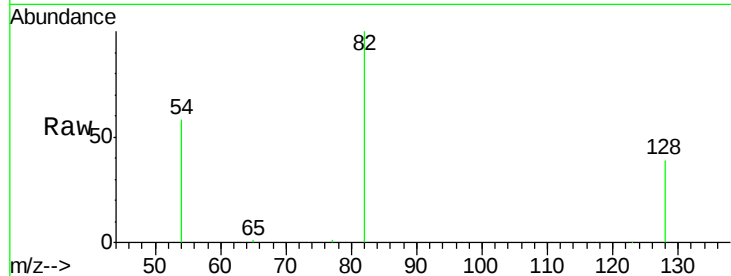

Abundance Ion 82.00 (81.70 to 82.70): BM001328.D (-369) (-)

Ion 128.00 (127.70 to 128.70): BM001328.D (-369) (-)

Ion 54.00 (53.70 to 54.70): BM001328.D (-369) (-)

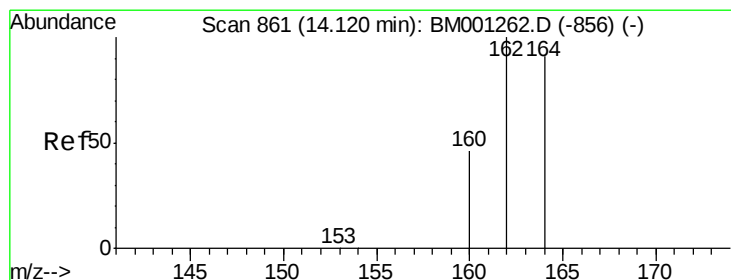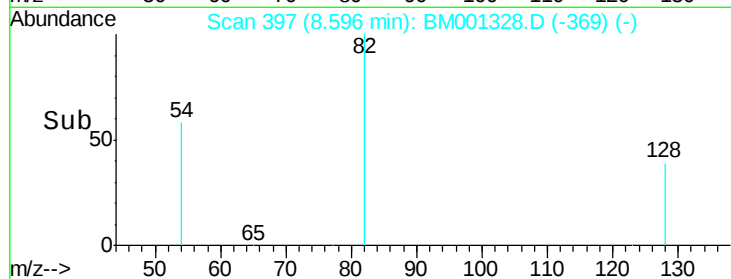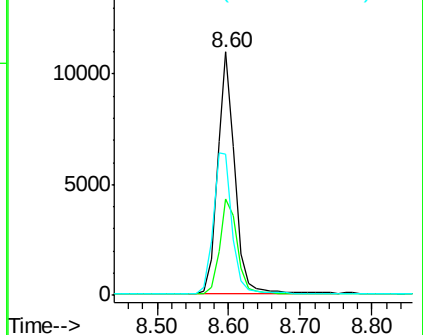

#12

Acenaphthene-d10

Concen: 5.00 ng

RT: 14.12 min Scan# 861

Delta R.T. 0.00 min

Lab File: BM001328.D

Acq: 15 May 2015 15:19


Tgt Ion: 164 Resp: 25198

Ion Ratio Lower Upper

164 100

162 101.1 87.9 131.9



160 43.9 40.9 61.3

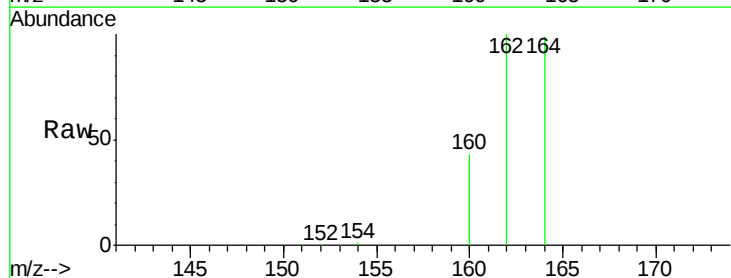


Abundance Ion 164.00 (163.70 to 164.70): BM001328.D (-850) (-)

Ion 162.00 (161.70 to 162.70): BM001328.D (-850) (-)

Ion 160.00 (159.70 to 160.70): BM001328.D (-850) (-)



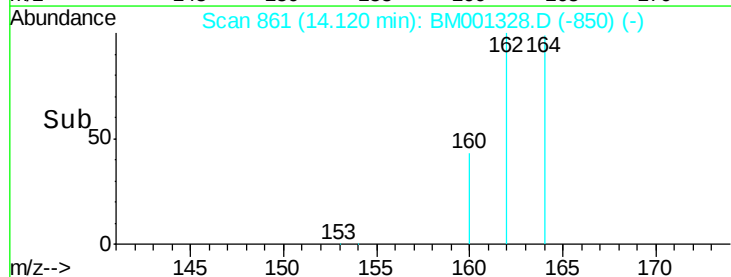
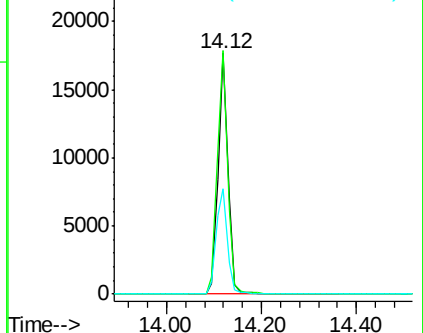


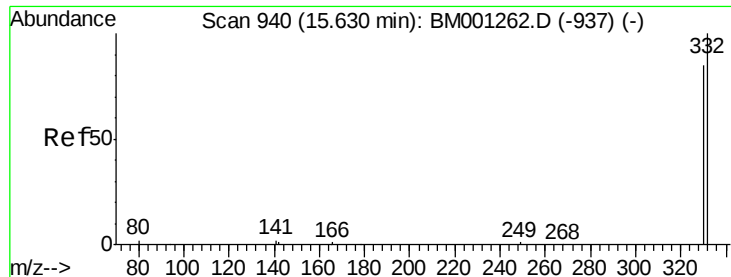

#13
 2,4,6-Tribromophenol
 Concen: 8.53 ng
 RT: 15.63 min Scan# 940
 Delta R.T. 0.03 min
 Lab File: BM001328.D
 Acq: 15 May 2015 15:19




Instrument :
 BNA_M
 ClientSampleId :
 S32-0483


Tgt Ion:330 Resp: 7373
 Ion Ratio Lower Upper
 330 100
 332 104.0 89.0 133.4
 141 0.0 0.0 0.0

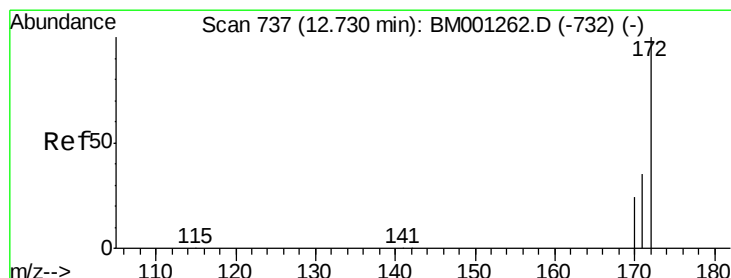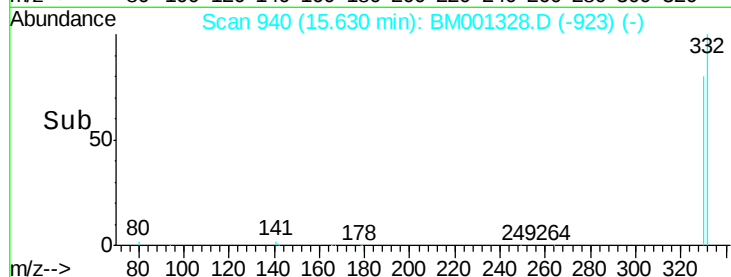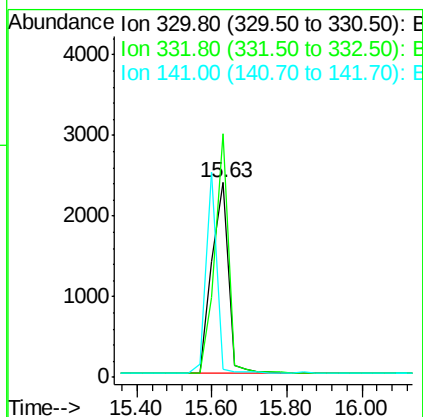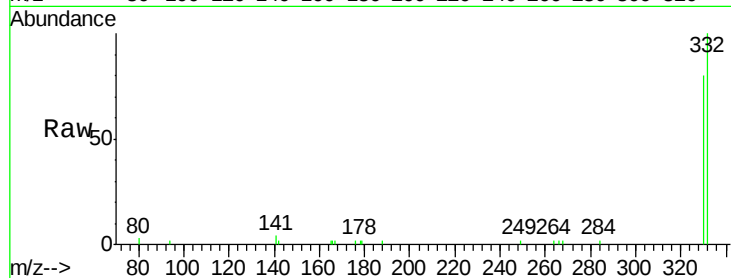

#14
 2-Fluorobiphenyl
 Concen: 7.23 ng
 RT: 12.73 min Scan# 737
 Delta R.T. 0.00 min
 Lab File: BM001328.D
 Acq: 15 May 2015 15:19

Tgt Ion:172 Resp: 56526
 Ion Ratio Lower Upper
 172 100
 171 32.3 28.7 43.1
 170 19.9 19.5 29.3

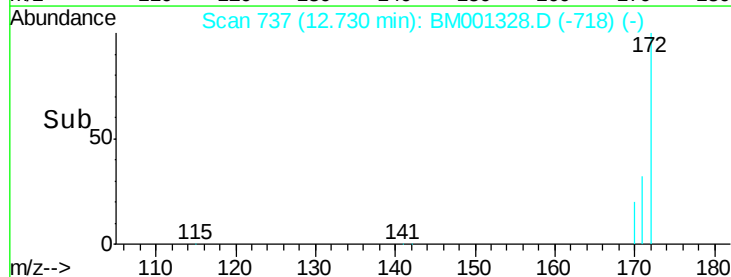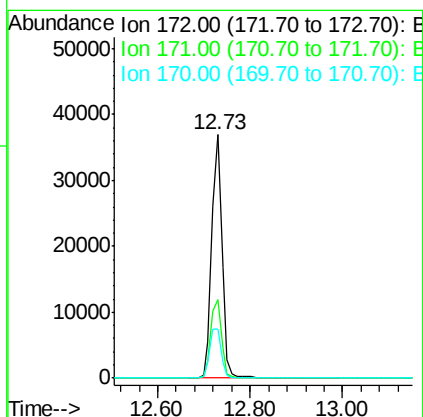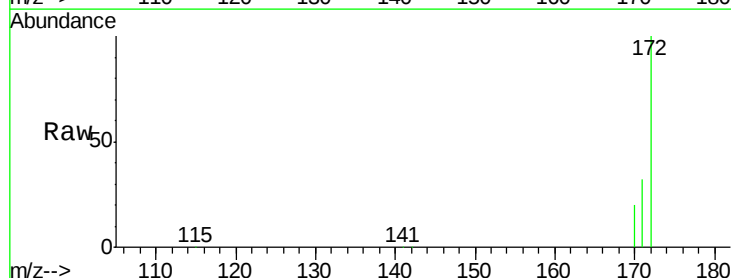

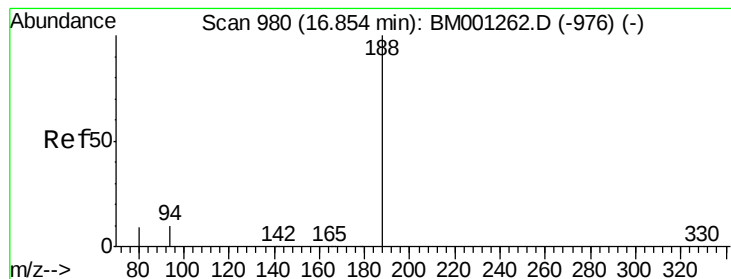

#18

Phenanthrene-d10

Concen: 5.00 ng

RT: 16.85 min Scan# 980

Delta R.T. 0.00 min

Lab File: BM001328.D

Acq: 15 May 2015 15:19

Instrument :

BNA_M

ClientSampleId :

S32-0483


Tgt Ion:188 Resp: 73067

Ion Ratio Lower Upper

188 100

94 4.2 7.8 11.8#




80 3.7 7.5 11.3#

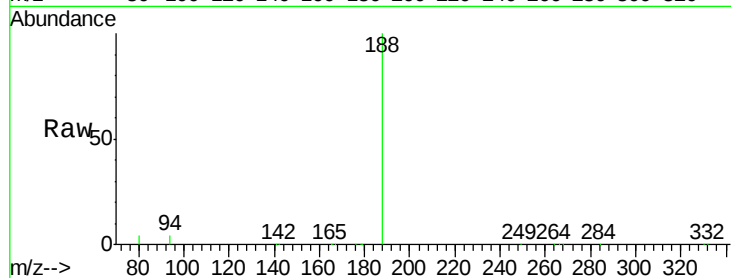

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BM

Ion 80.00 (79.70 to 80.70): BM

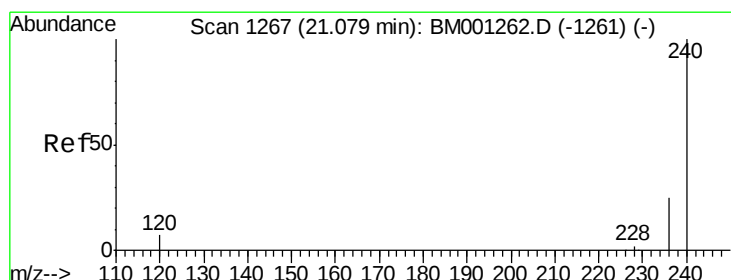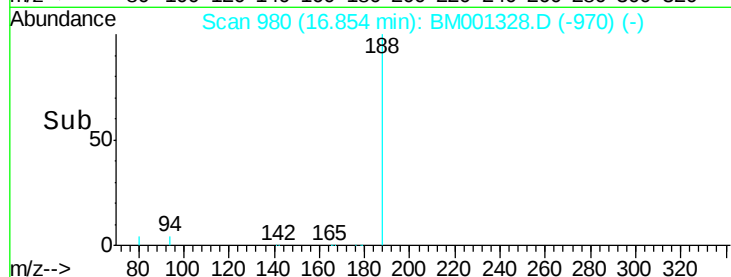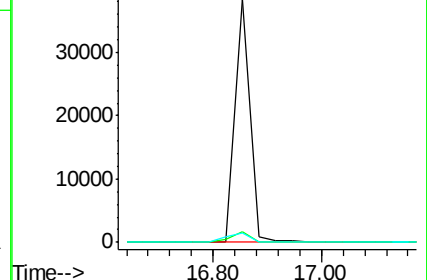

#24

Chrysene-d12

Concen: 5.00 ng

RT: 21.08 min Scan# 1267

Delta R.T. 0.01 min

Lab File: BM001328.D

Acq: 15 May 2015 15:19


Tgt Ion:240 Resp: 47192

Ion Ratio Lower Upper

240 100

120 5.3 5.5 8.3#



236 24.1 20.4 30.6

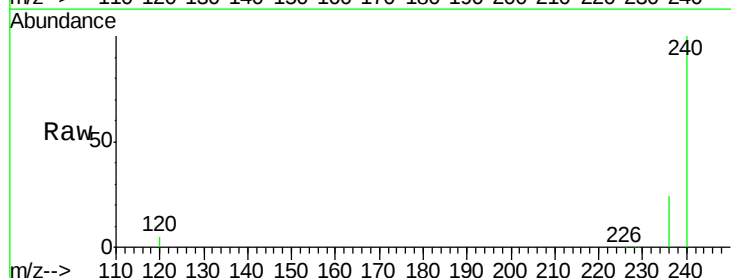


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

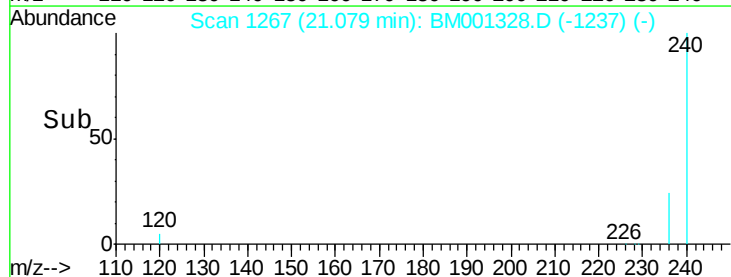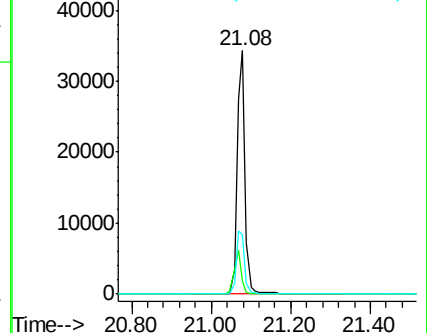

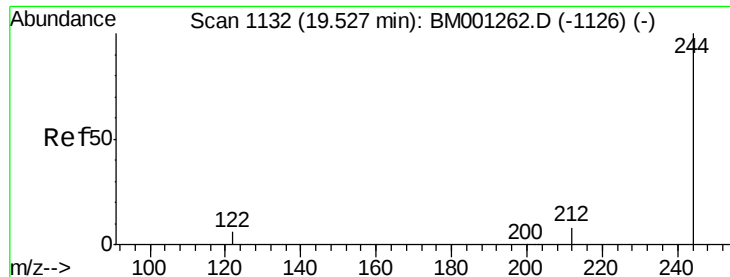

#26

Terphenyl-d14

Concen: 8.53 ng

RT: 19.51 min Scan# 1131

Delta R.T. 0.00 min

Lab File: BM001328.D

Acq: 15 May 2015 15:19

Instrument :

BNA_M

ClientSampleId :

S32-0483


Tgt Ion:244 Resp: 54085

Ion Ratio Lower Upper




244 100

212 10.3 7.2 10.8

122 15.8 5.6 8.4#

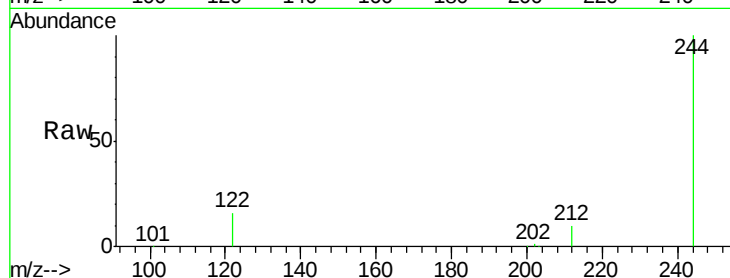

Abundance Ion 244.00 (243.70 to 244.70): E
Ion 212.00 (211.70 to 212.70): E
Ion 122.00 (121.70 to 122.70): E

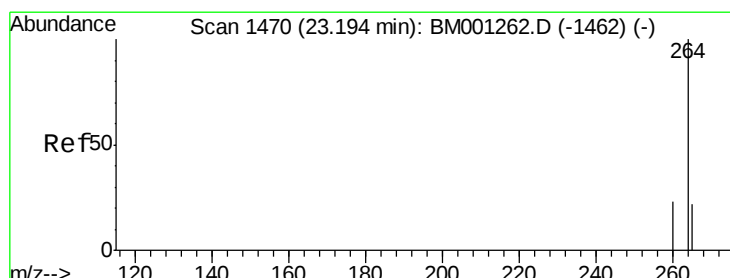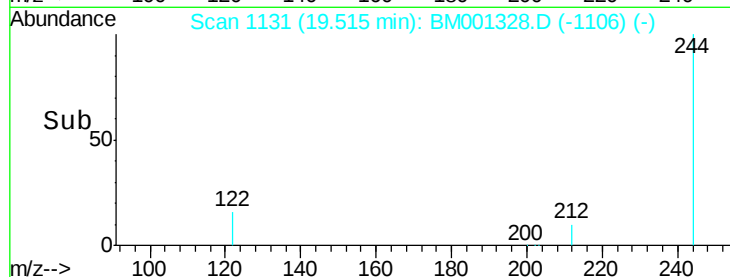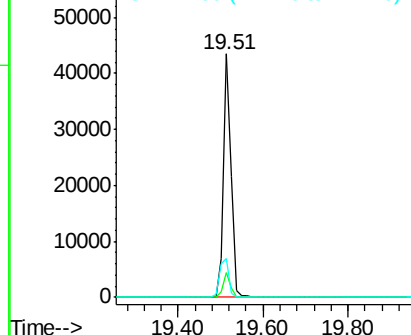

#30

Perylene-d12

Concen: 5.00 ng

RT: 23.18 min Scan# 1469

Delta R.T. 0.00 min

Lab File: BM001328.D

Acq: 15 May 2015 15:19


Tgt Ion:264 Resp: 45502

Ion Ratio Lower Upper

264 100

260 26.1 18.9 28.3

265 21.1 18.1 27.1

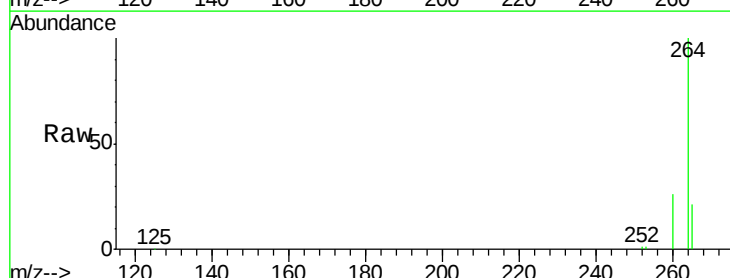

Abundance Ion 264.00 (263.70 to 264.70): E
Ion 260.00 (259.70 to 260.70): E
Ion 265.00 (264.70 to 265.70): E

