


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM051815\
 Data File : BM001330.D
 Acq On : 18 May 2015 12:25
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM031115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Mar 28 05:37:34 2015

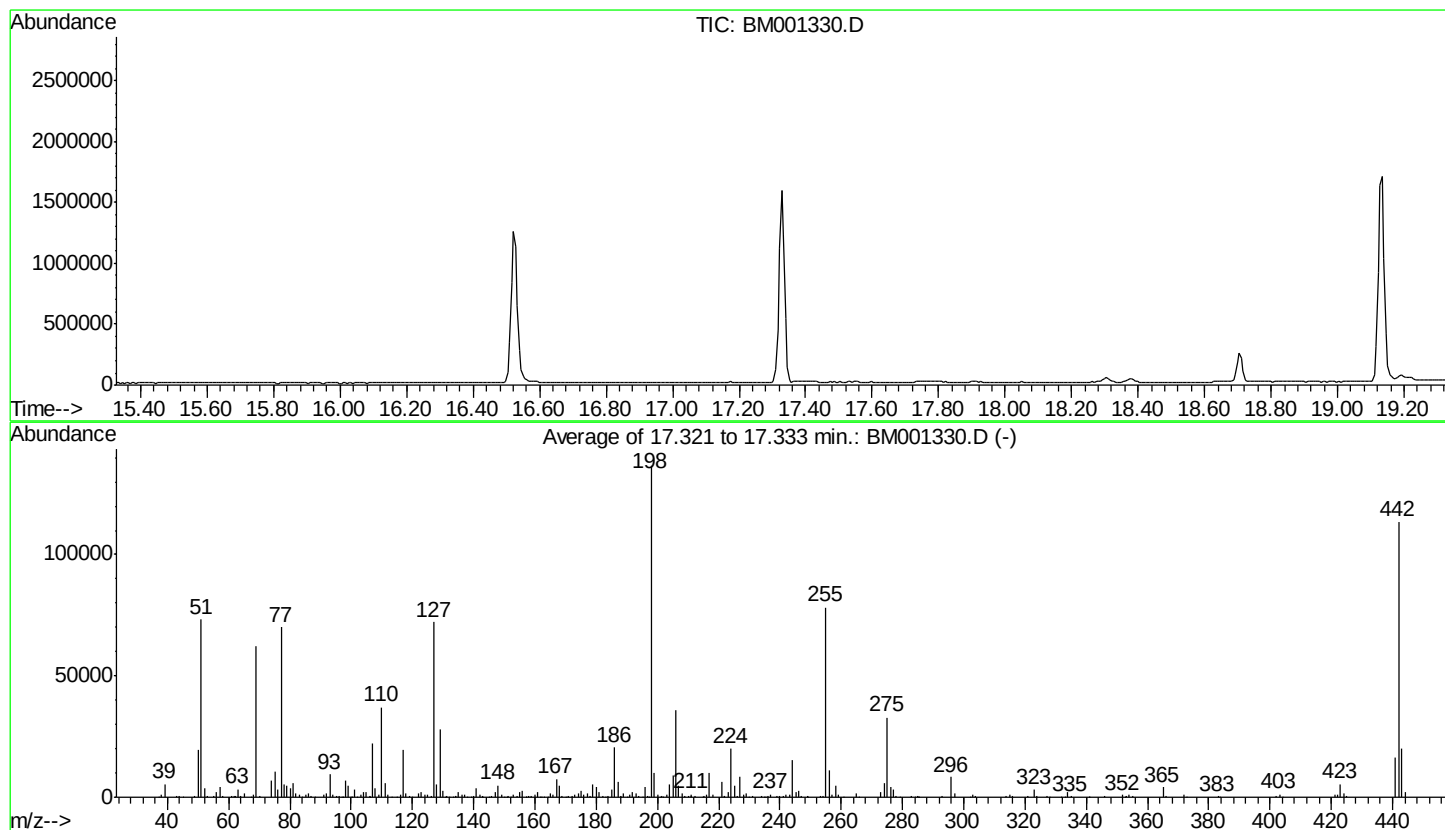

AutoFind: Scans 2488, 2489, 2490; Background Corrected with Scan 2482

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	53.6	73272	PASS
68	69	0.00	2	1.6	979	PASS
69	198	0.00	100	45.6	62288	PASS
70	69	0.00	2	0.9	532	PASS
127	198	10	80	52.8	72178	PASS
197	198	0.00	2	0.3	472	PASS
198	198	100	100	100.0	136674	PASS
199	198	5	9	7.3	10031	PASS
275	198	10	60	24.1	32909	PASS
365	198	1	100	3.0	4059	PASS
441	442	0.01	24	14.6	16566	PASS
442	198	50	100	83.1	113546	PASS
443	442	15	24	17.8	20218	PASS