

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM051816\
 Data File : BM005476.D
 Acq On : 18 May 2016 19:07
 Operator : UM/SJ
 Sample : H2844-04
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AC0

Quant Time: May 19 01:44:56 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM051816.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed May 18 14:47:27 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.84	152	34397	20.00	ng/ul	0.00
18) Naphthalene-d8	10.63	136	165438	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.47	164	109041	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.20	188	289033	20.00	ng/ul	0.00
75) Chrysene-d12	21.38	240	461098	20.00	ng/ul	0.00
83) Perylene-d12	23.67	264	553474	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.32	96	1026	1.15	ng/uL	0.00
5) Phenol-d5	6.99	99	21790	6.59	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.17	67	63515	35.10	ng/ul	0.00
9) 2-Chlorophenol-d4	7.37	132	64623	25.46	ng/ul	0.00
13) 4-Methylphenol-d8	8.53	113	42482	15.09	ng/ul	0.00
19) Nitrobenzene-d5	8.99	128	40814	34.27	ng/ul	0.00
22) 2-Nitrophenol-d4	9.71	143	43519	33.50	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.25	165	79218	30.68	ng/ul	0.00
29) 4-Chloroaniline-d4	0.00	131	0	0.00	ng/ul	0.00
43) Dimethylphthalate-d6	13.87	166	332715	37.12	ng/ul	0.00
46) Acenaphthylene-d8	14.16	160	388830	36.74	ng/ul	0.00
51) 4-Nitrophenol-d4	14.64	143	11066	6.02	ng/ul	0.00
57) Fluorene-d10	15.46	176	301005	38.05	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.57	200	44774	29.39	ng/ul	0.00
70) Anthracene-d10	17.30	188	506247	38.08	ng/ul	0.00
76) Pyrene-d10	19.59	212	660055	35.60	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.52	264	958639	38.74	ng/ul	0.00

Target Compounds


						Qvalue
15) N-Nitroso-di-n-propylamine	8.53	70	913	0.38	ng/ul#	1
21) Isophorone	9.71	82	3849	0.63	ng/ul#	67
28) Naphthalene	10.68	128	384	0.05	ng/ul#	69
45) 2,6-Dinitrotoluene	13.88	165	1667	0.95	ng/ul#	30
56) Diethylphthalate	15.29	149	351	0.04	ng/ul#	59
58) Fluorene	15.46	166	586	0.06	ng/ul#	9
73) Di-n-butylphthalate	18.17	149	797	0.04	ng/ul#	78
74) Fluoranthene	19.26	202	539	0.03	ng/ul#	72
77) Pyrene	19.62	202	408	0.02	ng/ul#	69
78) Butylbenzylphthalate	20.69	149	122	0.01	ng/ul#	22
80) Benzo(a)anthracene	21.38	228	1391	0.05	ng/ul#	52
81) Bis(2-ethylhexyl)phthalate	21.31	149	1682	0.11	ng/ul#	52
82) Chrysene	21.42	228	564	0.02	ng/ul#	50
84) Di-n-octyl phthalate	22.20	149	107	0.00	ng/ul#	1
85) Benzo(b)fluoranthene	22.98	252	234	0.01	ng/ul#	60
86) Benzo(k)fluoranthene	22.99	252	106	0.00	ng/ul#	1
88) Benzo(a)pyrene	23.56	252	266	0.01	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM051816\
Data File : BM005476.D
Acq On : 18 May 2016 19:07
Operator : UM/SJ
Sample : H2844-04
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AC0

Quant Time: May 19 01:44:56 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM051816.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed May 18 14:47:27 2016
Response via : Initial Calibration




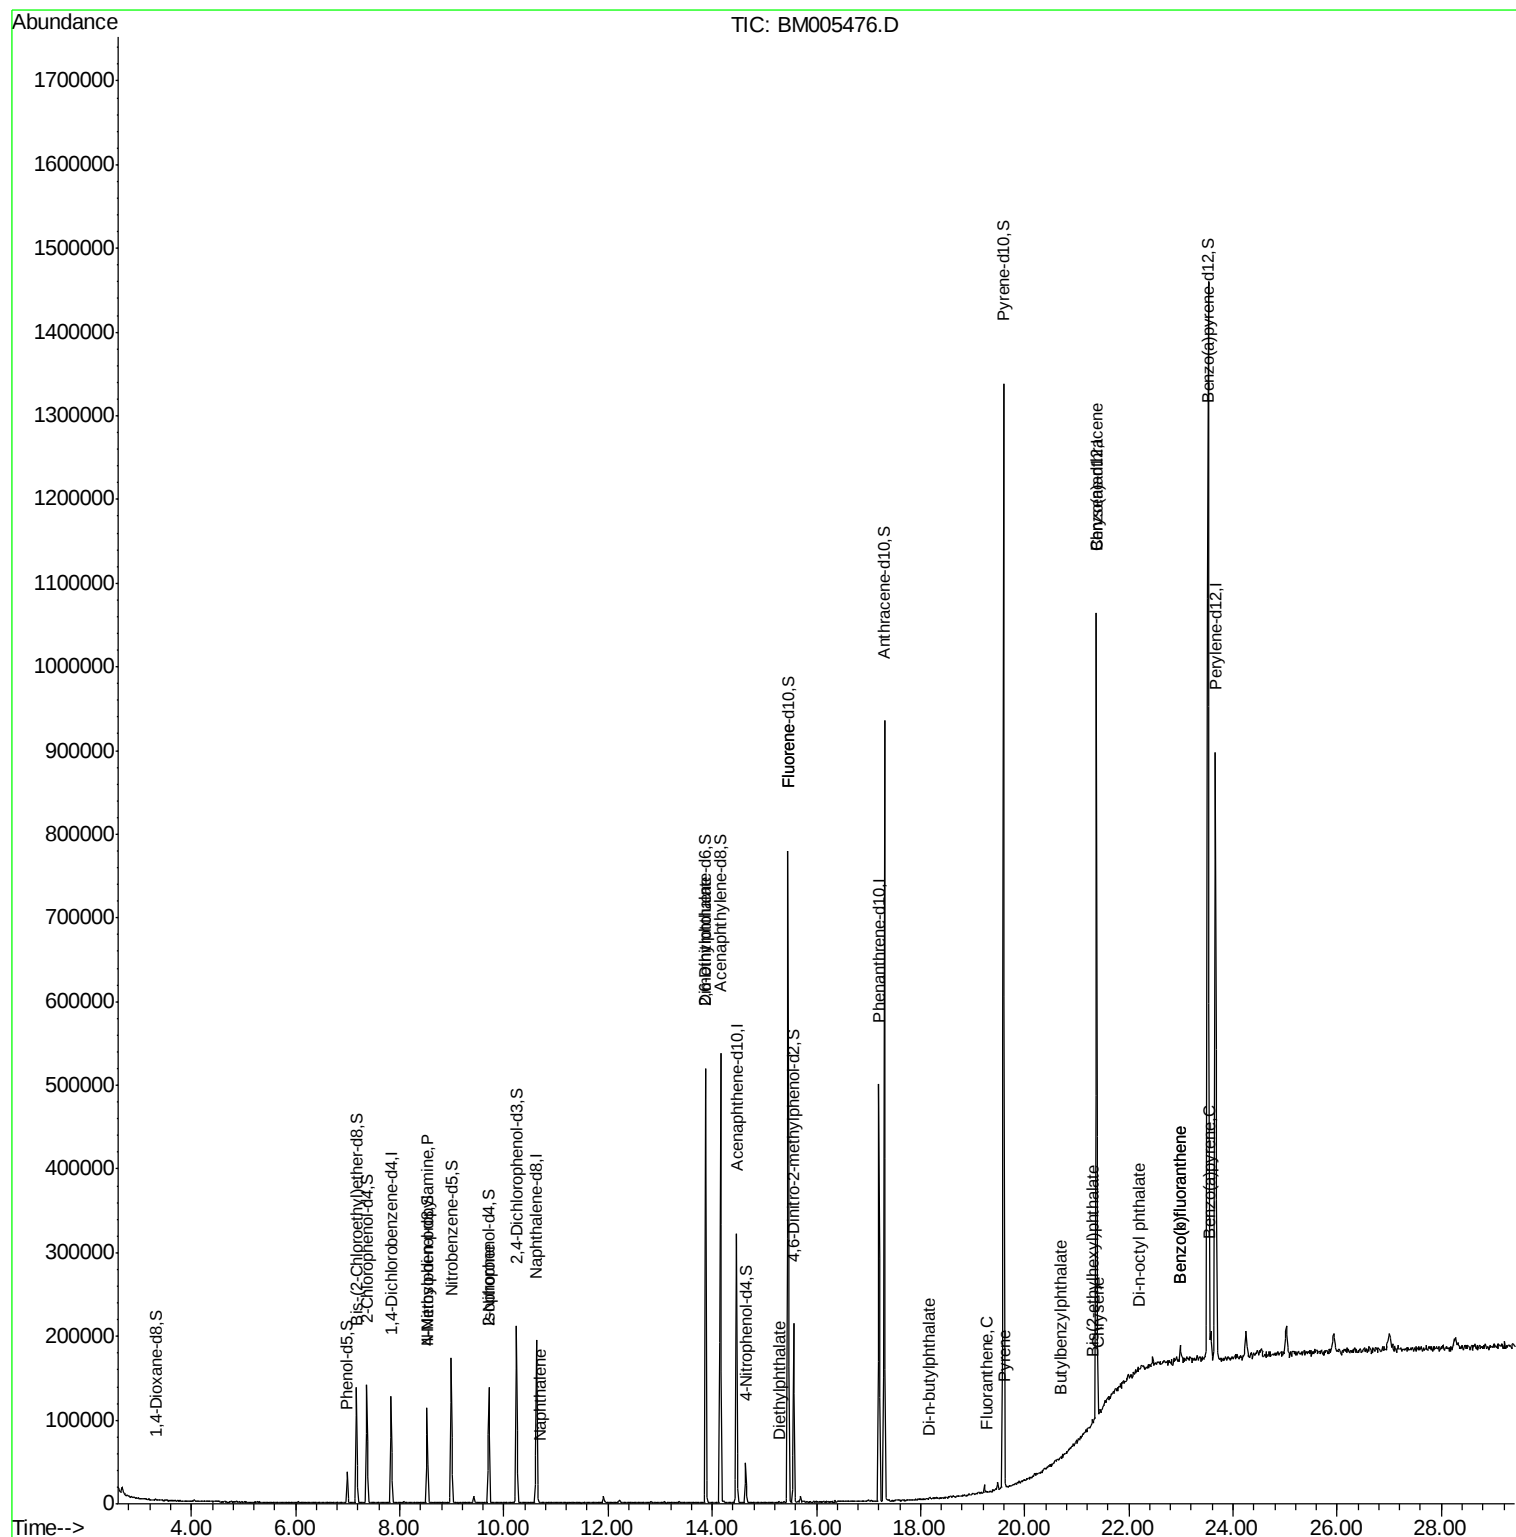




#15
N-Nitroso-di-n-propylamine
Concen: 0.38 ng/ul
RT: 8.53 min Scan# 1010
Delta R.T. -0.11 min
Lab File: BM005476.D
Acq: 18 May 2016 19:07




Instrument :
BNA_M
ClientSampleId :
C0AC0


Tgt Ion: 70 Resp: 913
Ion Ratio Lower Upper
70 100
42 393.5 42.8 64.2#
101 0.0 7.8 11.6#
130 0.0 15.7 23.5#

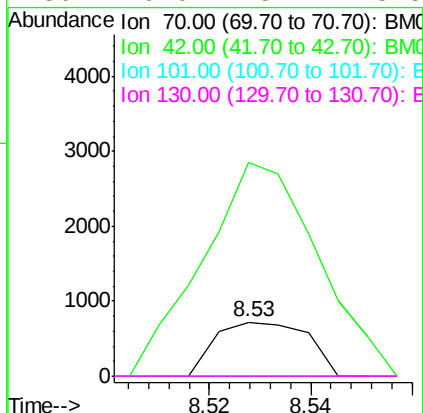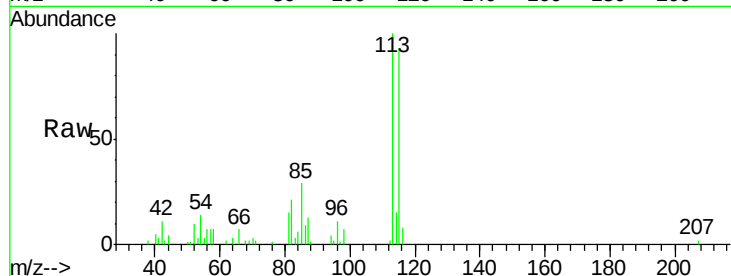

#21
Isophorone
Concen: 0.63 ng/ul
RT: 9.71 min Scan# 1211
Delta R.T. 0.15 min
Lab File: BM005476.D
Acq: 18 May 2016 19:07

Tgt Ion: 82 Resp: 3849
Ion Ratio Lower Upper
82 100
95 0.0 5.4 8.0#
138 0.0 13.4 20.2#

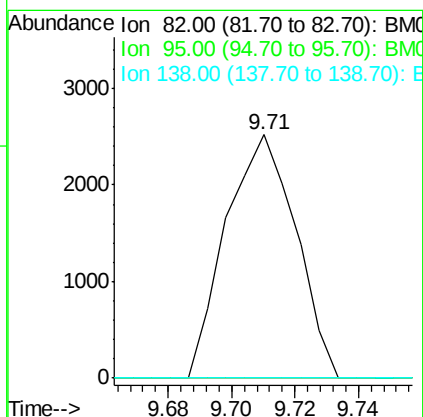

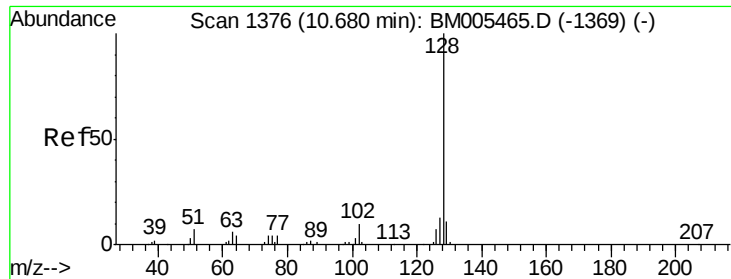

#28

Naphthalene

Concen: 0.05 ng/ul

RT: 10.68 min Scan# 1376

Delta R.T. 0.00 min

Lab File: BM005476.D

Acq: 18 May 2016 19:07

Instrument :

BNA_M

ClientSampleId :

C0AC0


Tgt Ion:128 Resp: 384

Ion Ratio Lower Upper

128 100

129 0.0 8.4 12.6#




127 0.0 10.8 16.2#

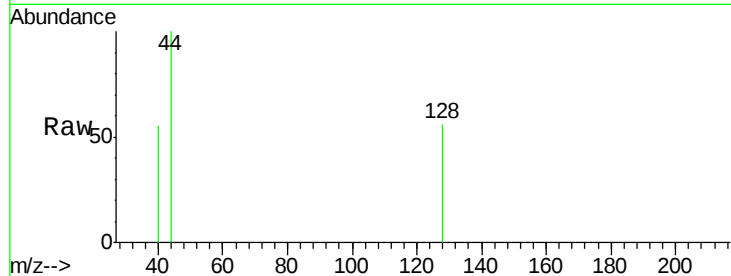

Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

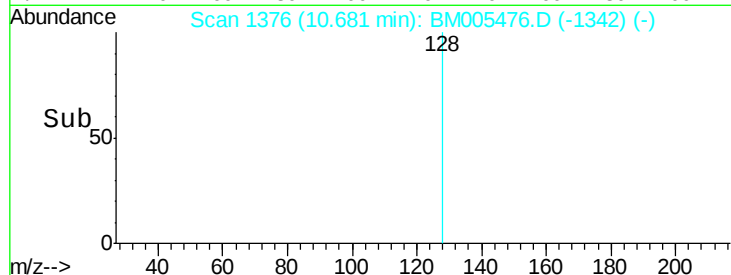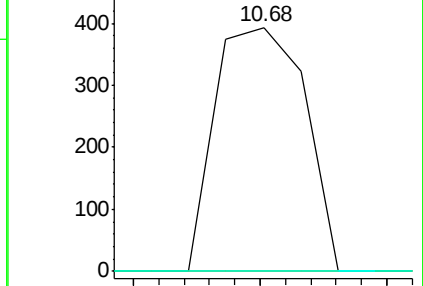

#45

2,6-Dinitrotoluene

Concen: 0.95 ng/ul

RT: 13.88 min Scan# 1920

Delta R.T. -0.16 min

Lab File: BM005476.D

Acq: 18 May 2016 19:07


Tgt Ion:165 Resp: 1667

Ion Ratio Lower Upper

165 100

89 0.0 52.2 78.4#



121 45.4 21.0 31.4#




Abundance Ion 165.00 (164.70 to 165.70): E

Ion 89.00 (88.70 to 89.70): BM

Ion 121.00 (120.70 to 121.70): E




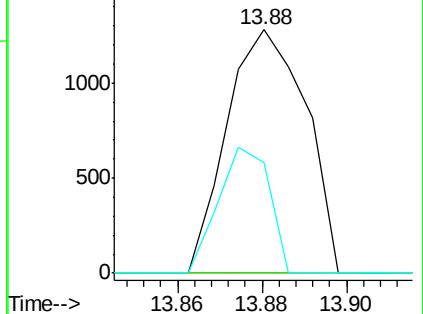


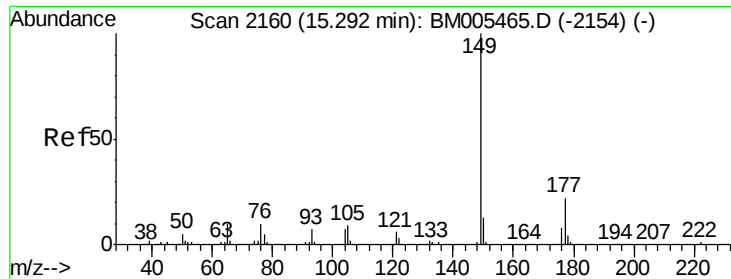

#56
Diethylphthalate
Concen: 0.04 ng/ul
RT: 15.29 min Scan# 2159
Delta R.T. -0.01 min
Lab File: BM005476.D
Acq: 18 May 2016 19:07




Instrument :
BNA_M
ClientSampleId :
C0AC0


Tgt Ion:149 Resp: 351
Ion Ratio Lower Upper
149 100
177 0.0 17.6 26.4#
150 0.0 9.8 14.8#

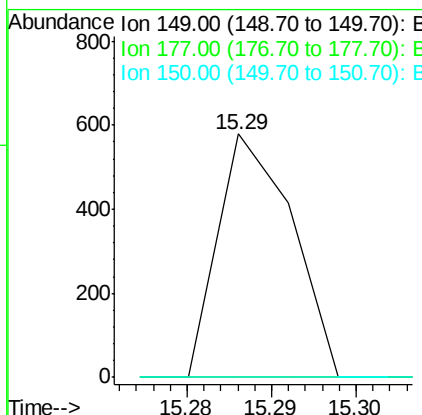

#58
Fluorene
Concen: 0.06 ng/ul
RT: 15.46 min Scan# 2188
Delta R.T. -0.06 min
Lab File: BM005476.D
Acq: 18 May 2016 19:07

Tgt Ion:166 Resp: 586
Ion Ratio Lower Upper
166 100
165 0.0 77.9 116.9#
167 0.0 10.6 16.0#

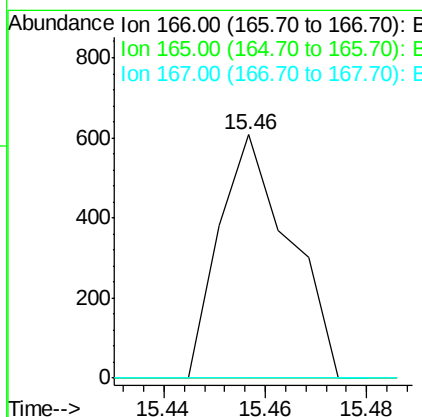

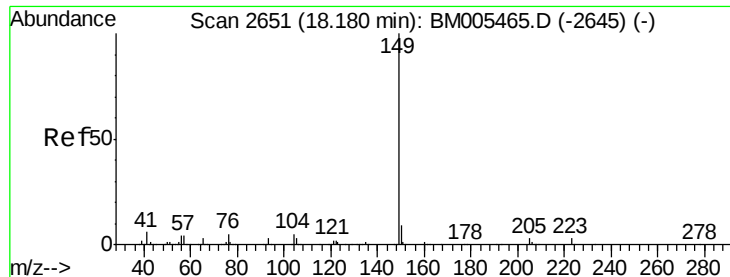

#73

Di-n-butylphthalate

Concen: 0.04 ng/ul

RT: 18.17 min Scan# 2650

Delta R.T. -0.01 min

Lab File: BM005476.D

Acq: 18 May 2016 19:07

Instrument :

BNA_M

ClientSampleId :

C0AC0


Tgt Ion:149 Resp: 797

Ion Ratio Lower Upper

149 100

150 0.0 7.3 10.9#




104 0.0 4.1 6.1#

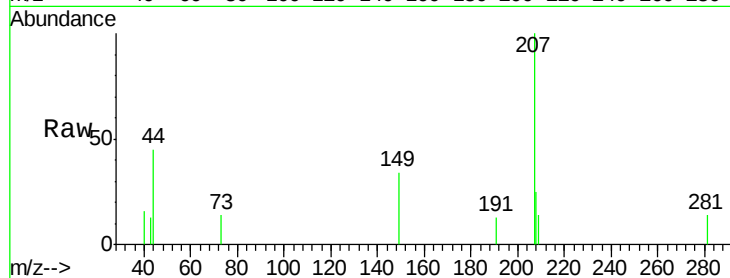

Abundance Ion 149.00 (148.70 to 149.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 104.00 (103.70 to 104.70): E

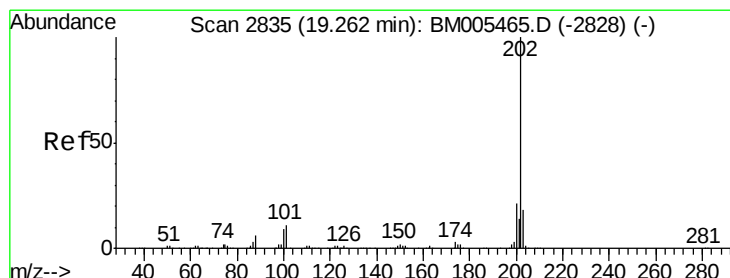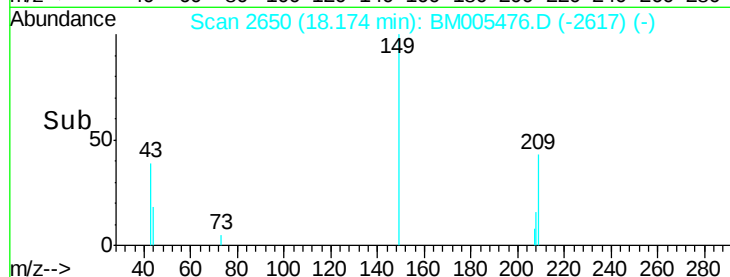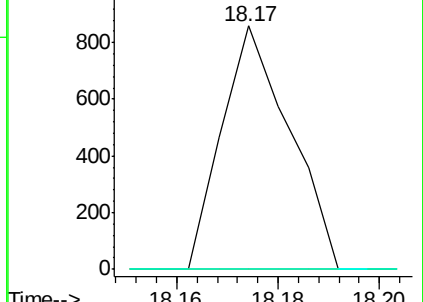

#74

Fluoranthene

Concen: 0.03 ng/ul

RT: 19.26 min Scan# 2834

Delta R.T. -0.01 min

Lab File: BM005476.D

Acq: 18 May 2016 19:07


Tgt Ion:202 Resp: 539

Ion Ratio Lower Upper

202 100

101 0.0 9.2 13.8#



100 0.0 7.1 10.7#

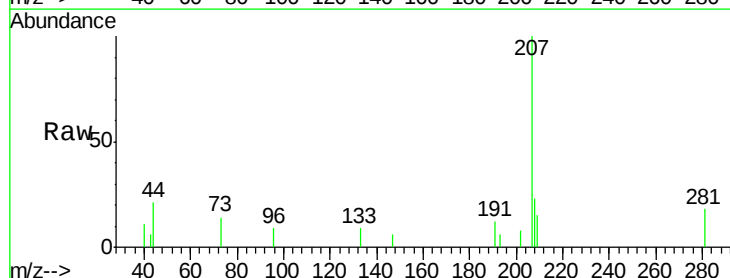


Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): E

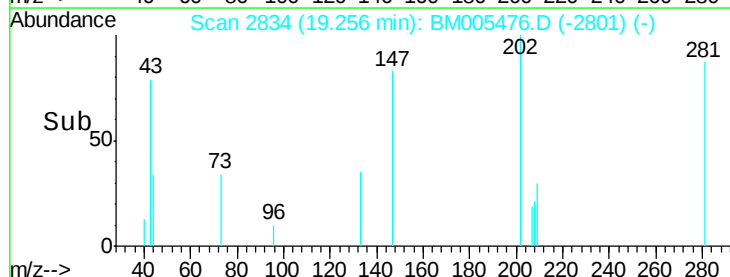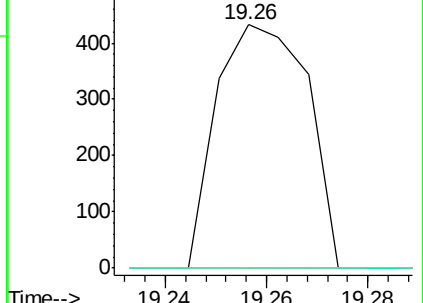



#77

Pyrene

Concen: 0.02 ng/ul

RT: 19.62 min Scan# 2896

Delta R.T. 0.00 min

Lab File: BM005476.D

Acq: 18 May 2016 19:07

Instrument :

BNA_M

ClientSampleId :

C0AC0


Tgt Ion:202 Resp: 408

Ion Ratio Lower Upper

202 100

101 0.0 10.8 16.2#




100 0.0 8.4 12.6#



Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

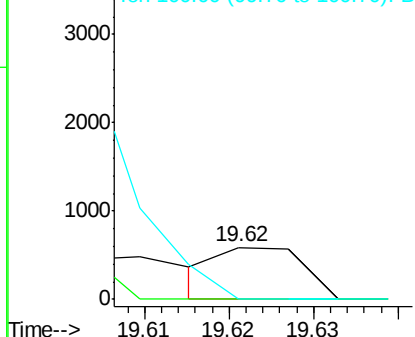

#78

Butylbenzylphthalate

Concen: 0.01 ng/ul

RT: 20.69 min Scan# 3077

Delta R.T. 0.16 min

Lab File: BM005476.D

Acq: 18 May 2016 19:07


Tgt Ion:149 Resp: 122

Ion Ratio Lower Upper

149 100

91 0.0 58.4 87.6#



206 0.0 17.3 25.9#




Abundance Ion 149.00 (148.70 to 149.70): E

Ion 91.00 (90.70 to 91.70): B

Ion 206.00 (205.70 to 206.70): E

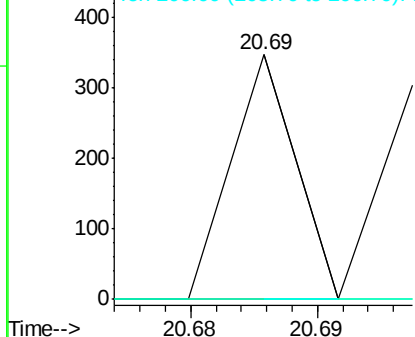



#80

Benzo(a)anthracene

Concen: 0.05 ng/ul

RT: 21.38 min Scan# 3195

Delta R.T. 0.01 min

Lab File: BM005476.D

Acq: 18 May 2016 19:07

Instrument :

BNA_M

ClientSampleId :

C0AC0


Tgt Ion:228 Resp: 1391

Ion Ratio Lower Upper

228 100

229 0.0 15.5 23.3#




226 0.0 21.8 32.8#

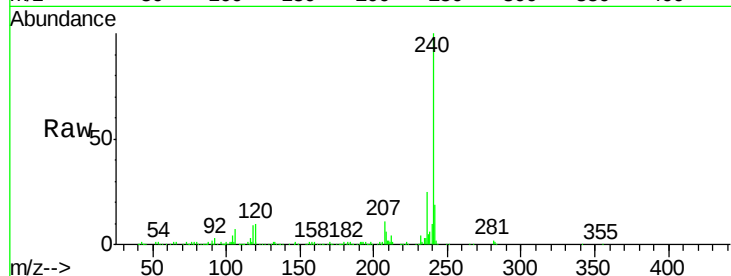

Abundance Ion 228.00 (227.70 to 228.70): E

Ion 229.00 (228.70 to 229.70): E

Ion 226.00 (225.70 to 226.70): E

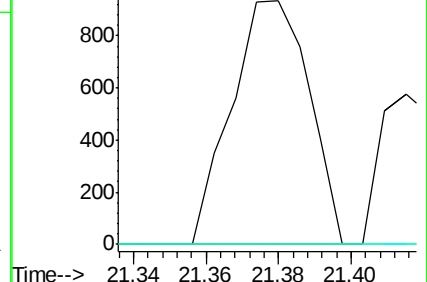

#81

Bis(2-ethylhexyl)phthalate

Concen: 0.11 ng/ul

RT: 21.31 min Scan# 3183

Delta R.T. 0.00 min

Lab File: BM005476.D

Acq: 18 May 2016 19:07


Tgt Ion:149 Resp: 1682

Ion Ratio Lower Upper

149 100

167 0.0 21.9 32.9#



279 0.0 3.0 4.4#




Abundance Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E

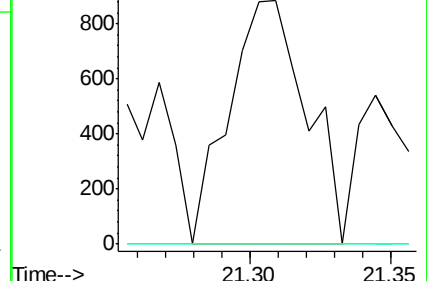







#82
Chrysene
Concen: 0.02 ng/ul
RT: 21.42 min Scan# 3201
Delta R.T. -0.01 min
Lab File: BM005476.D
Acq: 18 May 2016 19:07

Instrument :
BNA_M
ClientSampleId :
C0AC0

Tgt Ion: 228 Resp: 564
Ion Ratio Lower Upper
228 100
226 0.0 23.6 35.4#
229 0.0 15.4 23.0#




Abundance Ion 228.00 (227.70 to 228.70): E
Ion 226.00 (225.70 to 226.70): E
Ion 229.00 (228.70 to 229.70): E

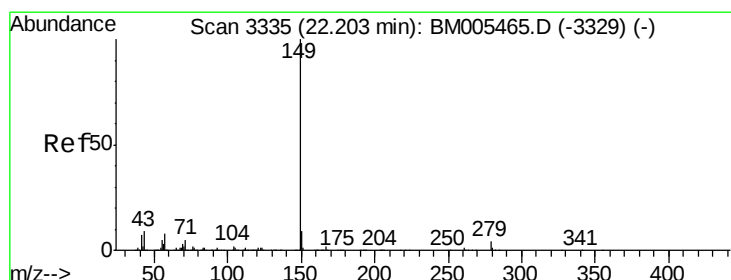
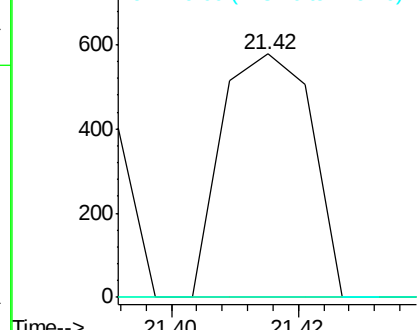



#84
Di-n-octyl phthalate
Concen: 0.00 ng/ul
RT: 22.20 min Scan# 3334
Delta R.T. -0.01 min
Lab File: BM005476.D
Acq: 18 May 2016 19:07

Tgt Ion: 149 Resp: 107
Ion Ratio Lower Upper
149 100
167 0.0 1.3 1.9#
43 79.4 7.4 11.0#



Abundance Ion 149.00 (148.70 to 149.70): E
Ion 167.00 (166.70 to 167.70): E
Ion 43.00 (42.70 to 43.70): BM0

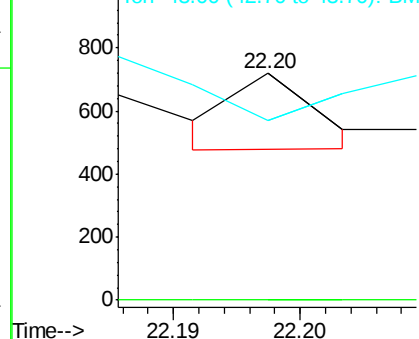



#85

Benzo(b)fluoranthene

Concen: 0.01 ng/ul

RT: 22.98 min Scan# 3467

Delta R.T. 0.00 min

Lab File: BM005476.D

Acq: 18 May 2016 19:07

Instrument :

BNA_M

ClientSampleId :

C0AC0


Tgt Ion:252 Resp: 234

Ion Ratio Lower Upper

252 100

253 0.0 17.4 26.2#




125 0.0 8.4 12.6#

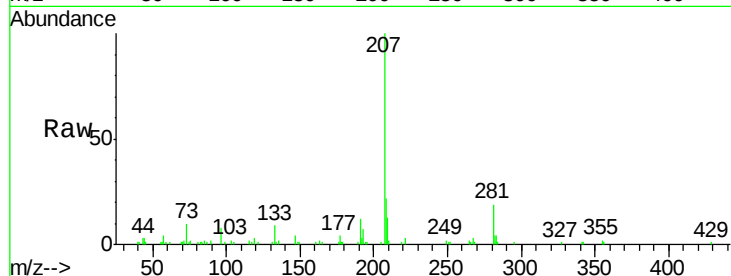

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

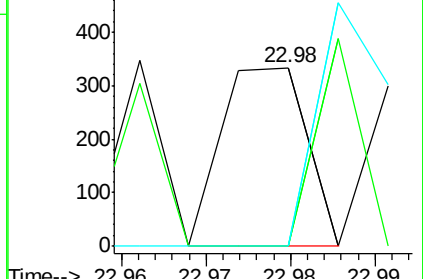

#86

Benzo(k)fluoranthene

Concen: 0.00 ng/ul

RT: 22.99 min Scan# 3469

Delta R.T. -0.04 min

Lab File: BM005476.D

Acq: 18 May 2016 19:07


Tgt Ion:252 Resp: 106

Ion Ratio Lower Upper

252 100

253 0.0 17.3 25.9#



125 101.0 8.0 12.0#




Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

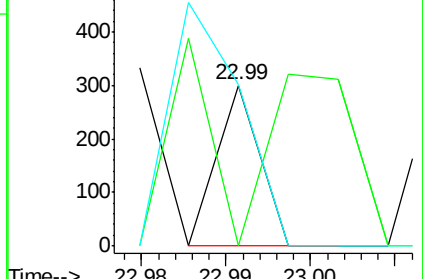

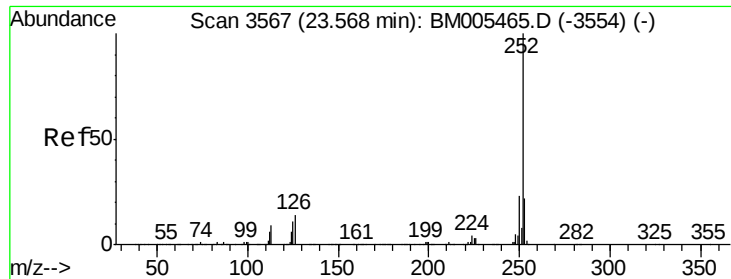

#88

Benzo(a)pyrene

Concen: 0.01 ng/ul

RT: 23.56 min Scan# 3565

Delta R.T. -0.01 min

Lab File: BM005476.D


Acq: 18 May 2016 19:07

Instrument :

BNA_M

ClientSampleId :

C0AC0



Tgt Ion:	252	Resp:	266
Ion	Ratio	Lower	Upper
252	100		
253	84.5	17.5	26.3#
125	81.4	8.7	13.1#

