

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM051816\
 Data File : BM005478.D
 Acq On : 18 May 2016 20:19
 Operator : UM/SJ
 Sample : H2841-11
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9WS6

Quant Time: May 19 01:45:20 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM051816.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed May 18 14:47:27 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.84	152	21377	20.00	ng/ul	0.00
18) Naphthalene-d8	10.63	136	105951	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.47	164	71903	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.20	188	199456	20.00	ng/ul	0.00
75) Chrysene-d12	21.38	240	354627	20.00	ng/ul	0.00
83) Perylene-d12	23.66	264	454696	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.32	96	1557	2.80	ng/uL	0.00
5) Phenol-d5	6.99	99	41024	19.98	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.17	67	24894	22.13	ng/ul	0.00
9) 2-Chlorophenol-d4	7.37	132	32261	20.45	ng/ul	0.00
13) 4-Methylphenol-d8	8.53	113	30430	17.40	ng/ul	0.00
19) Nitrobenzene-d5	8.99	128	15343	20.11	ng/ul	0.00
22) 2-Nitrophenol-d4	9.71	143	16376	19.68	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.24	165	34312	20.75	ng/ul	0.00
29) 4-Chloroaniline-d4	10.76	131	31509	16.57	ng/ul	0.00
43) Dimethylphthalate-d6	13.87	166	135430	22.91	ng/ul	0.00
46) Acenaphthylene-d8	14.16	160	159561	22.86	ng/ul	0.00
51) 4-Nitrophenol-d4	14.64	143	24408	20.13	ng/ul	0.00
57) Fluorene-d10	15.46	176	127993	24.54	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.56	200	16216	15.42	ng/ul	0.00
70) Anthracene-d10	17.30	188	217147	23.67	ng/ul	0.00
76) Pyrene-d10	19.59	212	311050	21.81	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.51	264	498510	24.52	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
44) Dimethylphthalate	13.92	163	28588	4.74	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM051816\
Data File : BM005478.D
Acq On : 18 May 2016 20:19
Operator : UM/SJ
Sample : H2841-11
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
D9WS6

Quant Time: May 19 01:45:20 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM051816.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed May 18 14:47:27 2016
Response via : Initial Calibration

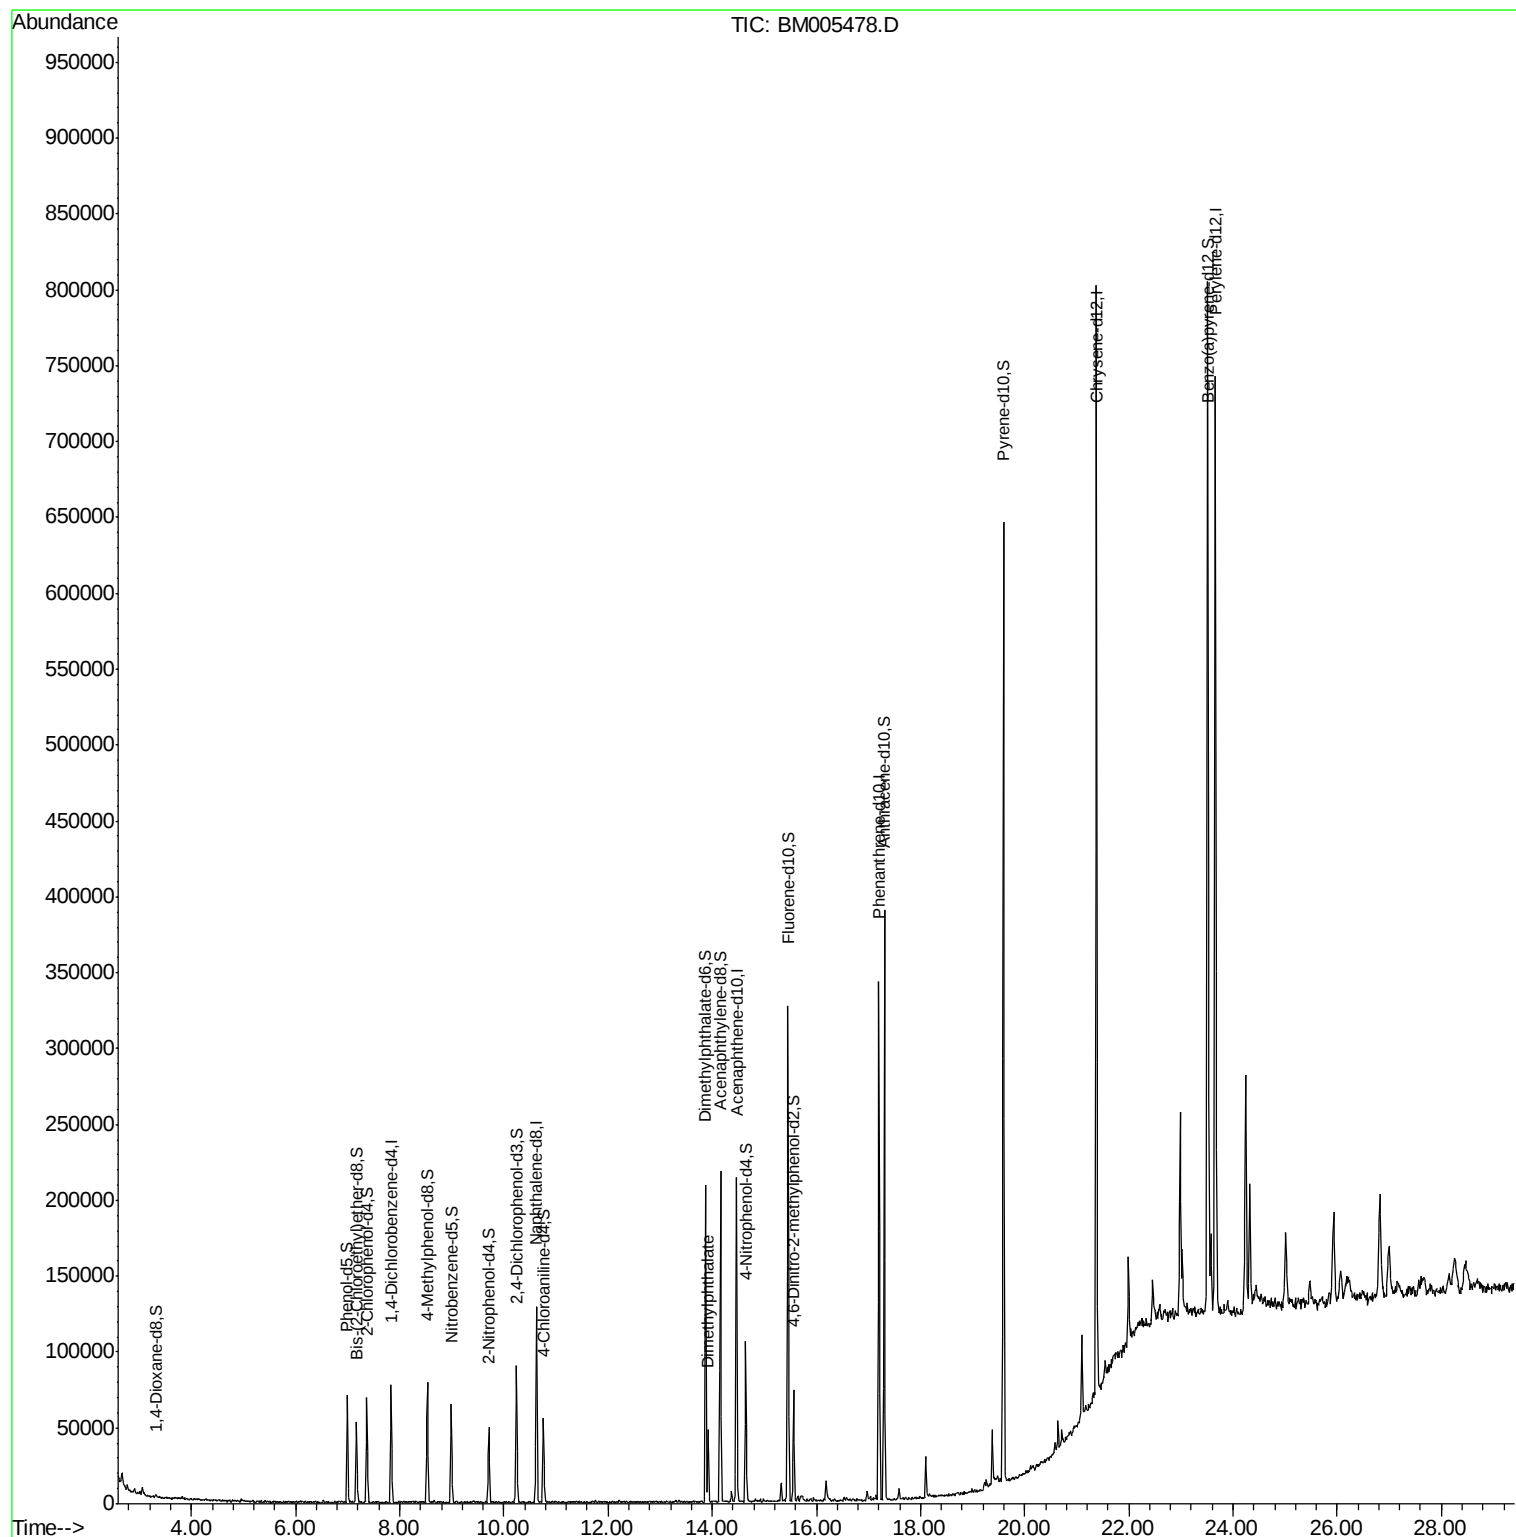

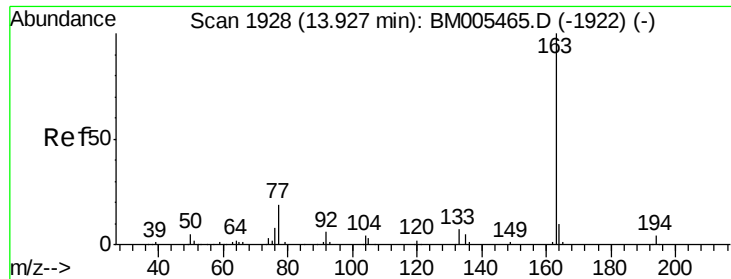

#44
 Dimethylphthalate
 Concen: 4.74 ng/ul
 RT: 13.92 min Scan# 1927
 Delta R.T. -0.01 min
 Lab File: BM005478.D
 Acq: 18 May 2016 20:19

Instrument :
 BNA_M
 ClientSampleId :
 D9WS6

Tgt Ion	Ratio	Lower	Upper
163	100		
194	3.7	3.4	5.0
164	9.6	7.9	11.9

