

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM051816\
 Data File : BM005480.D
 Acq On : 18 May 2016 21:32
 Operator : UM/SJ
 Sample : H2841-13
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9WS8

Quant Time: May 19 01:45:45 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM051816.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed May 18 14:47:27 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.84	152	31900	20.00	ng/ul	0.00
18) Naphthalene-d8	10.63	136	156957	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.46	164	109267	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.20	188	298810	20.00	ng/ul	0.00
75) Chrysene-d12	21.37	240	494934	20.00	ng/ul	-0.01
83) Perylene-d12	23.66	264	594584	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.32	96	2887	3.48	ng/uL	0.00
5) Phenol-d5	6.99	99	75881	24.76	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.17	67	46589	27.76	ng/ul	0.00
9) 2-Chlorophenol-d4	7.37	132	59224	25.16	ng/ul	0.00
13) 4-Methylphenol-d8	8.53	113	66093	25.32	ng/ul	0.00
19) Nitrobenzene-d5	8.99	128	30039	26.58	ng/ul	0.00
22) 2-Nitrophenol-d4	9.71	143	31786	25.79	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.24	165	64805	26.45	ng/ul	0.00
29) 4-Chloroaniline-d4	10.76	131	81426	28.90	ng/ul	0.00
43) Dimethylphthalate-d6	13.87	166	271915	30.27	ng/ul	0.00
46) Acenaphthylene-d8	14.16	160	310442	29.27	ng/ul	0.00
51) 4-Nitrophenol-d4	14.64	143	47531	25.79	ng/ul	0.00
57) Fluorene-d10	15.46	176	245282	30.95	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.56	200	31488	19.99	ng/ul	0.00
70) Anthracene-d10	17.30	188	429541	31.25	ng/ul	0.00
76) Pyrene-d10	19.59	212	591517	29.72	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.52	264	868910	32.69	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
44) Dimethylphthalate	13.92	163	74877	8.18	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM051816\
Data File : BM005480.D
Acq On : 18 May 2016 21:32
Operator : UM/SJ
Sample : H2841-13
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
D9WS8

Quant Time: May 19 01:45:45 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM051816.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed May 18 14:47:27 2016
Response via : Initial Calibration

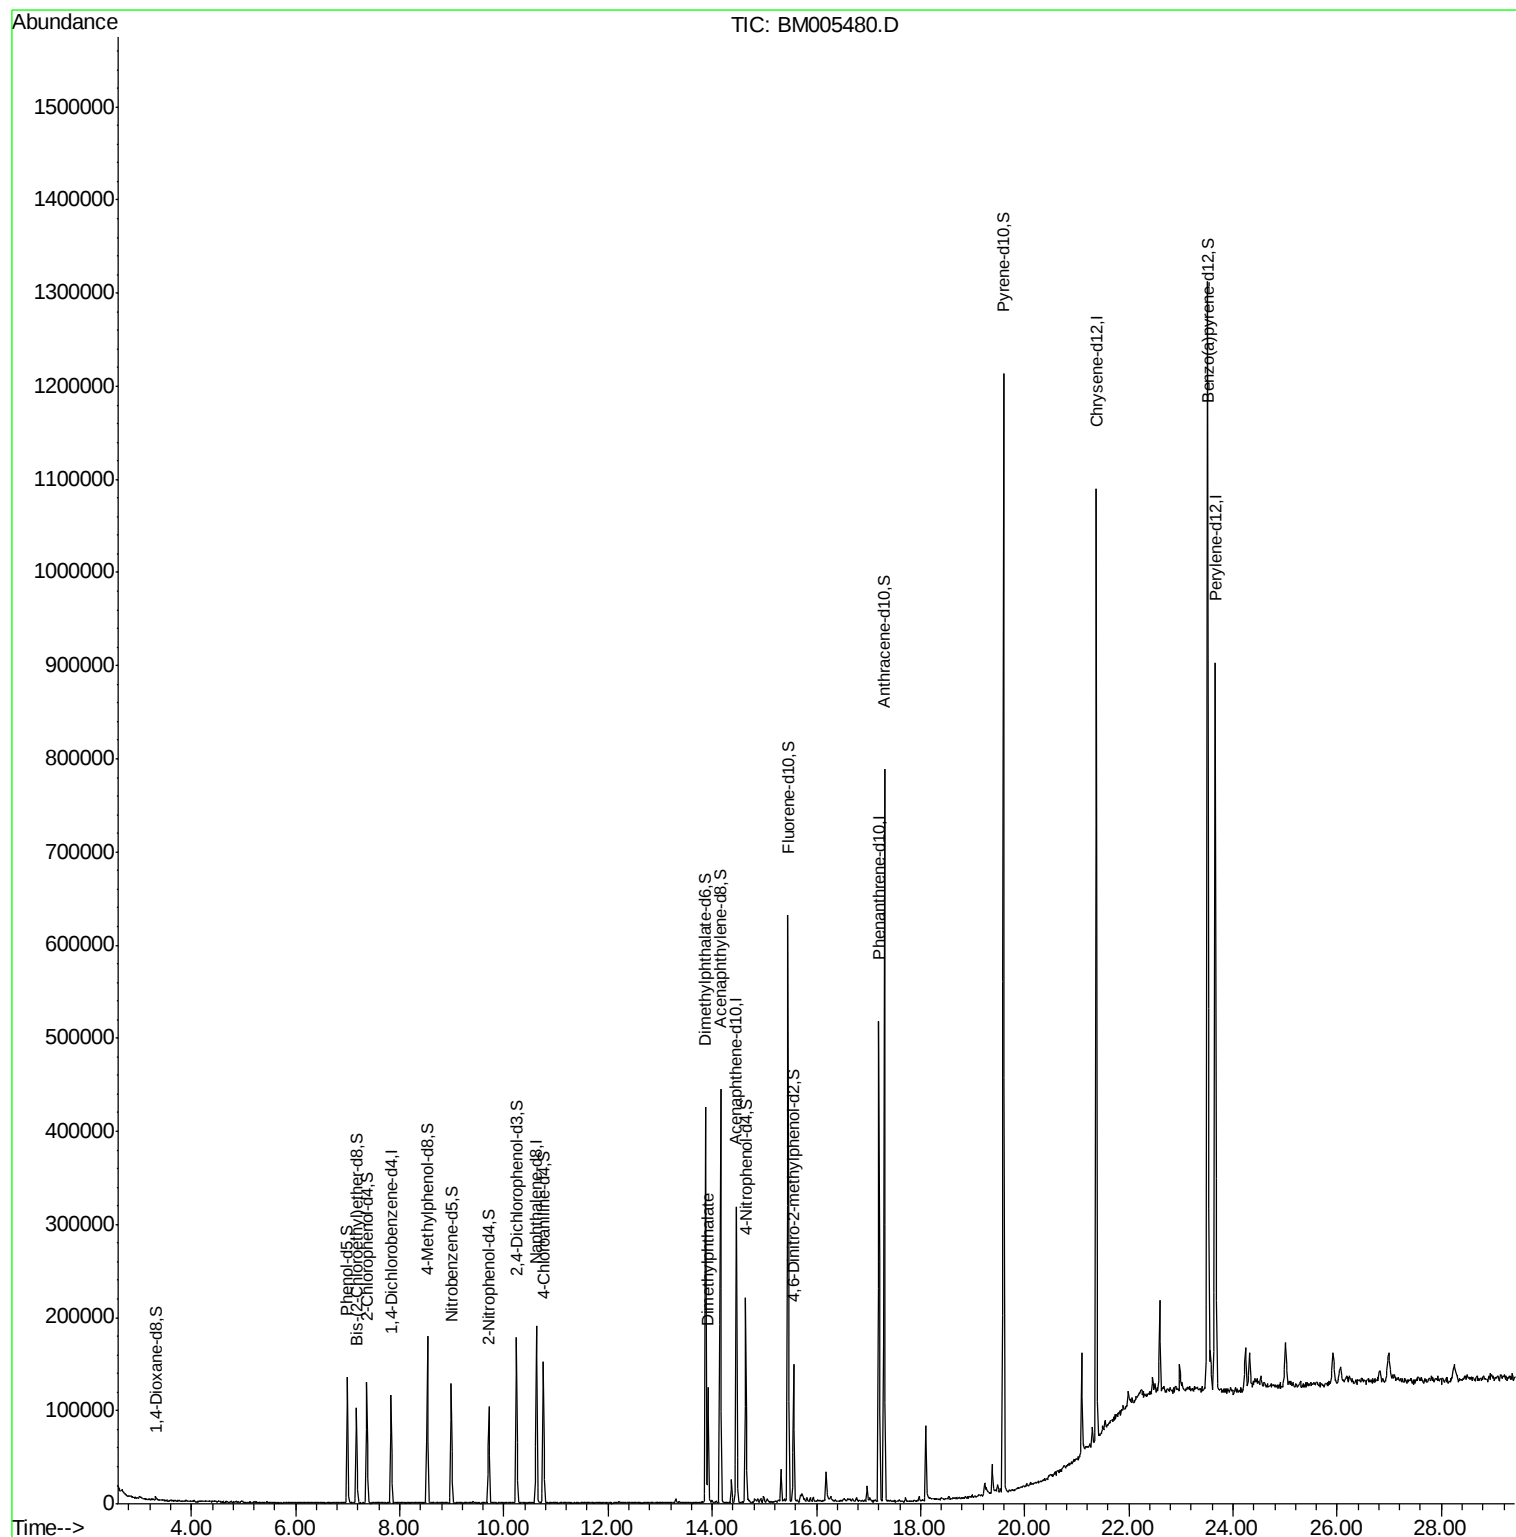


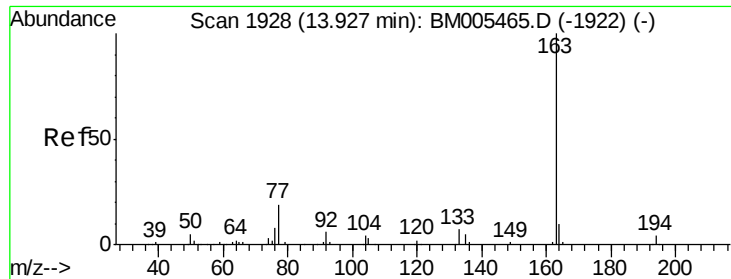

#44
 Dimethylphthalate
 Concen: 8.18 ng/ul
 RT: 13.92 min Scan# 1927
 Delta R.T. -0.01 min
 Lab File: BM005480.D
 Acq: 18 May 2016 21:32

Instrument :
 BNA_M
 ClientSampleId :
 D9WS8

Tgt Ion	Ratio	Lower	Upper
163	100		
194	4.1	3.4	5.0
164	10.1	7.9	11.9

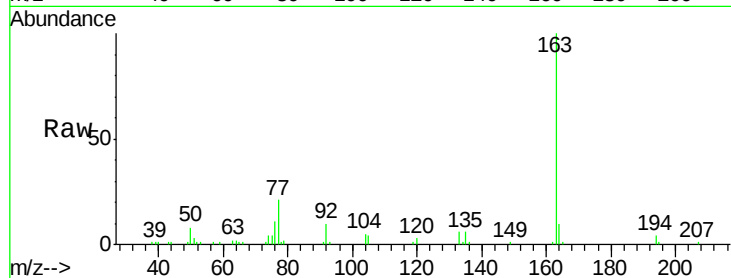

Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

