

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM051816\
 Data File : BM005481.D
 Acq On : 18 May 2016 22:09
 Operator : UM/SJ
 Sample : H2841-14
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9WS9

Quant Time: May 19 01:45:58 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM051816.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed May 18 14:47:27 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.84	152	25226	20.00	ng/ul	0.00
18) Naphthalene-d8	10.63	136	125615	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.46	164	90987	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.20	188	257056	20.00	ng/ul	0.00
75) Chrysene-d12	21.37	240	443121	20.00	ng/ul	-0.01
83) Perylene-d12	23.66	264	540864	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.32	96	1792	2.73	ng/uL	0.00
5) Phenol-d5	6.99	99	42112	17.38	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.17	67	25367	19.11	ng/ul	0.00
9) 2-Chlorophenol-d4	7.37	132	32535	17.48	ng/ul	0.00
13) 4-Methylphenol-d8	8.53	113	33424	16.19	ng/ul	0.00
19) Nitrobenzene-d5	8.99	128	16074	17.77	ng/ul	0.00
22) 2-Nitrophenol-d4	9.71	143	17424	17.66	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.24	165	35517	18.12	ng/ul	0.00
29) 4-Chloroaniline-d4	10.76	131	43279	19.19	ng/ul	0.00
43) Dimethylphthalate-d6	13.87	166	150485	20.12	ng/ul	0.00
46) Acenaphthylene-d8	14.16	160	169215	19.16	ng/ul	0.00
51) 4-Nitrophenol-d4	14.65	143	25225	16.44	ng/ul	0.00
57) Fluorene-d10	15.46	176	138593	21.00	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.56	200	17985	13.27	ng/ul	0.00
70) Anthracene-d10	17.30	188	243076	20.56	ng/ul	0.00
76) Pyrene-d10	19.59	212	354849	19.92	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.52	264	523171	21.64	ng/ul	0.00


Target Compounds						Qvalue
44) Dimethylphthalate	13.92	163	47887	6.28	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM051816\
Data File : BM005481.D
Acq On : 18 May 2016 22:09
Operator : UM/SJ
Sample : H2841-14
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
D9WS9

Quant Time: May 19 01:45:58 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM051816.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed May 18 14:47:27 2016
Response via : Initial Calibration

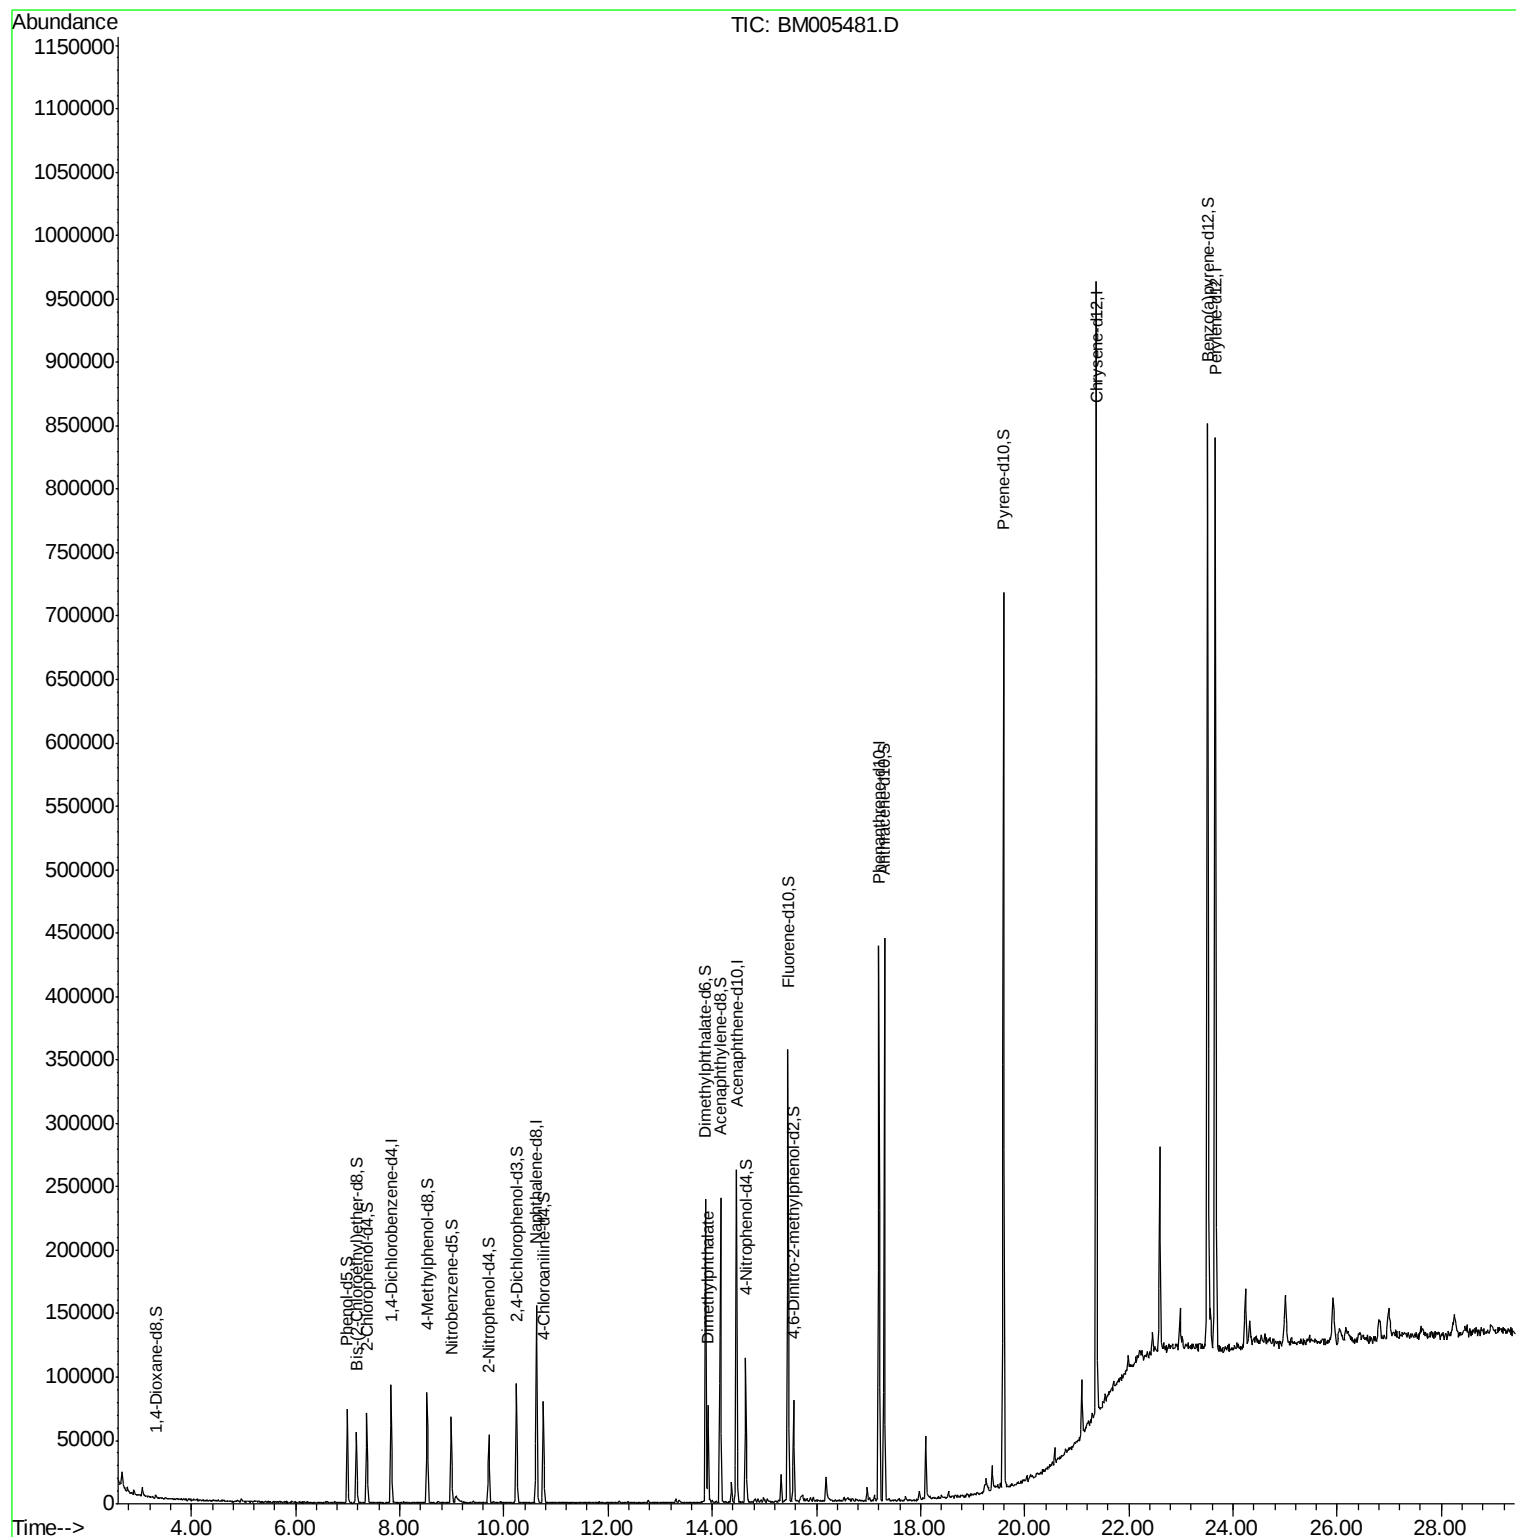

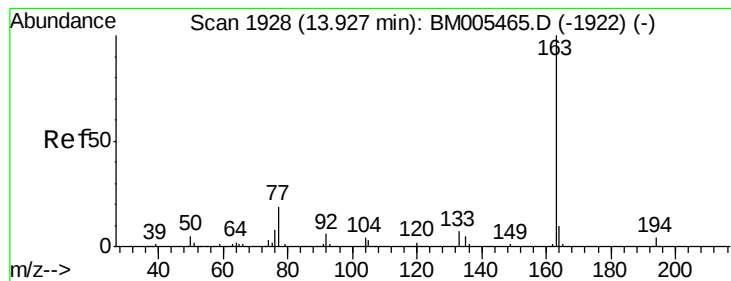

#44
 Dimethylphthalate
 Concen: 6.28 ng/ul
 RT: 13.92 min Scan# 1927
 Delta R.T. -0.01 min
 Lab File: BM005481.D
 Acq: 18 May 2016 22:09

Instrument :
 BNA_M
 ClientSampleId :
 D9WS9

Tgt Ion:	163	Resp:	47887
Ion	Ratio	Lower	Upper
163	100		
194	3.7	3.4	5.0
164	10.2	7.9	11.9

