

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM051816\
 Data File : BM005484.D
 Acq On : 18 May 2016 23:58
 Operator : UM/SJ
 Sample : H2841-19
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9WX5

Quant Time: May 19 01:46:56 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM051816.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed May 18 14:47:27 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.84	152	24554	20.00	ng/ul	0.00
18) Naphthalene-d8	10.63	136	125081	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.46	164	89860	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.20	188	257538	20.00	ng/ul	0.00
75) Chrysene-d12	21.37	240	459173	20.00	ng/ul	-0.01
83) Perylene-d12	23.66	264	560525	20.00	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.31	96	947	1.48	ng/uL	0.00
5) Phenol-d5	6.99	99	31240	13.24	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.17	67	19676	15.23	ng/ul	0.00
9) 2-Chlorophenol-d4	7.37	132	24648	13.60	ng/ul	0.00
13) 4-Methylphenol-d8	8.53	113	25275	12.58	ng/ul	0.00
19) Nitrobenzene-d5	8.99	128	12001	13.33	ng/ul	0.00
22) 2-Nitrophenol-d4	9.71	143	12747	12.98	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.24	165	26090	13.36	ng/ul	0.00
29) 4-Chloroaniline-d4	10.76	131	35551	15.83	ng/ul	0.00
43) Dimethylphthalate-d6	13.87	166	115060	15.58	ng/ul	0.00
46) Acenaphthylene-d8	14.16	160	129696	14.87	ng/ul	0.00
51) 4-Nitrophenol-d4	14.64	143	20050	13.23	ng/ul	0.00
57) Fluorene-d10	15.46	176	108080	16.58	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.56	200	14385	10.60	ng/ul	0.00
70) Anthracene-d10	17.30	188	191473	16.16	ng/ul	0.00
76) Pyrene-d10	19.59	212	273846	14.83	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.51	264	420979	16.80	ng/ul	-0.01


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
44) Dimethylphthalate	13.92	163	19818	2.63	ng/ul#	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM051816\
Data File : BM005484.D
Acq On : 18 May 2016 23:58
Operator : UM/SJ
Sample : H2841-19
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
D9WX5

Quant Time: May 19 01:46:56 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM051816.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed May 18 14:47:27 2016
Response via : Initial Calibration

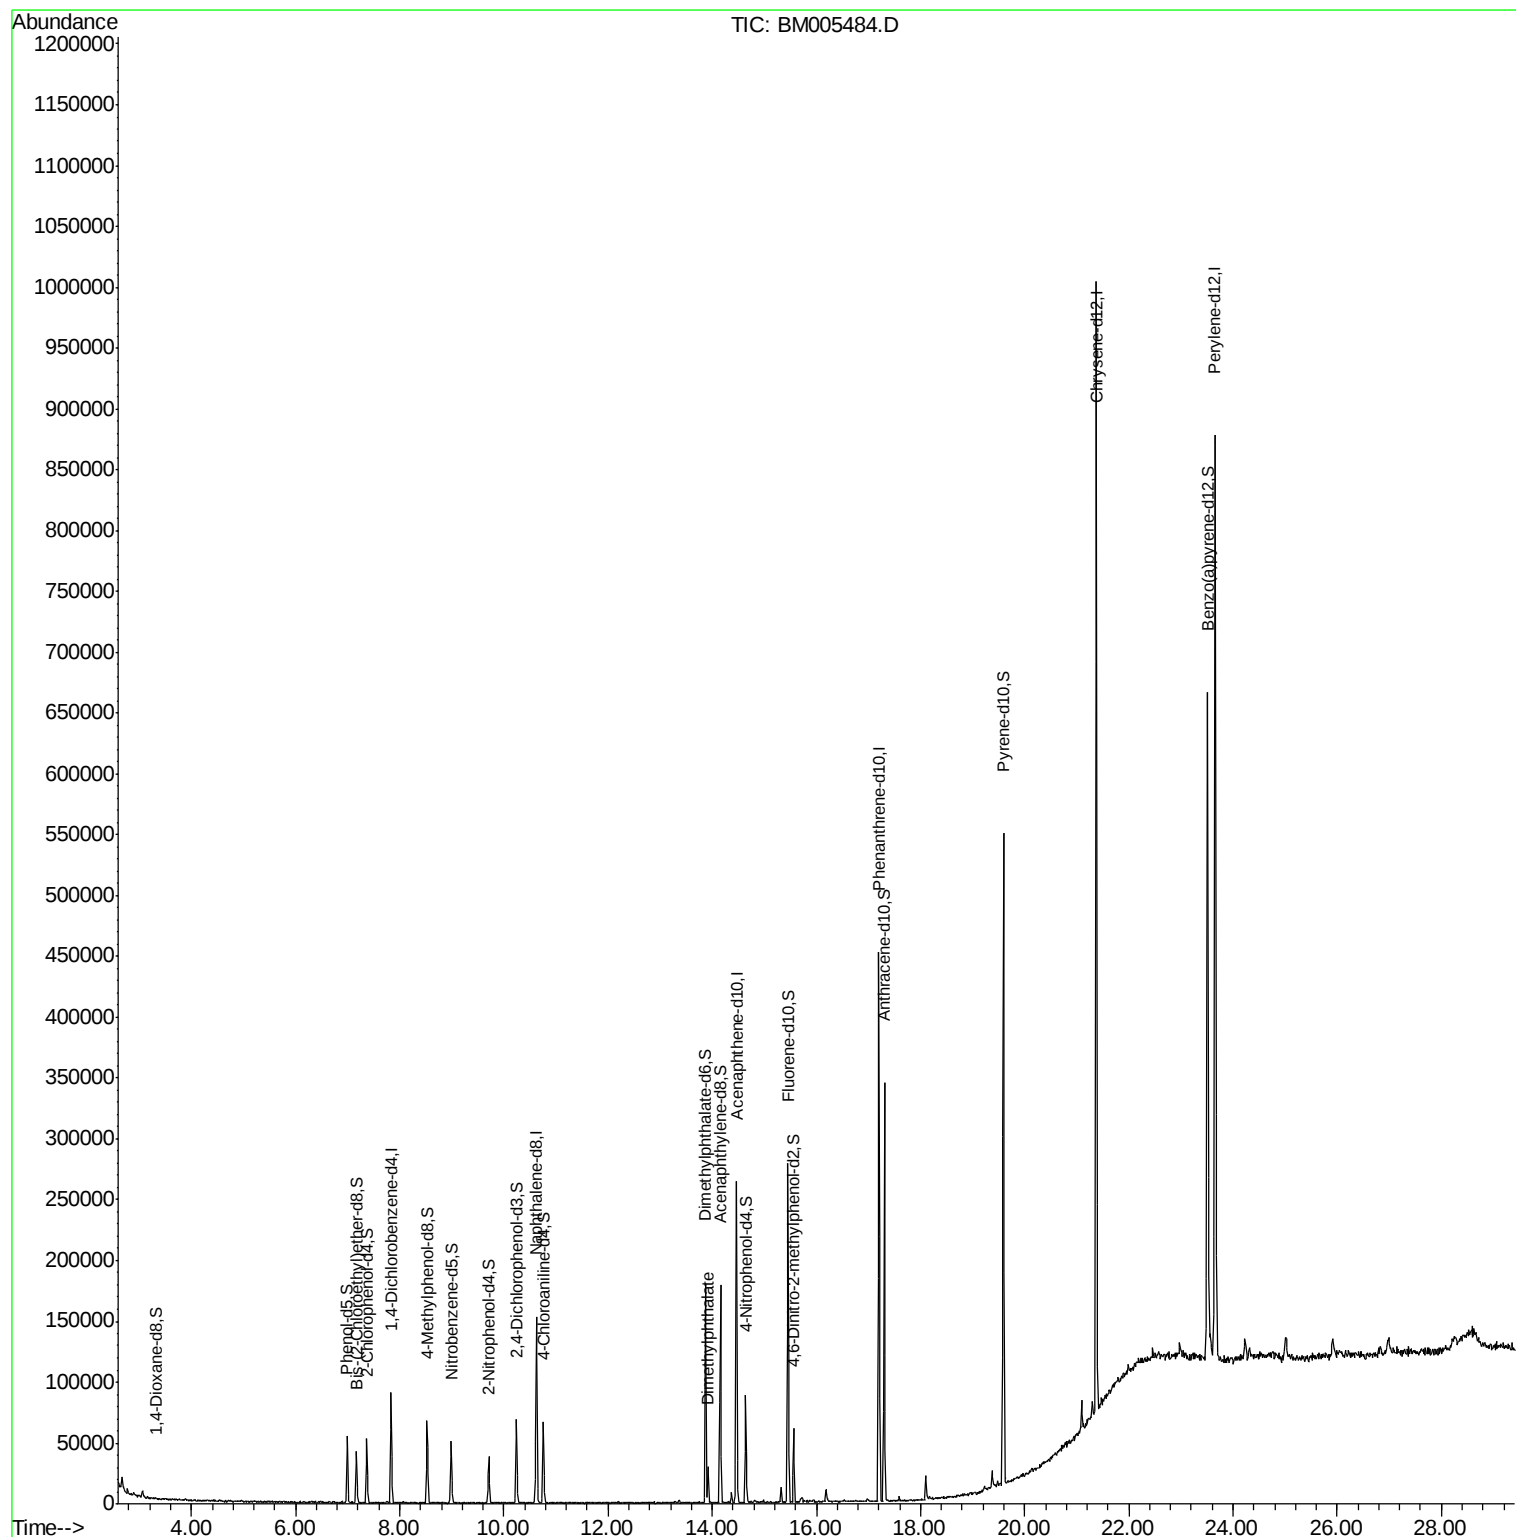


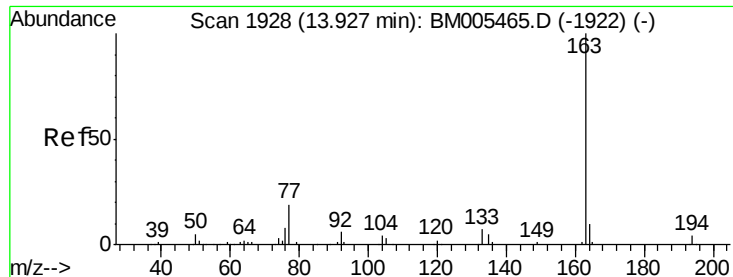

#44
 Dimethylphthalate
 Concen: 2.63 ng/ul
 RT: 13.92 min Scan# 1927
 Delta R.T. -0.01 min
 Lab File: BM005484.D
 Acq: 18 May 2016 23:58

Instrument :
 BNA_M
 ClientSampleId :
 D9WX5

Tgt Ion:163 Resp: 19818
 Ion Ratio Lower Upper
 163 100
 194 4.3 3.4 5.0
 164 11.9 7.9 11.9#

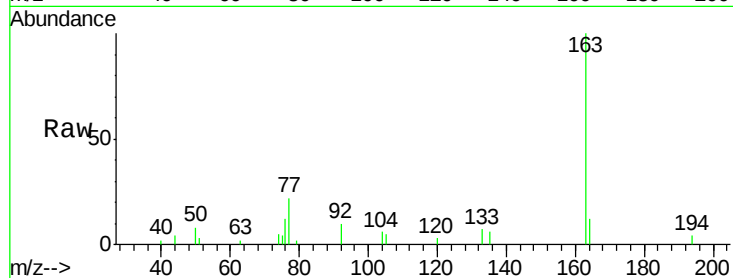

Abundance Ion 163.00 (162.70 to 163.70): E
 Ion 194.00 (193.70 to 194.70): E
 Ion 164.00 (163.70 to 164.70): E

