

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM051816\
 Data File : BM005485.D
 Acq On : 19 May 2016 00:34
 Operator : UM/SJ
 Sample : H2841-20
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9WX6

Quant Time: May 19 01:47:08 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM051816.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed May 18 14:47:27 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.84	152	19740	20.00	ng/ul	0.00
18) Naphthalene-d8	10.63	136	97792	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.46	164	69743	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.20	188	201830	20.00	ng/ul	0.00
75) Chrysene-d12	21.37	240	360145	20.00	ng/ul	-0.01
83) Perylene-d12	23.66	264	446331	20.00	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.32	96	1220	2.38	ng/uL	0.00
5) Phenol-d5	6.99	99	32326	17.05	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.17	67	19993	19.25	ng/ul	0.00
9) 2-Chlorophenol-d4	7.37	132	25780	17.70	ng/ul	0.00
13) 4-Methylphenol-d8	8.53	113	27957	17.31	ng/ul	0.00
19) Nitrobenzene-d5	8.99	128	12080	17.16	ng/ul	0.00
22) 2-Nitrophenol-d4	9.71	143	12940	16.85	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.24	165	26936	17.65	ng/ul	0.00
29) 4-Chloroaniline-d4	10.76	131	24266	13.82	ng/ul	0.00
43) Dimethylphthalate-d6	13.87	166	120492	21.02	ng/ul	0.00
46) Acenaphthylene-d8	14.16	160	132164	19.53	ng/ul	0.00
51) 4-Nitrophenol-d4	14.64	143	19929	16.94	ng/ul	0.00
57) Fluorene-d10	15.46	176	111304	22.00	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.56	200	13535	12.72	ng/ul	0.00
70) Anthracene-d10	17.30	188	198076	21.34	ng/ul	0.00
76) Pyrene-d10	19.59	212	280873	19.40	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.51	264	436025	21.85	ng/ul	-0.01


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
44) Dimethylphthalate	13.92	163	19039	3.26	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM051816\
Data File : BM005485.D
Acq On : 19 May 2016 00:34
Operator : UM/SJ
Sample : H2841-20
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
D9WX6

Quant Time: May 19 01:47:08 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM051816.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed May 18 14:47:27 2016
Response via : Initial Calibration

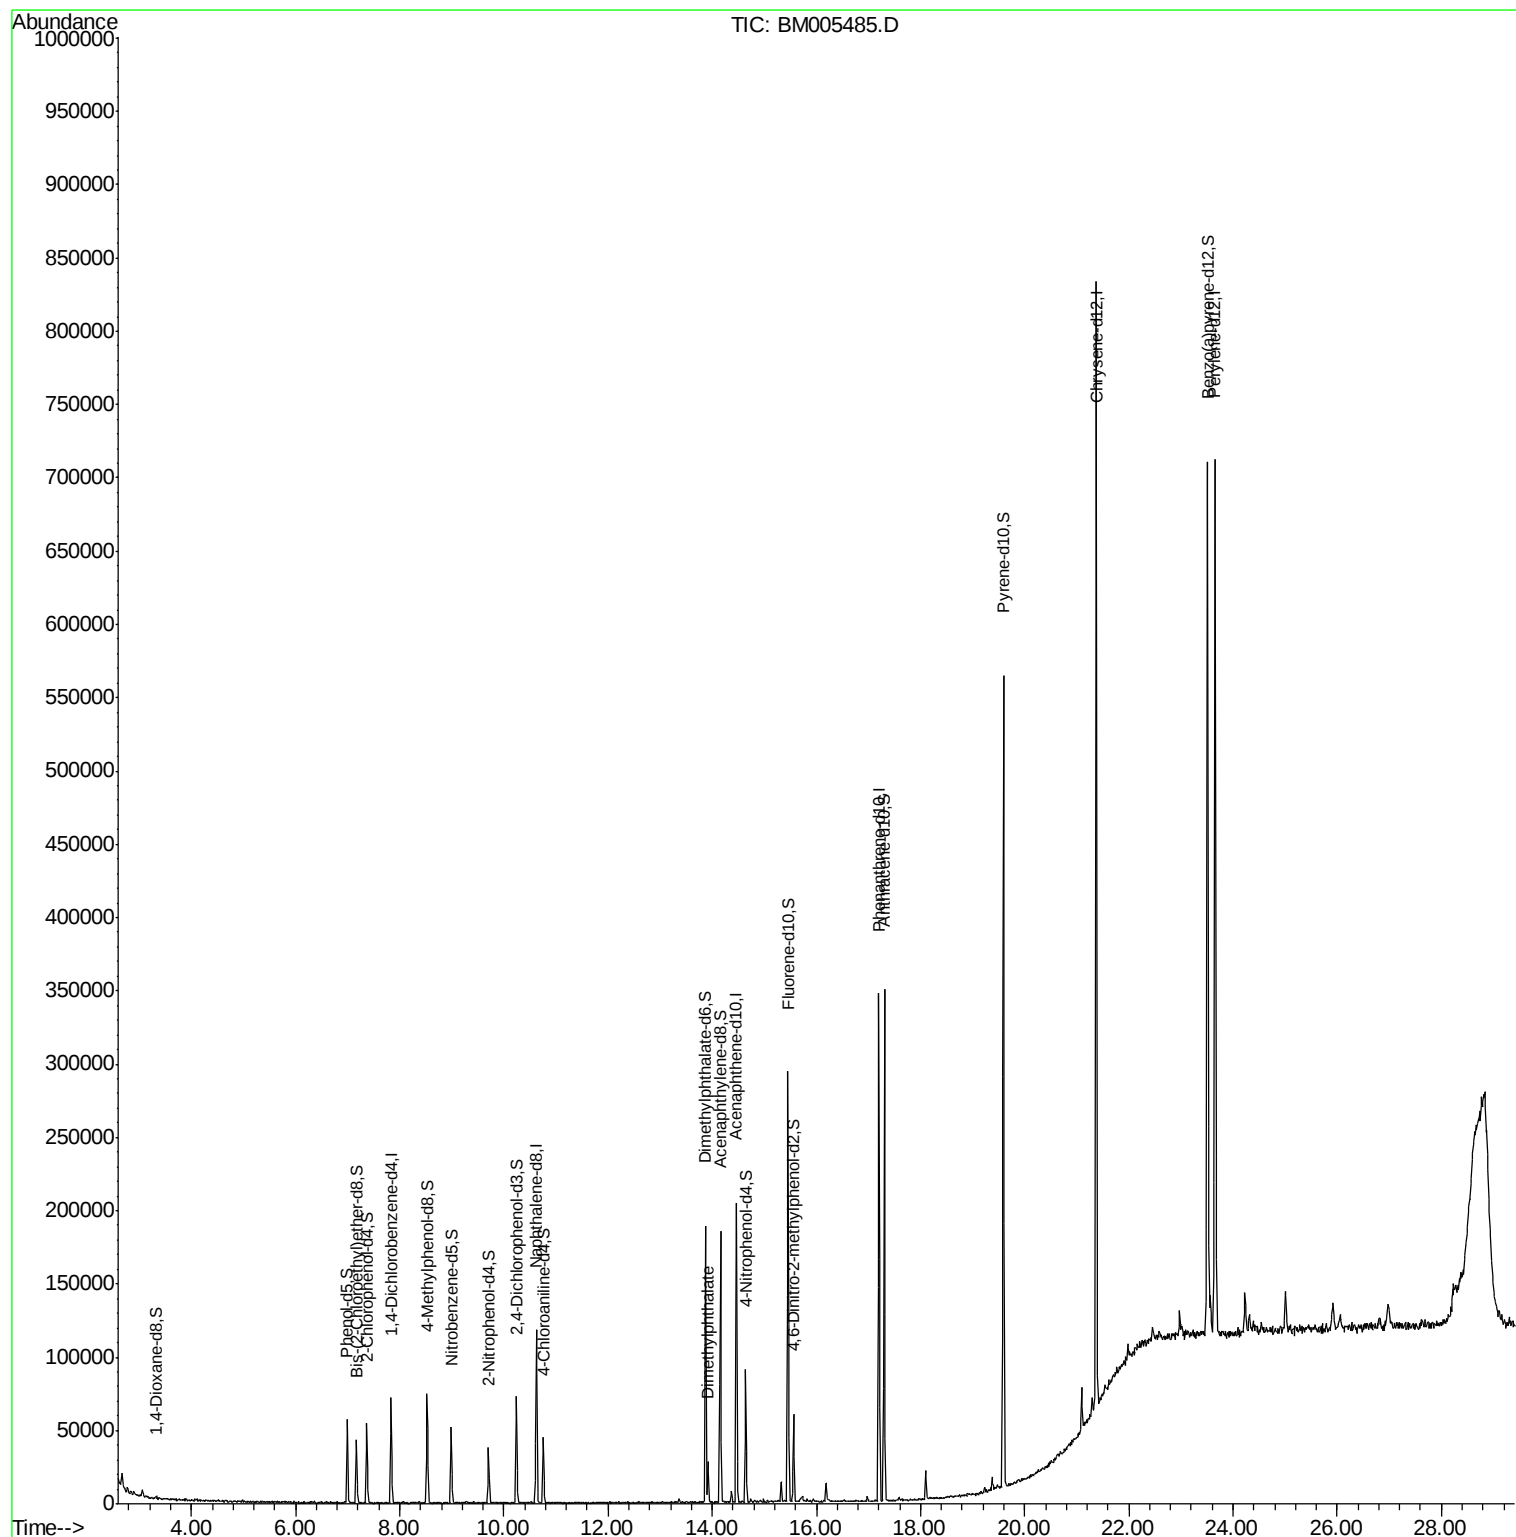

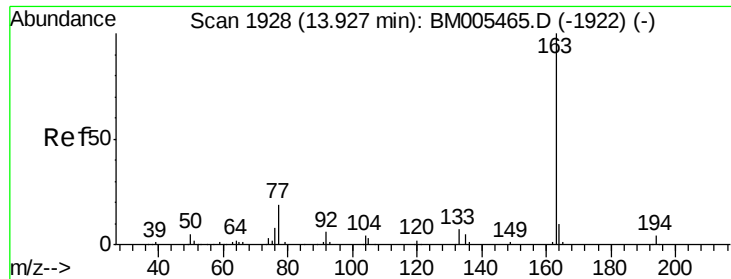

#44

Dimethylphthalate

Concen: 3.26 ng/ul

RT: 13.92 min Scan# 1927

Delta R.T. -0.01 min

Lab File: BM005485.D


Acq: 19 May 2016 00:34

Instrument :

BNA_M

ClientSampleId :

D9WX6

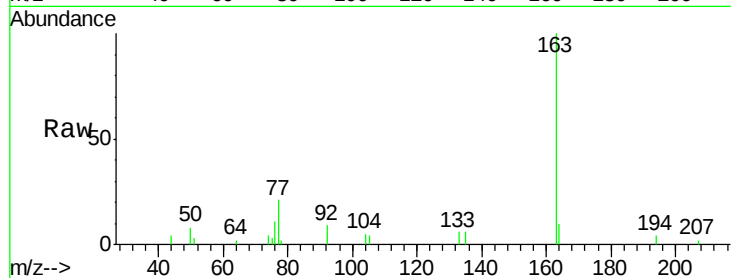

Tgt Ion:163 Resp: 19039

Ion Ratio Lower Upper

163 100

194 4.3 3.4 5.0

164 10.4 7.9 11.9

