

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM051816\
 Data File : BM005486.D
 Acq On : 19 May 2016 01:10
 Operator : UM/SJ
 Sample : H2890-01
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9WY5

Quant Time: May 19 01:47:20 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM051816.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed May 18 14:47:27 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.83	152	23307	20.00	ng/ul	0.00
18) Naphthalene-d8	10.63	136	120833	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.46	164	85058	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.20	188	242874	20.00	ng/ul	0.00
75) Chrysene-d12	21.37	240	429424	20.00	ng/ul	-0.01
83) Perylene-d12	23.66	264	531811	20.00	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.32	96	2497	4.12	ng/uL	0.00
5) Phenol-d5	6.99	99	64286	28.71	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.17	67	38133	31.10	ng/ul	0.00
9) 2-Chlorophenol-d4	7.36	132	48007	27.91	ng/ul	0.00
13) 4-Methylphenol-d8	8.53	113	56179	29.46	ng/ul	0.00
19) Nitrobenzene-d5	8.99	128	24825	28.54	ng/ul	0.00
22) 2-Nitrophenol-d4	9.71	143	27181	28.64	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.24	165	55667	29.52	ng/ul	0.00
29) 4-Chloroaniline-d4	10.76	131	90434	41.69	ng/ul	0.00
43) Dimethylphthalate-d6	13.87	166	237944	34.03	ng/ul	0.00
46) Acenaphthylene-d8	14.16	160	269401	32.63	ng/ul	0.00
51) 4-Nitrophenol-d4	14.64	143	43783	30.52	ng/ul	0.00
57) Fluorene-d10	15.46	176	215847	34.98	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.57	200	30292	23.66	ng/ul	0.00
70) Anthracene-d10	17.30	188	389648	34.88	ng/ul	0.00
76) Pyrene-d10	19.59	212	546148	31.63	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.51	264	852837	35.87	ng/ul	-0.01


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
44) Dimethylphthalate	13.92	163	70673	9.91	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM051816\
Data File : BM005486.D
Acq On : 19 May 2016 01:10
Operator : UM/SJ
Sample : H2890-01
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
D9WY5

Quant Time: May 19 01:47:20 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM051816.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed May 18 14:47:27 2016
Response via : Initial Calibration

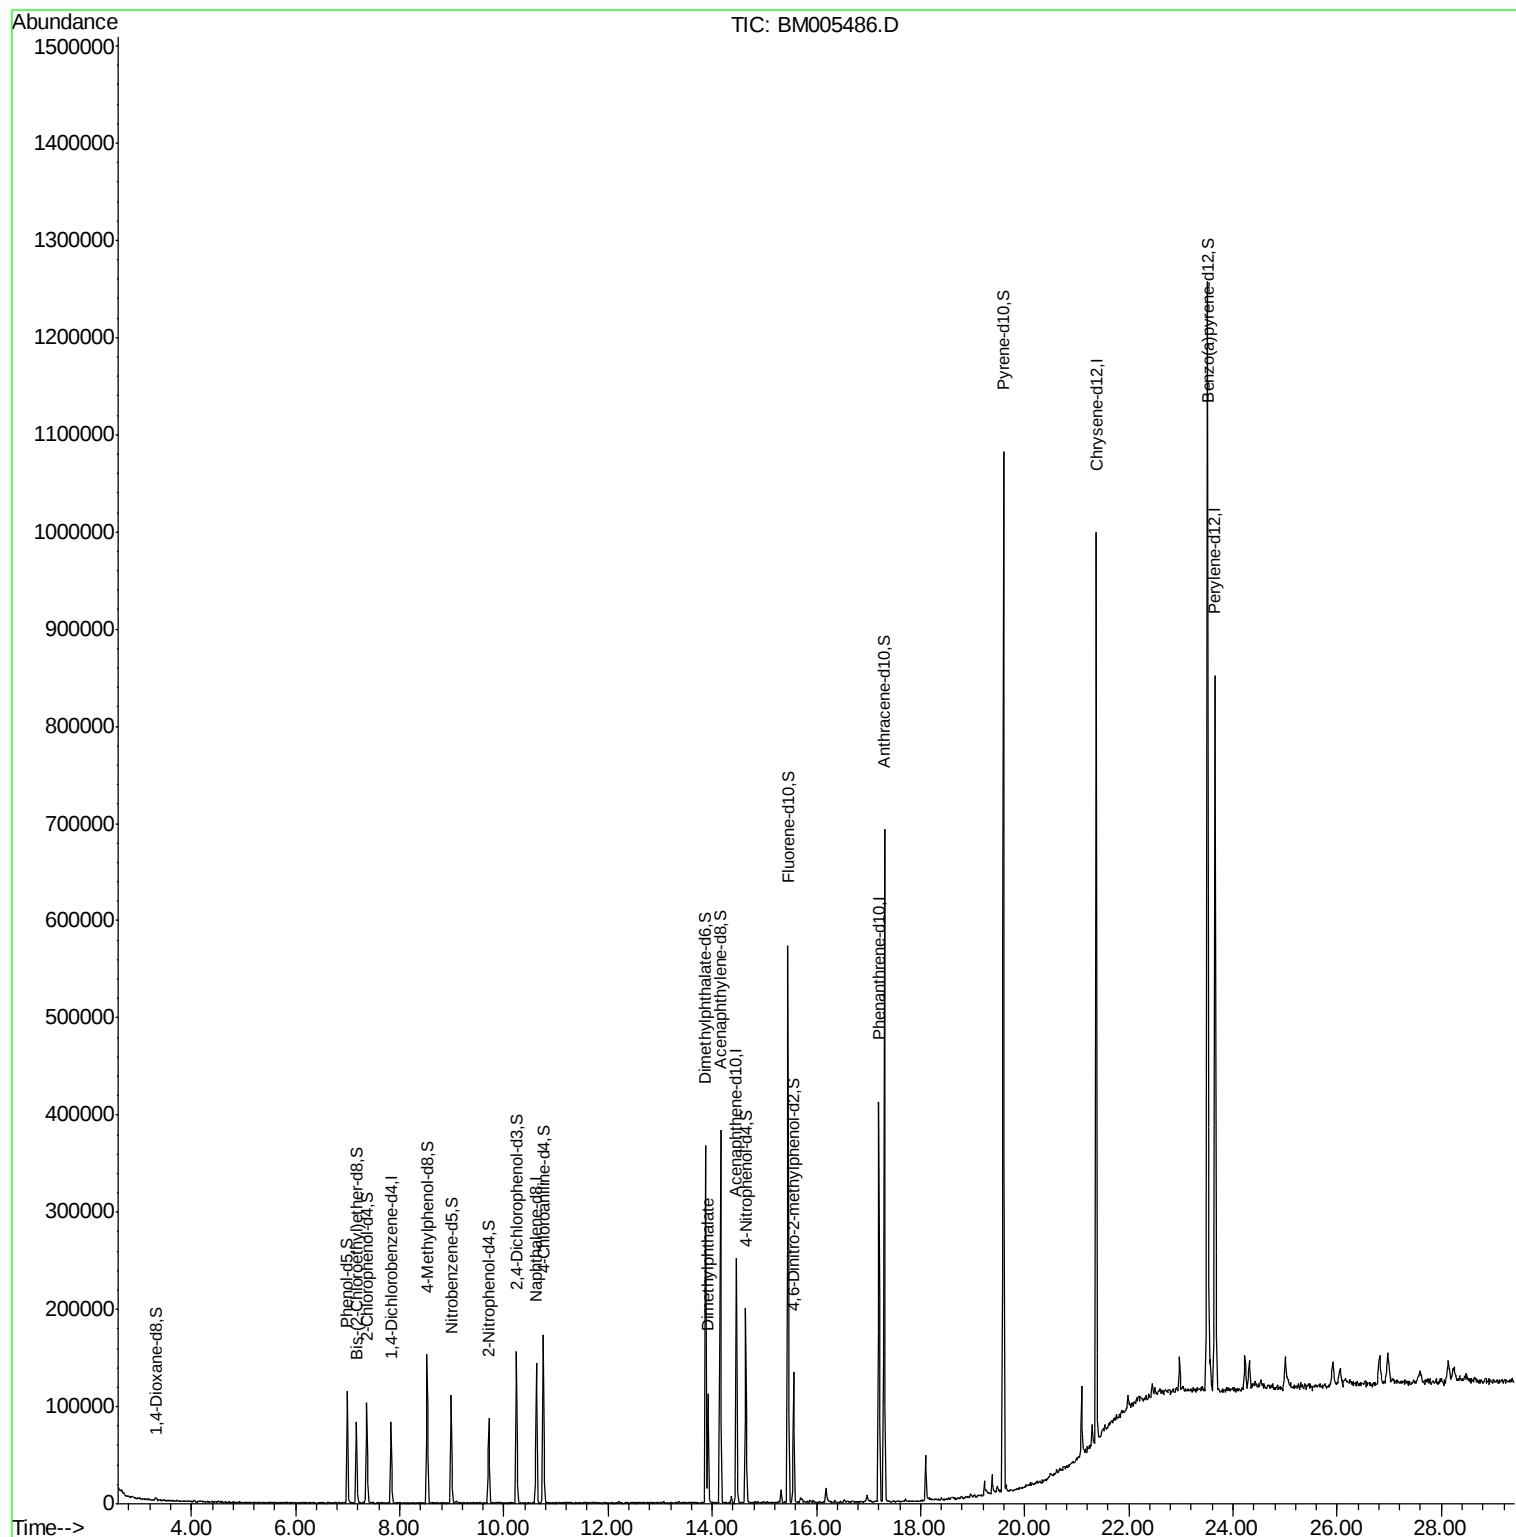

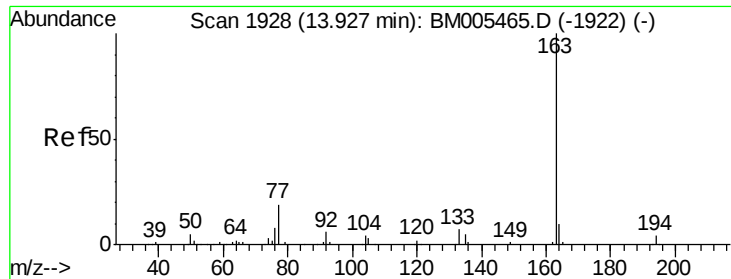

#44

Dimethylphthalate

Concen: 9.91 ng/ul

RT: 13.92 min Scan# 1927

Delta R.T. -0.01 min

Lab File: BM005486.D

Acq: 19 May 2016 01:10

Instrument :

BNA_M

ClientSampleId :

D9WY5


Tgt Ion:163 Resp: 70673

Ion Ratio Lower Upper

163 100

194 3.9 3.4 5.0

164 10.5 7.9 11.9

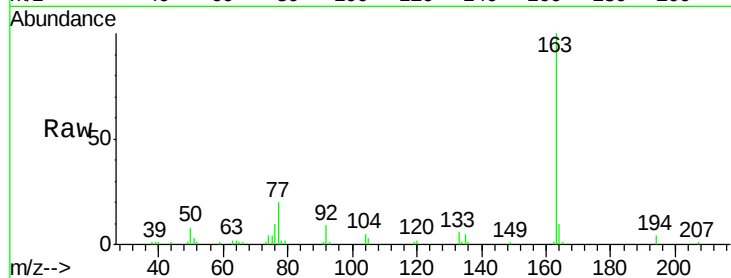

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

