

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM051816\
 Data File : BM005497.D
 Acq On : 19 May 2016 07:49
 Operator : UM/SJ
 Sample : H2890-22RX
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9X07RX

Quant Time: May 19 08:21:11 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM051816.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed May 18 14:47:27 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.84	152	22357	20.00	ng/ul	0.00
18) Naphthalene-d8	10.62	136	113696	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.46	164	79563	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.20	188	223395	20.00	ng/ul	0.00
75) Chrysene-d12	21.37	240	368924	20.00	ng/ul	-0.01
83) Perylene-d12	23.66	264	447201	20.00	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	0.00	96	0	0.00	ng/uL	
5) Phenol-d5	6.99	99	3902	1.82	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.17	67	6308	5.36	ng/ul	0.00
9) 2-Chlorophenol-d4	7.36	132	7614	4.62	ng/ul	0.00
13) 4-Methylphenol-d8	8.53	113	6586	3.60	ng/ul	0.00
19) Nitrobenzene-d5	8.99	128	3528	4.31	ng/ul	0.00
22) 2-Nitrophenol-d4	9.71	143	4339	4.86	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.24	165	9951	5.61	ng/ul	0.00
29) 4-Chloroaniline-d4	0.00	131	0	0.00	ng/ul	
43) Dimethylphthalate-d6	13.87	166	35288	5.40	ng/ul	0.00
46) Acenaphthylene-d8	14.16	160	34399	4.45	ng/ul	0.00
51) 4-Nitrophenol-d4	14.64	143	2375	1.77	ng/ul	-0.01
57) Fluorene-d10	15.45	176	26422	4.58	ng/ul	-0.01
62) 4,6-Dinitro-2-methylphenol	15.56	200	4276	3.63	ng/ul	0.00
70) Anthracene-d10	17.30	188	39103	3.81	ng/ul	0.00
76) Pyrene-d10	19.59	212	53088	3.58	ng/ul	-0.01
87) Benzo(a)pyrene-d12	23.51	264	73196	3.66	ng/ul	-0.01


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
44) Dimethylphthalate	13.92	163	45448	6.82	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM051816\
Data File : BM005497.D
Acq On : 19 May 2016 07:49
Operator : UM/SJ
Sample : H2890-22RX
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
D9X07RX

Quant Time: May 19 08:21:11 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM051816.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed May 18 14:47:27 2016
Response via : Initial Calibration

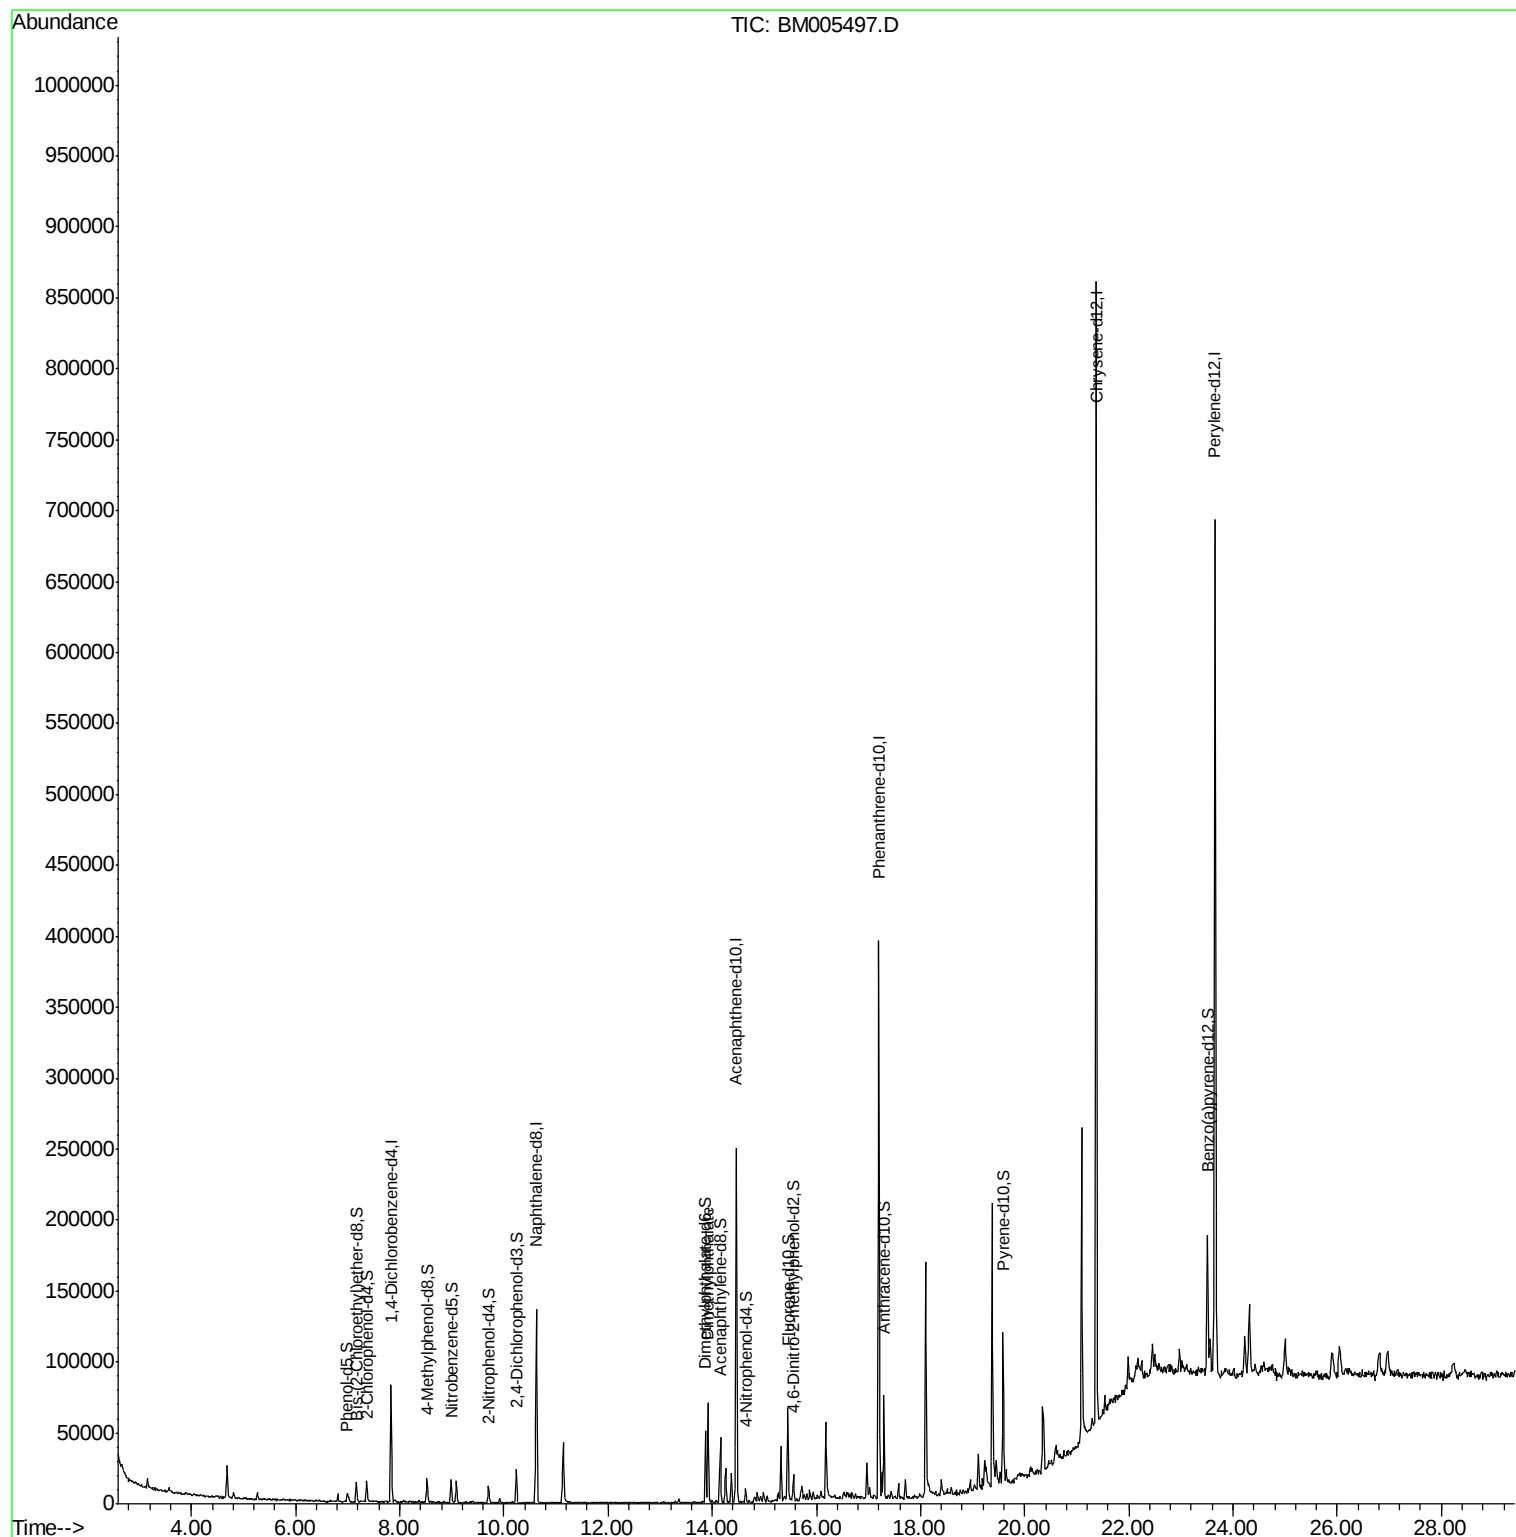

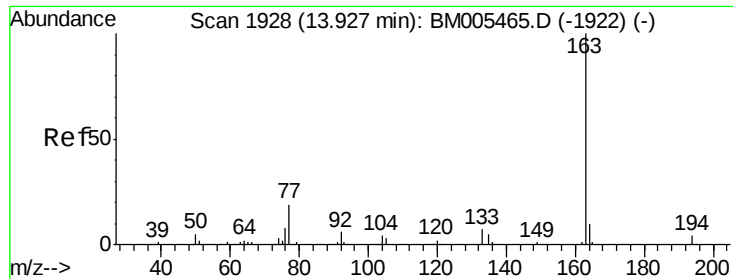

#44

Dimethylphthalate

Concen: 6.82 ng/ul

RT: 13.92 min Scan# 1927

Delta R.T. -0.01 min

Lab File: BM005497.D

Acq: 19 May 2016 07:49

Instrument :

BNA_M

ClientSampleId :

D9X07RX


Tgt Ion:163 Resp: 45448

Ion Ratio Lower Upper

163 100

194 4.3 3.4 5.0

164 9.6 7.9 11.9

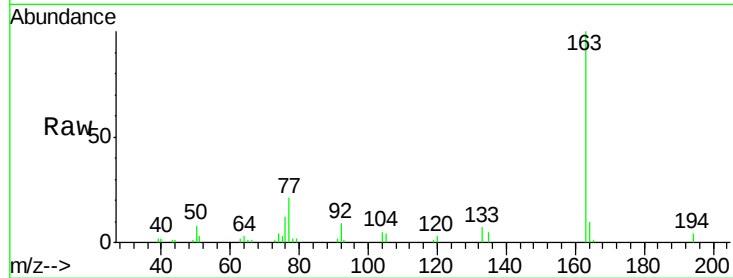

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

