

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM051816\
 Data File : BM005477.D
 Acq On : 18 May 2016 19:43
 Operator : UM/SJ
 Sample : H2841-10
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9WS5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM051816.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.669	11	14	29	rVB2	13761	31913	2.00%	0.329%
2	6.992	744	749	756	rBV	65531	102531	6.43%	1.056%
3	7.169	774	779	788	rVB	52332	82025	5.14%	0.844%
4	7.369	807	813	819	rBV	62763	97839	6.13%	1.007%
5	7.839	882	893	899	rBV	122935	198124	12.42%	2.040%
6	8.534	1005	1011	1017	rBV	85143	136337	8.55%	1.404%
7	8.992	1082	1089	1096	rBV	59640	101261	6.35%	1.043%
8	9.710	1205	1211	1217	rBV	48506	77516	4.86%	0.798%
9	10.239	1295	1301	1310	rVB	85872	137335	8.61%	1.414%
10	10.628	1359	1367	1375	rBV	204493	334721	20.98%	3.446%
11	10.757	1384	1389	1397	rVB	58219	97106	6.09%	1.000%
12	13.874	1913	1919	1924	rBV	214874	292042	18.30%	3.007%
13	13.921	1924	1927	1932	rVB	42412	53552	3.36%	0.551%
14	14.157	1961	1967	1974	rBV	208247	313857	19.67%	3.231%
15	14.468	2014	2020	2030	rVB2	334453	525448	32.93%	5.410%
16	14.645	2044	2050	2059	rBV	97719	140117	8.78%	1.443%
17	15.327	2159	2166	2169	rBV	14863	18137	1.14%	0.187%
18	15.457	2182	2188	2194	rVB	346384	475387	29.80%	4.894%
19	15.562	2202	2206	2215	rBV	72935	101254	6.35%	1.042%
20	16.186	2307	2312	2324	rBV	15899	30617	1.92%	0.315%
21	17.204	2479	2485	2493	rVB2	546343	764186	47.90%	7.868%
22	17.304	2495	2502	2509	rBV2	402268	554496	34.75%	5.709%
23	18.098	2633	2637	2645	rBV2	31395	42465	2.66%	0.437%
24	18.962	2780	2784	2792	rBV6	10845	19028	1.19%	0.196%
25	19.380	2852	2855	2858	rBV3	15000	16937	1.06%	0.174%
26	19.592	2885	2891	2897	rBV	623790	837324	52.48%	8.621%
27	21.097	3144	3147	3152	rBV3	37420	45319	2.84%	0.467%
28	21.380	3190	3195	3202	rBV	1065400	1381691	86.60%	14.225%
29	23.521	3552	3559	3565	rBV2	568837	1108909	69.50%	11.417%
30	23.662	3577	3583	3597	rVB	818871	1595507	100.00%	16.427%


Sum of corrected areas: 9712981

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM051816\
Data File : BM005477.D
Acq On : 18 May 2016 19:43
Operator : UM/SJ
Sample : H2841-10
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
D9WS5

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM051816.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

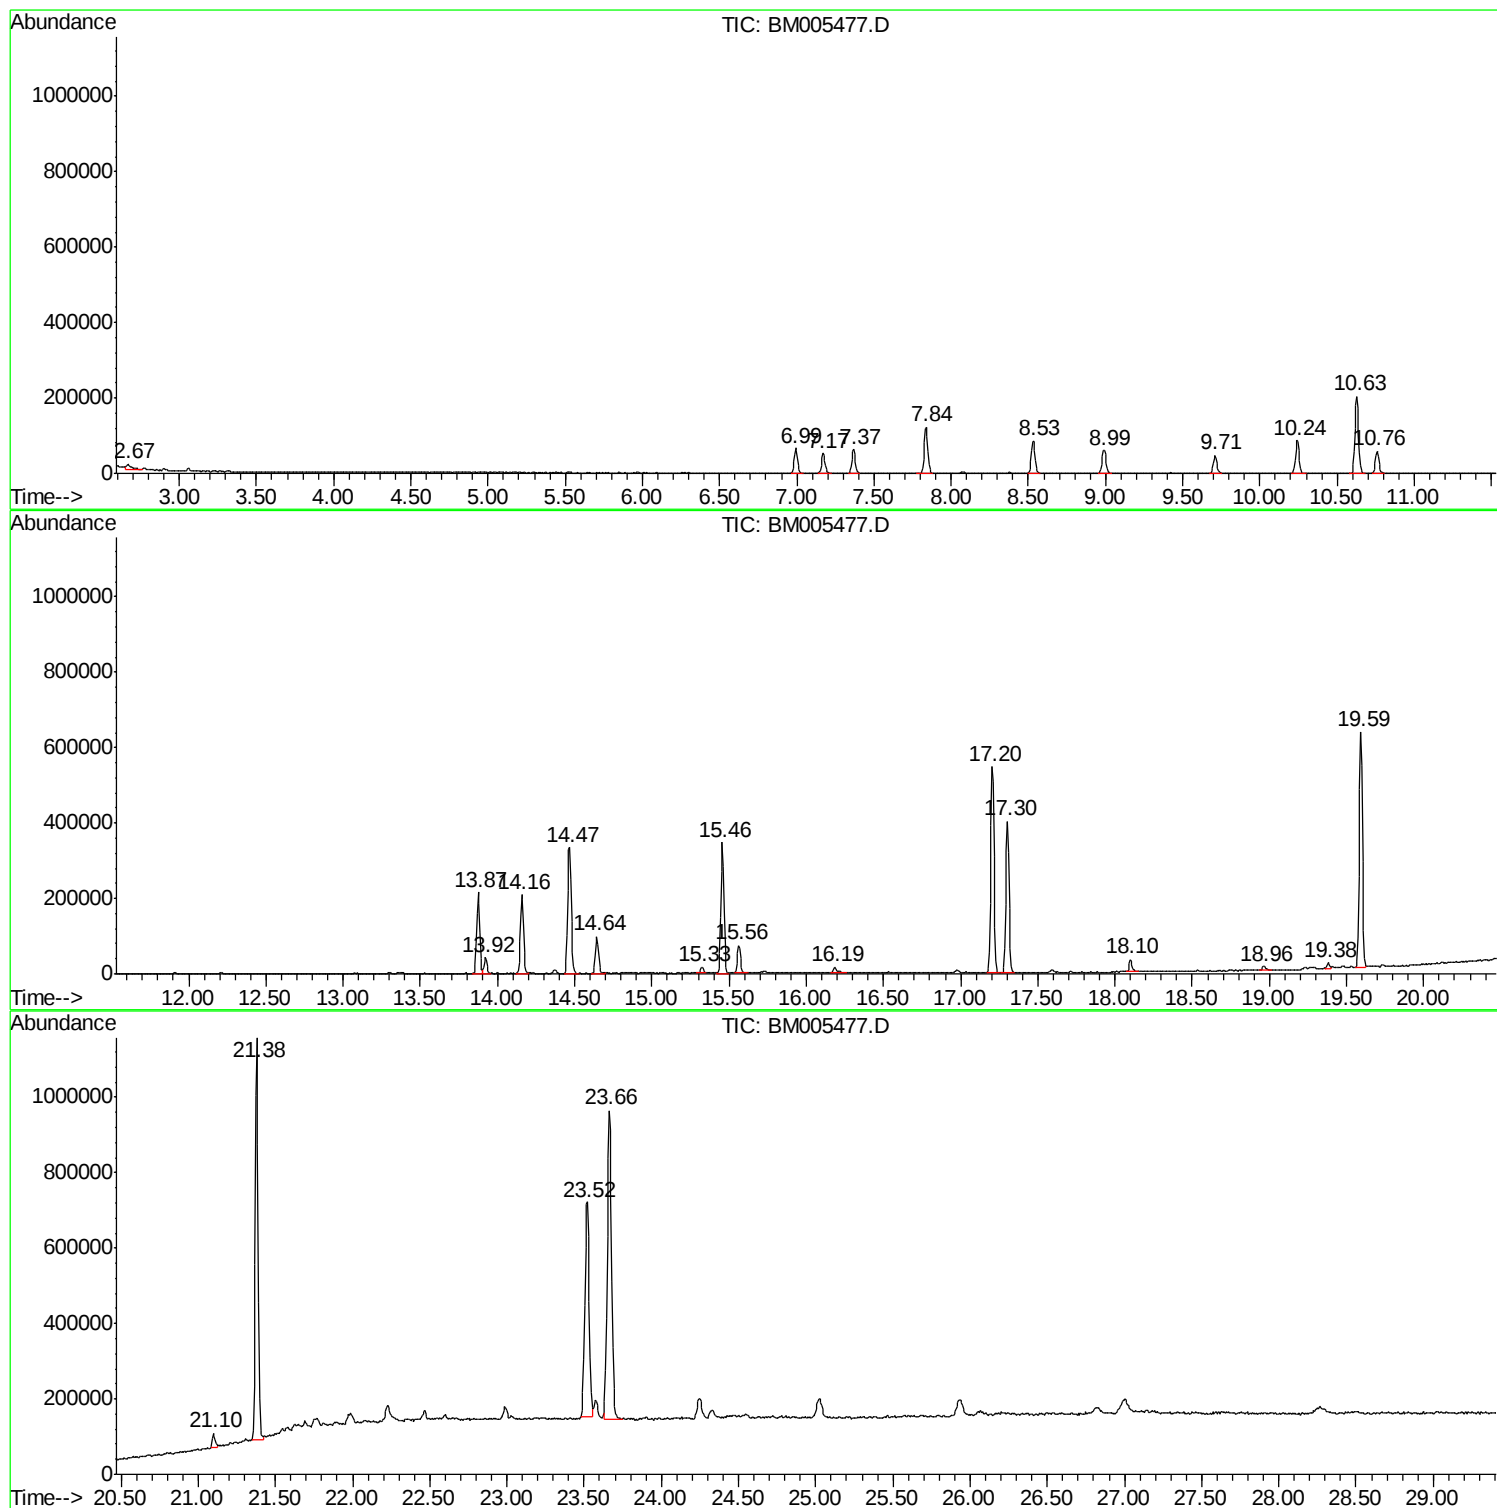

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM051816\
Data File : BM005477.D
Acq On : 18 May 2016 19:43
Operator : UM/SJ
Sample : H2841-10
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
D9WS5










Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM051816.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Propane, 3,3-dichloro-1,1,1... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.67	3.22 ng/ul	31913	1,4-Dichlorobenzene-d4	7.84

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	Propane, 3,3-dichloro-1,1,1,2,2-...	202	C3HCl2F5	000422-56-0	74		
2	Methane, bromodichloro-	162	CHBrCl2	000075-27-4	64		
3	Methane, bromodichloro-	162	CHBrCl2	000075-27-4	64		
4	Methane, dichloronitro-	129	CHCl2NO2	007119-89-3	64		
5	Dichloroacetic anhydride	238	C4H2Cl4O3	004124-30-5	64		

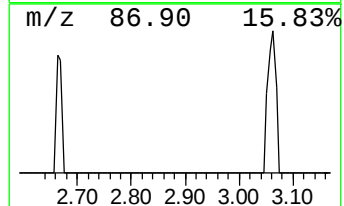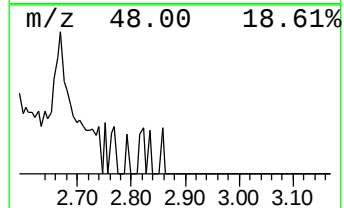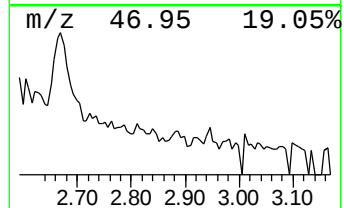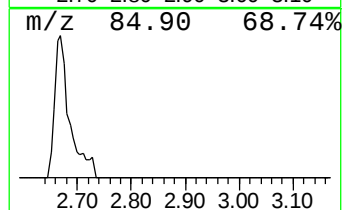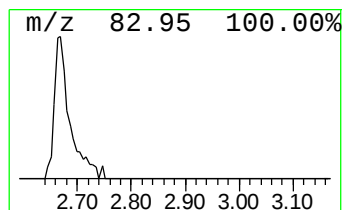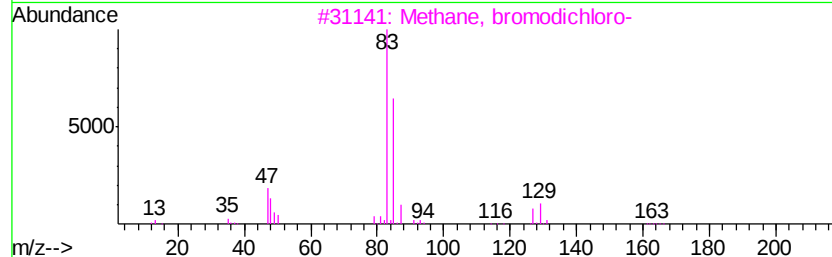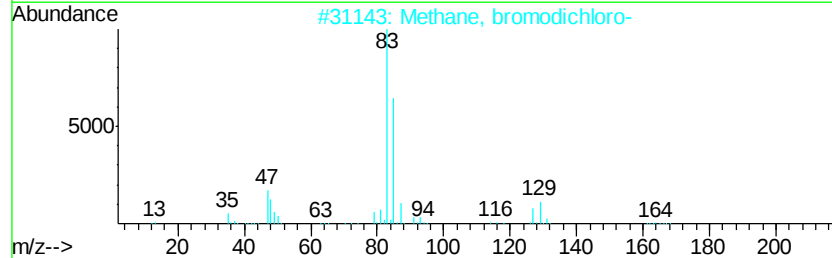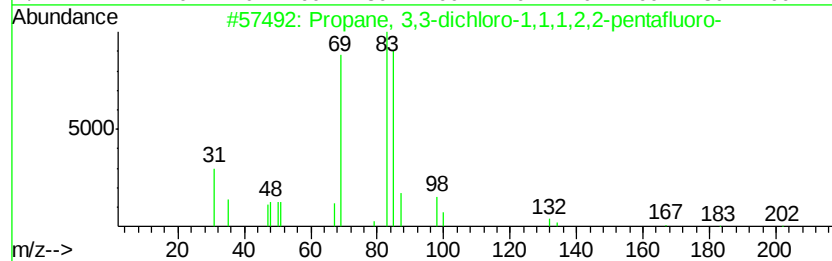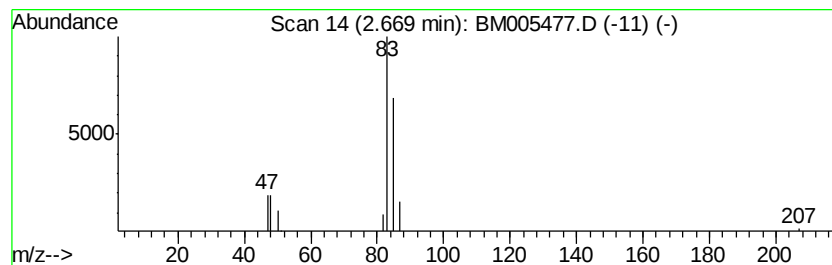

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM051816\
Data File : BM005477.D
Acq On : 18 May 2016 19:43
Operator : UM/SJ
Sample : H2841-10
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
D9WS5

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM051816.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Propane, 3,3-dich...	2.67	3.2	ng/ul	31913	1	7.84	198124	20.0