

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM051821\
 Data File : BM030064.D
 Acq On : 18 May 2021 13:01
 Operator : CG/JU
 Sample : PB136458BS
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SLCS458

Manual Integrations
 APPROVED

mohammad
 5/19/2021 11:38:38 AM

Quant Time: May 18 16:46:01 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 18 16:38:21 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.52	152	153252	20.00	ng/ul	0.00
20) Naphthalene-d8	10.29	136	717485	20.00	ng/ul	0.00
38) Acenaphthene-d10	14.17	164	487451	20.00	ng/ul	0.00
64) Phenanthrene-d10	16.92	188	1005906	20.00	ng/ul	0.00
79) Chrysene-d12	21.12	240	1075726	20.00	ng/ul	0.00
88) Perylene-d12	23.26	264	1030068	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.03	96	19001	4.95	ng/uL	0.00
4) Pyridine-d5	3.45	84	128947	13.42	ng/ul	0.00
7) Phenol-d5	6.70	99	292713	20.54	ng/ul	0.00
9) Bis-(2-Chloroethyl)ether-d	6.87	67	188383	21.32	ng/ul	0.00
11) 2-Chlorophenol-d4	7.05	132	238753	21.71	ng/ul	0.00
15) 4-Methylphenol-d8	8.24	113	245167	20.80	ng/ul	0.00
21) Nitrobenzene-d5	8.67	128	115512	23.36	ng/ul	0.00
24) 2-Nitrophenol-d4	9.39	143	128820	23.08	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	9.93	165	256713	22.94	ng/ul	0.00
31) 4-Chloroaniline-d4	10.44	131	320492	18.82	ng/ul	0.00
46) Dimethylphthalate-d6	13.59	166	787852	20.85	ng/ul	0.00
49) Acenaphthylene-d8	13.86	160	985967	20.59	ng/ul	0.00
54) 4-Nitrophenol-d4	14.40	143	125162	20.34	ng/ul	0.00
60) Fluorene-d10	15.17	176	668888	20.85	ng/ul	0.00
65) 4,6-Dinitro-2-methylphenol	15.31	200	148444	22.72	ng/ul	0.00
73) Anthracene-d10	17.02	188	1040049	20.53	ng/ul	0.00
81) Pyrene-d10	19.32	212	1154234	20.92	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.13	264	1227044	21.01	ng/ul	0.00

Target Compounds

					Ovalue
2) 1,4-Dioxane	3.06	88	58923	14.189	ng/uL# 91
5) Pyridine	3.46	79	343183	34.823	ng/ul 91
6) Benzaldehyde	6.67	77	308045	41.872	ng/ul 98
8) Phenol	6.73	94	561523	38.591	ng/ul 97
10) Bis(2-Chloroethyl)ether	6.96	93	429690	37.348	ng/ul 98
12) 2-Chlorophenol	7.09	128	444209	39.599	ng/ul 99
13) 2-Methylphenol	7.97	108	427709	38.796	ng/ul 99
14) 2,2'-oxybis(1-Chloropropan	8.05	45	743220	42.886	ng/ul 96
16) Acetophenone	8.35	105	716694	37.892	ng/ul 98
17) N-Nitroso-di-n-propylamine	8.33	70	411500	42.522	ng/ul 96
18) 4-Methylphenol	8.30	108	480540	39.319	ng/ul 97
19) Hexachloroethane	8.57	117	187026	39.462	ng/ul 98
22) Nitrobenzene	8.72	77	553325	42.948	ng/ul 97
23) Isophorone	9.24	82	1106612	40.608	ng/ul 98
25) 2-Nitrophenol	9.42	139	263833	43.546	ng/ul 98
26) 2,4-Dimethylphenol	9.49	107	552542	40.417	ng/ul 98
27) Bis(2-Chloroethoxy)methane	9.73	93	649617	40.700	ng/ul 100
29) 2,4-Dichlorophenol	9.95	162	446652	40.644	ng/ul 99
30) Naphthalene	10.34	128	1492907	37.487	ng/ul 99
32) 4-Chloroaniline	10.46	127	579657	33.040	ng/ul 99
33) Hexachlorobutadiene	10.62	225	276466	37.521	ng/ul 98
34) Caprolactam	11.26	113	156598m	40.153	ng/ul

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM051821\
 Data File : BM030064.D
 Acq On : 18 May 2021 13:01
 Operator : CG/JU
 Sample : PB136458BS
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SLCS458

Manual Integrations
 APPROVED

mohammad
 5/19/2021 11:38:38 AM

Quant Time: May 18 16:46:01 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 18 16:38:21 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
35) 4-Chloro-3-methylphenol	11.60	107	518992	42.675	ng/ul	99
36) 2-Methylnaphthalene	11.96	142	1106183	38.291	ng/ul	99
37) 1-Methylnaphthalene	12.19	142	1088144	38.008	ng/ul	100
39) 1,2,4,5-Tetrachlorobenzene	12.34	216	566170	37.587	ng/ul	98
40) Hexachlorocyclopentadiene	12.32	237	277948	35.523	ng/ul	100
41) 2,4,6-Trichlorophenol	12.59	196	384150	41.822	ng/ul	99
42) 2,4,5-Trichlorophenol	12.67	196	410036	42.179	ng/ul	99
43) 1,1'-Biphenyl	13.00	154	1443241	38.088	ng/ul	98
44) 2-Chloronaphthalene	13.03	162	1126018	38.722	ng/ul	100
45) 2-Nitroaniline	13.26	65	371630	50.562	ng/ul	96
47) Dimethylphthalate	13.64	163	1492505	39.450	ng/ul	99
48) 2,6-Dinitrotoluene	13.76	165	315411	46.442	ng/ul	96
50) Acenaphthylene	13.89	152	1714085	37.015	ng/ul	98
51) 3-Nitroaniline	14.10	138	287003	37.617	ng/ul	95
52) Acenaphthene	14.23	153	1257493	38.423	ng/ul	99
53) 2,4-Dinitrophenol	14.32	184	171824	37.184	ng/ul	97
55) 4-Nitrophenol	14.42	109	187513	39.630	ng/ul	95
56) Dibenzofuran	14.57	168	1741916	38.860	ng/ul	98
57) 2,4-Dinitrotoluene	14.56	165	460007	45.772	ng/ul	88
58) 2,3,4,6-Tetrachlorophenol	14.81	232	368577	39.816	ng/ul	98
59) Diethylphthalate	15.02	149	1589296	40.277	ng/ul	100
61) Fluorene	15.23	166	1500104	39.146	ng/ul	100
62) 4-Chlorophenyl-phenylether	15.23	204	745492	39.591	ng/ul	98
63) 4-Nitroaniline	15.27	138	307955m	40.719	ng/ul	
66) 4,6-Dinitro-2-methylphenol	15.33	198	271804	42.269	ng/ul#	94
67) N-Nitrosodiphenylamine	15.44	169	1268250	38.812	ng/ul	99
68) 4-Bromophenyl-phenylether	16.12	248	448908	40.093	ng/ul	95
69) Hexachlorobenzene	16.23	284	514455	38.692	ng/ul	96
70) Atrazine	16.40	200	472519	39.194	ng/ul	99
71) Pentachlorophenol	16.58	266	298262	39.149	ng/ul	98
72) Phenanthrene	16.96	178	2304406	38.852	ng/ul	99
74) Anthracene	17.06	178	2351766	38.784	ng/ul	99
75) 1,2,3,4-Tetrachlorobenzene	12.96	216	580302	36.470	ng/uL	98
76) Pentachlorobenzene	14.49	250	567302	37.386	ng/uL	100
77) Carbazole	17.33	167	2072070	37.295	ng/ul	100
78) Di-n-butylphthalate	17.90	149	2845933	43.156	ng/ul	100
80) Fluoranthene	18.99	202	2713602	40.404	ng/ul	99
82) Pyrene	19.34	202	2799401	39.607	ng/ul	99
83) Butylbenzylphthalate	20.26	149	1318660	52.499	ng/ul	97
84) 3,3'-Dichlorobenzidine	21.04	252	1036732	42.362	ng/ul	99
85) Benzo(a)anthracene	21.10	228	2820870	40.192	ng/ul	99
86) Bis(2-ethylhexyl)phthalate	21.04	149	2165843	50.010	ng/ul	100
87) Chrysene	21.15	228	2725665	38.992	ng/ul	99
89) Di-n-octyl phthalate	21.90	149	3590263	45.548	ng/ul	100
90) Benzo(b)fluoranthene	22.62	252	2885832	43.191	ng/ul	99
91) Benzo(k)fluoranthene	22.67	252	2830398	40.293	ng/ul	100
93) Benzo(a)pyrene	23.17	252	2496895	41.147	ng/ul	99
94) Indeno(1,2,3-cd)pyrene	25.40	276	3047445	41.492	ng/ul	99
95) Dibenzo(a,h)anthracene	25.41	278	2582883	41.487	ng/ul	100
96) Benzo(g,h,i)perylene	26.05	276	2379195	39.981	ng/ul	99

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM051821\
Data File : BM030064.D
Acq On : 18 May 2021 13:01
Operator : CG/JU
Sample : PB136458BS
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SLCS458


Manual Integrations
APPROVED

mohammad
5/19/2021 11:38:38 AM

Quant Time: May 18 16:46:01 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 18 16:38:21 2021
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
--------------------	------	------	----------	------	-------	----------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

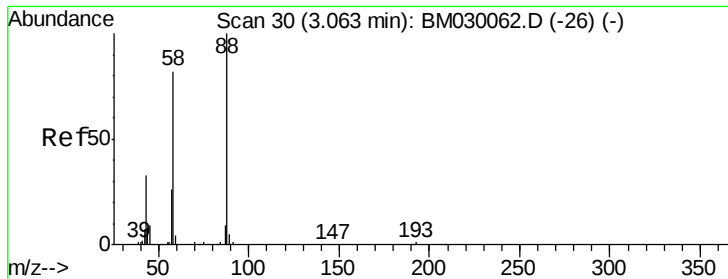

#2

1,4-Dioxane

Concen: 14.189 ng/uL

RT: 3.06 min Scan# 30

Delta R.T. -0.00 min

Lab File: BM030064.D

Acq: 18 May 2021 13:01

Instrument :

BNA_M





ClientSampleId :

SLCS458

Tot Ion:	88	Resp:	58923
Ion Ratio	Lower	Upper	
88	100		
43	39.9	26.2	39.2#
58	79.7	59.0	88.4

Manual Integrations
APPROVED

mohammad
5/19/2021 11:38:38 AM

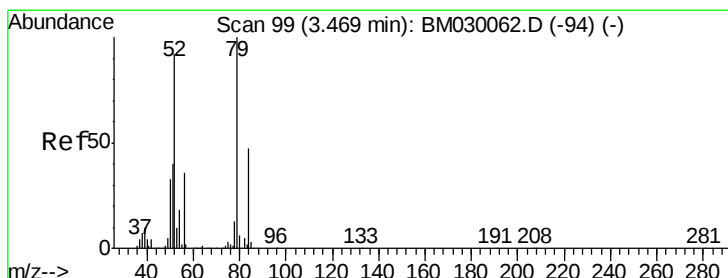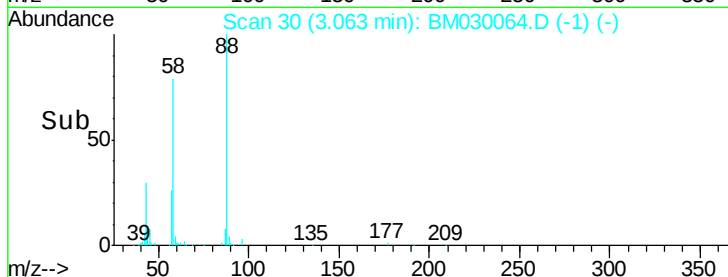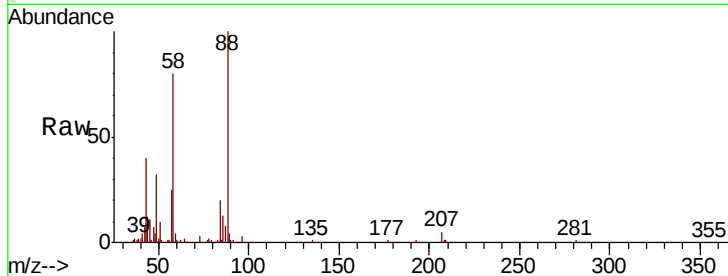

#5

Pyridine

Concen: 34.823 ng/uL




RT: 3.46 min Scan# 98


Delta R.T. -0.01 min

Lab File: BM030064.D

Acq: 18 May 2021 13:01

Tgt Ion:	79	Resp:	343183
Ion Ratio	Lower	Upper	
79	100		
52	81.0	74.6	111.8
51	39.8	32.6	48.8

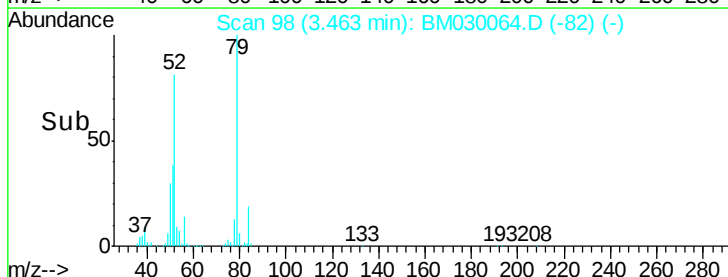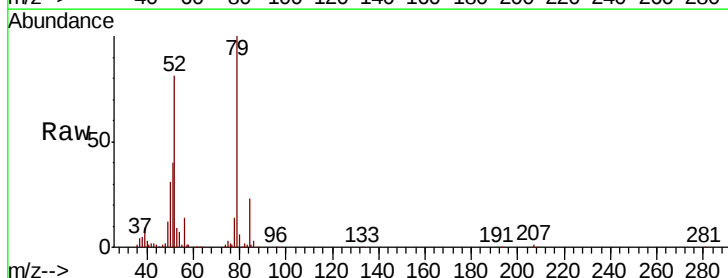



#6

Benzaldehyde

Concen: 41.872 ng/ul

RT: 6.67 min Scan# 644

Delta R.T. -0.00 min

Lab File: BM030064.D

Acq: 18 May 2021 13:01

Instrument :

BNA_M





ClientSampled :

SLCS458

Tot Ion:	77	Resp:	308045
Ion	Ratio	Lower	Upper
77	100		
105	95.0	77.7	116.5
106	91.7	72.2	108.4

Manual Integrations
APPROVED

mohammad
5/19/2021 11:38:38 AM



#8

Phenol

Concen: 38.591 ng/ul




RT: 6.73 min Scan# 654


Delta R.T. -0.00 min

Lab File: BM030064.D

Acq: 18 May 2021 13:01

Tgt Ion:	94	Resp:	561523
Ion	Ratio	Lower	Upper
94	100		
65	31.1	23.3	34.9
66	39.8	30.6	45.8









#10
Bis(2-Chloroethyl)ether
Concen: 37.348 ng/ul
RT: 6.96 min Scan# 692
Delta R.T. -0.00 min
Lab File: BM030064.D
Acq: 18 May 2021 13:01

Instrument :
BNA_M
ClientSampleId :
SLCS458

Tot Ion	Ratio	Lower	Upper
93	100		
63	84.8	66.0	99.0
95	32.3	25.7	38.5




Manual Integrations
APPROVED


mohammad
5/19/2021 11:38:38 AM

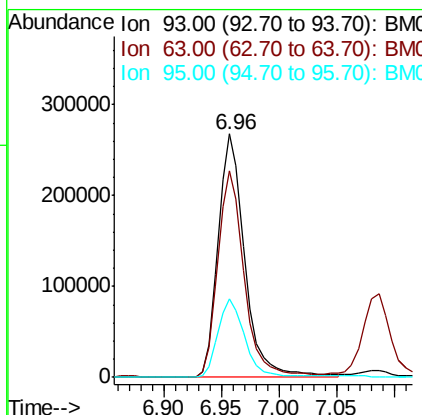

#12
2-Chlorophenol
Concen: 39.599 ng/ul
RT: 7.09 min Scan# 714
Delta R.T. -0.00 min
Lab File: BM030064.D
Acq: 18 May 2021 13:01

Tgt Ion	Ratio	Lower	Upper
128	100		
64	49.3	39.3	58.9
130	31.4	26.6	39.8



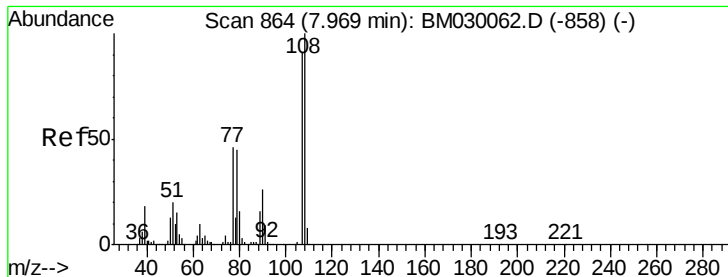

#13

2-Methylphenol

Concen: 38.796 ng/ul

RT: 7.97 min Scan# 864

Delta R.T. -0.00 min

Lab File: BM030064.D

Acq: 18 May 2021 13:01

Instrument :

BNA_M

ClientSampleId :

SLCS458

Tot Ion:108 Resp: 427709

Ion Ratio Lower Upper

108 100


107 92.9 73.8 110.6

Manual Integrations

APPROVED

mohammad

5/19/2021 11:38:38 AM

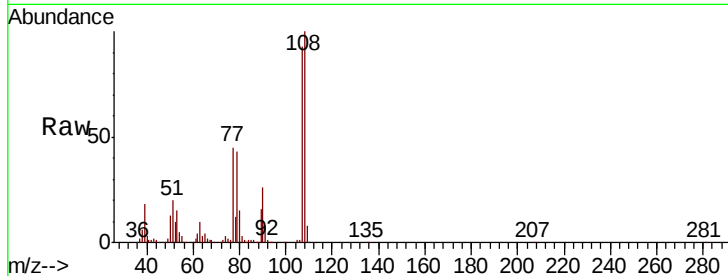

Abundance Ion 108.00 (107.70 to 108.70): E

Ion 107.00 (106.70 to 107.70): E

7.97

250000

200000



150000

100000

50000

0

Time--> 7.90 7.95 8.00 8.05 8.10

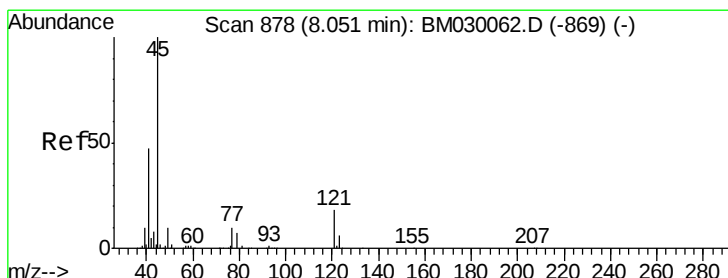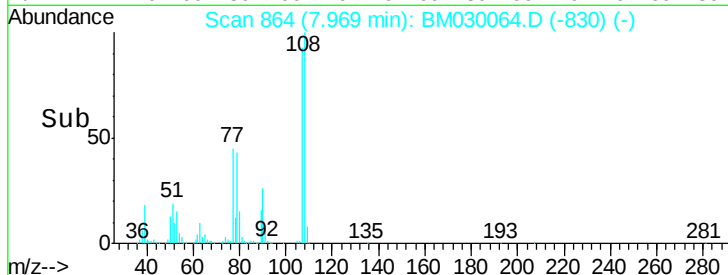

#14

2,2'-oxybis(1-chloropropane)

Concen: 42.886 ng/ul

RT: 8.05 min Scan# 878

Delta R.T. -0.00 min

Lab File: BM030064.D

Acq: 18 May 2021 13:01


Tgt Ion: 45 Resp: 743220

Ion Ratio Lower Upper

45 100

77 13.3 12.3 18.5

79 10.4 9.1 13.7

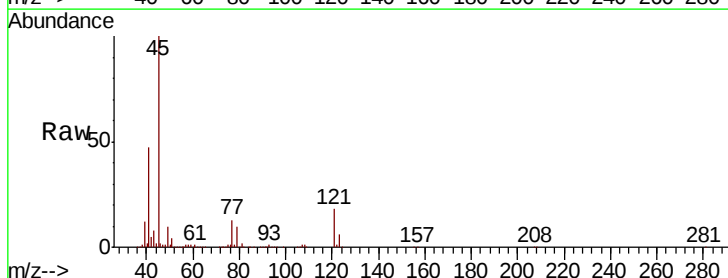

Abundance Ion 45.00 (44.70 to 45.70): BM0

Ion 77.00 (76.70 to 77.70): BM0

Ion 79.00 (78.70 to 79.70): BM0

8.05

400000


300000


200000

100000

0

Time--> 7.95 8.00 8.05 8.10

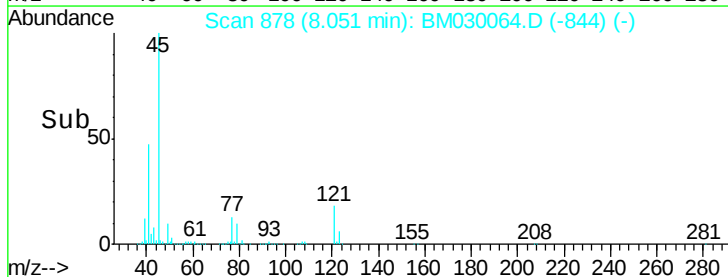

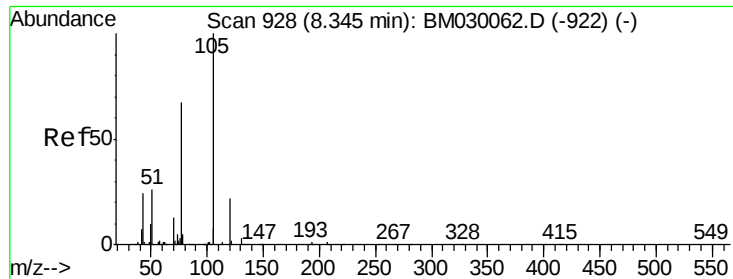





#16
Acetophenone
Concen: 37.892 ng/ul
RT: 8.35 min Scan# 928
Delta R.T. -0.00 min
Lab File: BM030064.D
Acq: 18 May 2021 13:01

Instrument :
BNA_M
ClientSampled :
SLCS458

Tot Ion:	105	Resp:	71694
Ion Ratio	Lower	Upper	
105	100		
77	81.7	64.2	96.4
51	31.1	24.3	36.5




Manual Integrations
APPROVED


mohammad
5/19/2021 11:38:38 AM

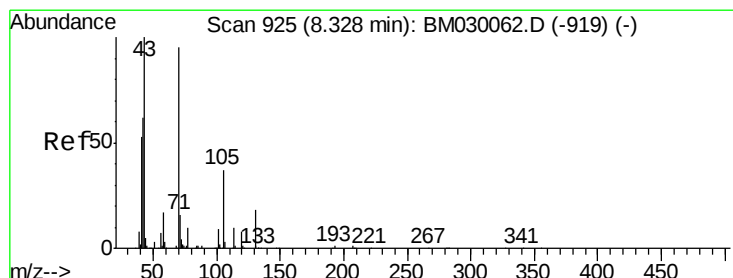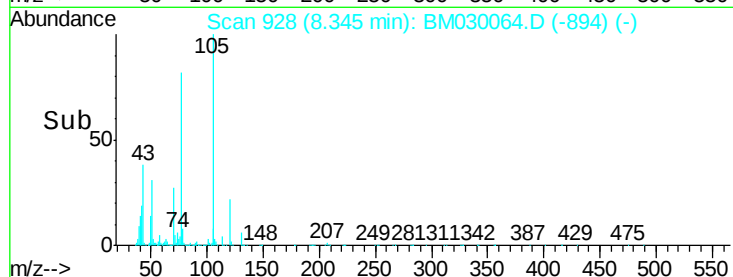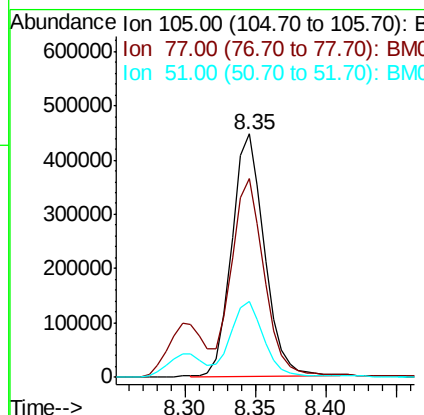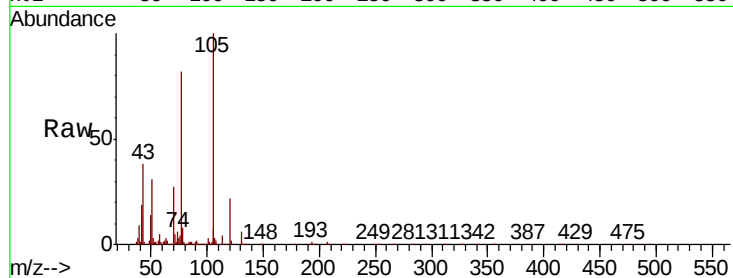

#17
N-Nitroso-di-n-propylamine
Concen: 42.522 ng/ul
RT: 8.33 min Scan# 926
Delta R.T. 0.01 min
Lab File: BM030064.D
Acq: 18 May 2021 13:01

Tgt Ion:	70	Resp:	411500
Ion Ratio	Lower	Upper	
70	100		
42	65.9	49.4	74.0
101	9.7	7.8	11.6
130	20.4	16.5	24.7

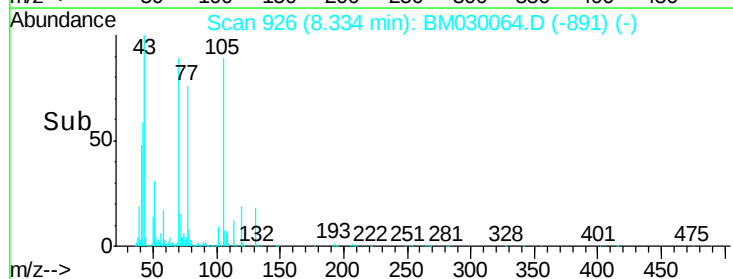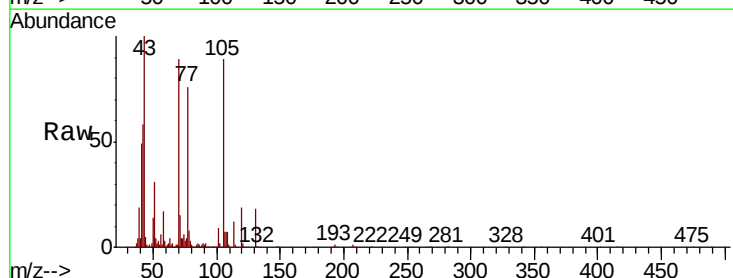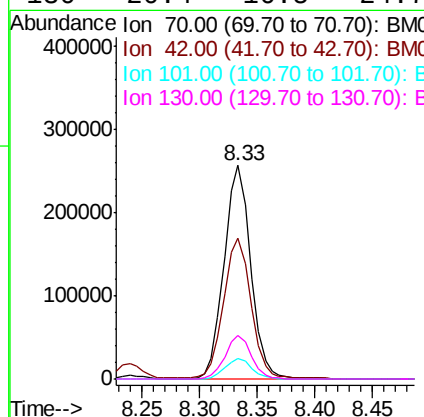

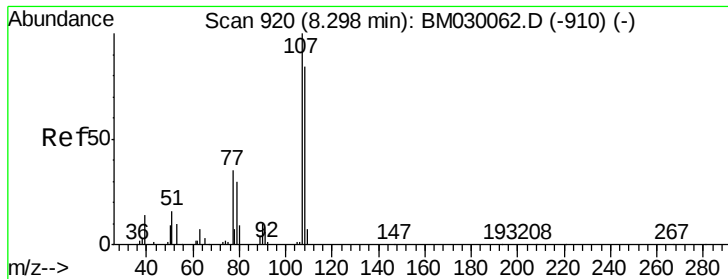





#18
4-Methylphenol
Concen: 39.319 ng/ul
RT: 8.30 min Scan# 920
Delta R.T. -0.00 min
Lab File: BM030064.D
Acq: 18 May 2021 13:01

Instrument :
BNA_M
ClientSampleId :
SLCS458

Tot Ion	Ratio	Resp	Lower	Upper
108	100	480540		
107	114.9	89.4	134.0	




Manual Integrations
APPROVED


mohammad
5/19/2021 11:38:38 AM

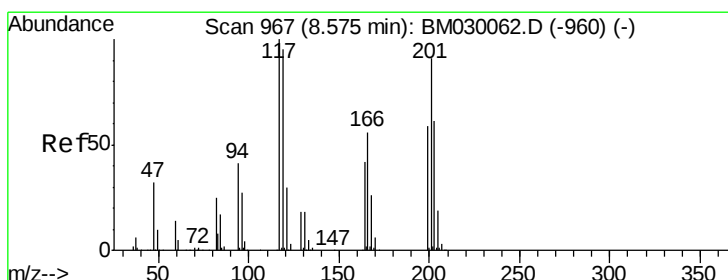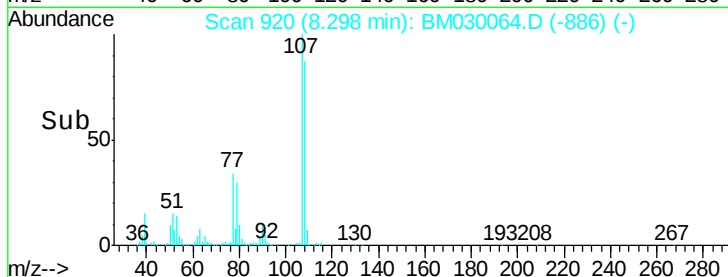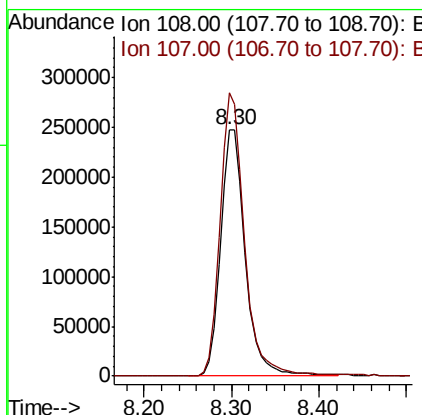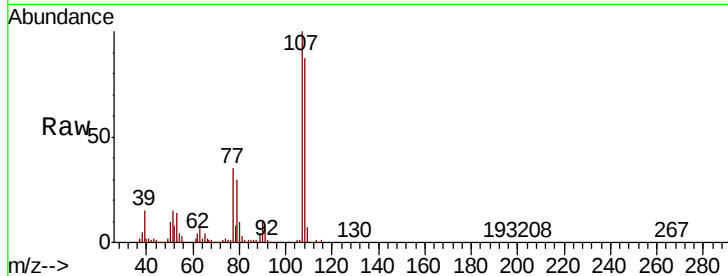

#19
Hexachloroethane
Concen: 39.462 ng/ul
RT: 8.57 min Scan# 967
Delta R.T. -0.00 min
Lab File: BM030064.D
Acq: 18 May 2021 13:01

Tgt Ion	Ratio	Resp	Lower	Upper
117	100	187026		
201	96.7	79.4	119.2	
199	59.5	48.0	72.0	

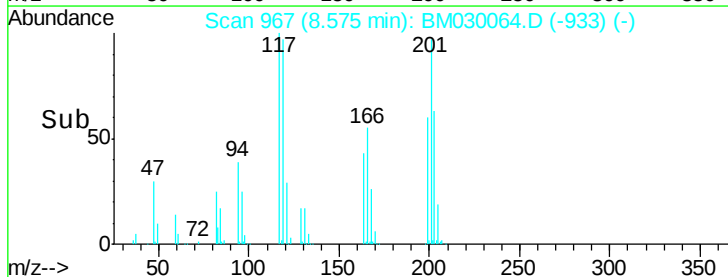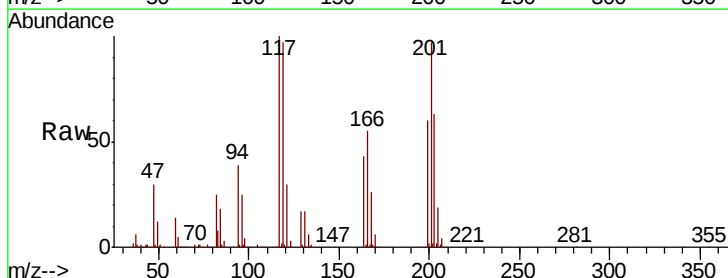







#22
Nitrobenzene
Concen: 42.948 ng/ul
RT: 8.72 min Scan# 991
Delta R.T. -0.00 min
Lab File: BM030064.D
Acq: 18 May 2021 13:01

Instrument :
BNA_M
ClientSampleId :
SLCS458

Tot Ion	Ratio	Lower	Upper
77	100		
123	41.5	35.0	52.6
65	13.6	10.3	15.5




Manual Integrations
APPROVED


mohammad
5/19/2021 11:38:38 AM



#23
Isophorone
Concen: 40.608 ng/ul
RT: 9.24 min Scan# 1080
Delta R.T. -0.00 min
Lab File: BM030064.D
Acq: 18 May 2021 13:01

Tgt Ion	Ratio	Lower	Upper
82	100		
95	6.9	5.5	8.3
138	16.1	13.8	20.6





#25

2-Nitrophenol

Concen: 43.546 ng/ul

RT: 9.42 min Scan# 1111

Delta R.T. -0.00 min

Lab File: BM030064.D

Acq: 18 May 2021 13:01

Instrument :

BNA_M





ClientSampled :

SLCS458

Tot Ion:	139	Resp:	263833
Ion Ratio	Lower	Upper	
139	100		
65	57.0	44.6	67.0
109	31.9	24.4	36.6

Manual Integrations
APPROVED

mohammad
5/19/2021 11:38:38 AM

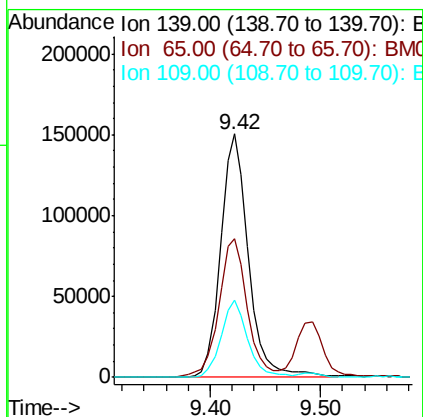

#26

2,4-Dimethylphenol

Concen: 40.417 ng/ul




RT: 9.49 min Scan# 1123


Delta R.T. 0.01 min

Lab File: BM030064.D

Acq: 18 May 2021 13:01

Tgt Ion:	107	Resp:	552542
Ion Ratio	Lower	Upper	
107	100		
121	51.1	40.7	61.1
122	83.5	68.9	103.3

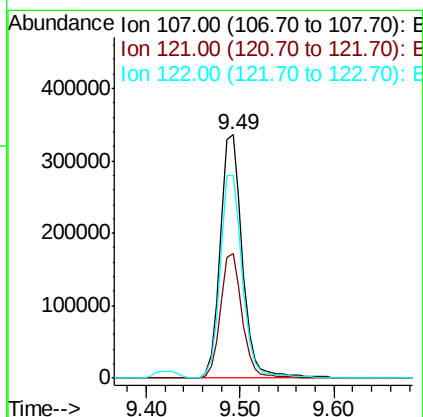



#27

Bis(2-Chloroethoxy)methane

Concen: 40.700 ng/ul

RT: 9.73 min Scan# 1163

Delta R.T. 0.01 min

Lab File: BM030064.D

Acq: 18 May 2021 13:01

Instrument :

BNA_M





ClientSampled :

SLCS458

Tot Ion:	93	Resp:	649617
Ion Ratio	Lower	Upper	
93	100		
95	31.7	25.3	37.9
123	10.6	8.8	13.2

Manual Integrations
APPROVED

mohammad
5/19/2021 11:38:38 AM



#29

2,4-Dichlorophenol

Concen: 40.644 ng/ul




RT: 9.95 min Scan# 1201


Delta R.T. -0.00 min

Lab File: BM030064.D

Acq: 18 May 2021 13:01

Tgt Ion:	162	Resp:	446652
Ion Ratio	Lower	Upper	
162	100		
164	63.4	51.2	76.8
98	37.1	29.7	44.5









#30
Naphthalene
Concen: 37.487 ng/ul
RT: 10.34 min Scan# 1267
Delta R.T. -0.00 min
Lab File: BM030064.D
Acq: 18 May 2021 13:01

Instrument :
BNA_M
ClientSampleId :
SLCS458

Tot Ion	Ratio	Lower	Upper
128	100		
129	11.0	8.5	12.7
127	13.1	10.4	15.6




Manual Integrations
APPROVED


mohammad
5/19/2021 11:38:38 AM

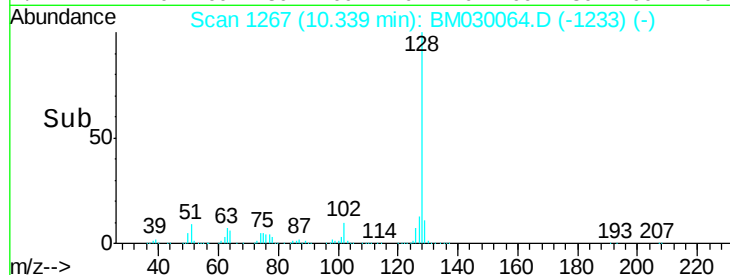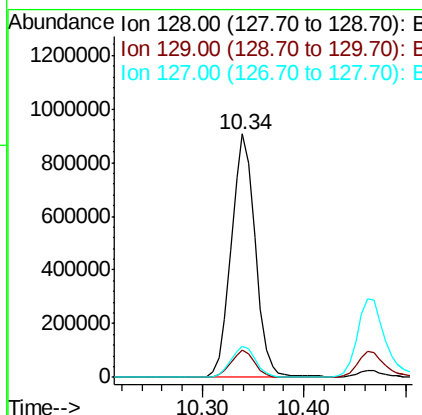

#32
4-Chloroaniline
Concen: 33.040 ng/ul
RT: 10.46 min Scan# 1288
Delta R.T. -0.01 min
Lab File: BM030064.D
Acq: 18 May 2021 13:01

Tgt Ion	Ratio	Lower	Upper
127	100		
129	32.4	26.3	39.5









#33
Hexachlorobutadiene
Concen: 37.521 ng/ul
RT: 10.62 min Scan# 1315
Delta R.T. -0.00 min
Lab File: BM030064.D
Acq: 18 May 2021 13:01

Instrument :
BNA_M
ClientSampled :
SLCS458

Tot Ion	Ratio	Resp	Lower	Upper
225	100	276466		
223	63.5		53.0	79.4
227	65.1		51.2	76.8




Manual Integrations
APPROVED


mohammad
5/19/2021 11:38:38 AM

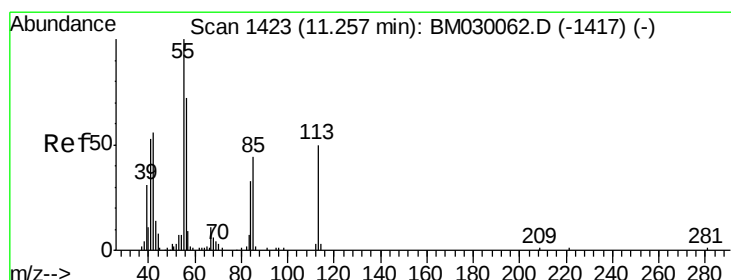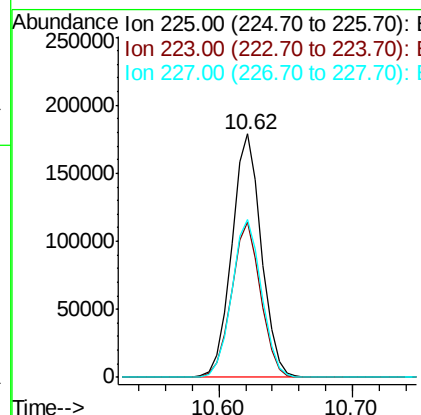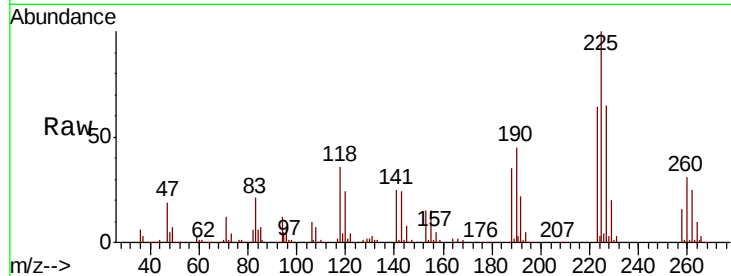

#34
Caprolactam
Concen: 40.153 ng/ul m
RT: 11.26 min Scan# 1424
Delta R.T. 0.01 min
Lab File: BM030064.D
Acq: 18 May 2021 13:01

Tgt Ion	Ratio	Resp	Lower	Upper
113	100	156598		
55	187.0		138.9	208.3
56	135.5		105.4	158.2

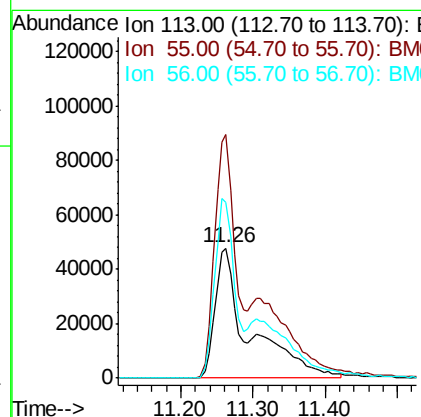







#35
4-Chloro-3-methylphenol
Concen: 42.675 ng/ul
RT: 11.60 min Scan# 1482
Delta R.T. 0.01 min
Lab File: BM030064.D
Acq: 18 May 2021 13:01

Instrument :
BNA_M
ClientSampleId :
SLCS458

Tot Ion	Ratio	Lower	Upper
107	100		
144	25.8	21.3	31.9
142	81.4	64.6	97.0




Manual Integrations
APPROVED


mohammad
5/19/2021 11:38:38 AM

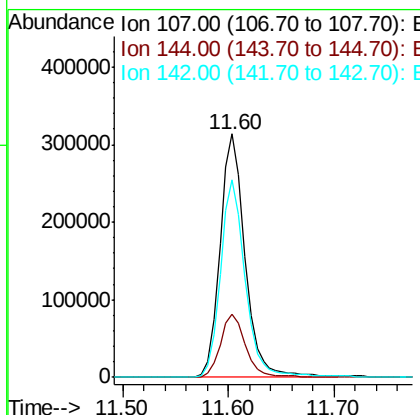

#36
2-Methylnaphthalene
Concen: 38.291 ng/ul
RT: 11.96 min Scan# 1543
Delta R.T. -0.00 min
Lab File: BM030064.D
Acq: 18 May 2021 13:01

Tgt Ion	Ratio	Lower	Upper
142	100		
141	89.2	72.1	108.1





#37

1-Methylnaphthalene

Concen: 38.008 ng/ul

RT: 12.19 min Scan# 1581

Delta R.T. -0.00 min

Lab File: BM030064.D

Acq: 18 May 2021 13:01

Instrument :

BNA_M

ClientSampleId :

SLCS458

Tot Ion:142 Resp: 1088144

Ion Ratio Lower Upper

142 100


141 91.5 72.9 109.3

116 3.9 3.0 4.6

Manual Integrations
APPROVED

mohammad

5/19/2021 11:38:38 AM




Abundance



Ion 142.00 (141.70 to 142.70): E

Ion 141.00 (140.70 to 141.70): E

Ion 116.00 (115.70 to 116.70): E

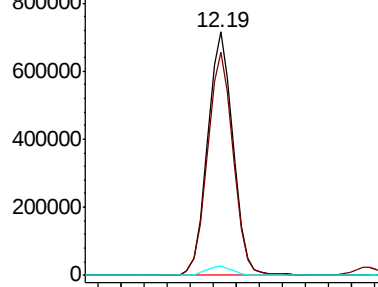

Time-->



#39

1,2,4,5-Tetrachlorobenzene

Concen: 37.587 ng/ul

RT: 12.34 min Scan# 1607

Delta R.T. -0.00 min

Lab File: BM030064.D

Acq: 18 May 2021 13:01

Tgt Ion:216 Resp: 566170

Ion Ratio Lower Upper

216 100

214 78.5 61.9 92.9

179 21.7 16.8 25.2

108 18.7 14.1 21.1


Abundance

Ion 216.00 (215.70 to 216.70): E



Ion 214.00 (213.70 to 214.70): E


Ion 179.00 (178.70 to 179.70): E

Ion 108.00 (107.70 to 108.70): E

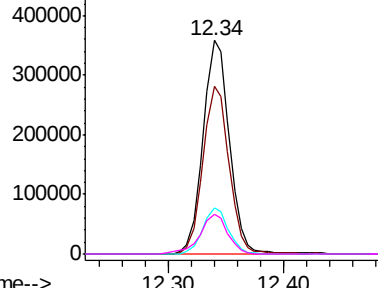

Time-->









#40
Hexachlorocyclopentadiene
Concen: 35.523 ng/ul
RT: 12.32 min Scan# 1603
Delta R.T. -0.00 min
Lab File: BM030064.D
Acq: 18 May 2021 13:01

Instrument :
BNA_M
ClientSampleId :
SLCS458

Tot Ion	Ratio	Resp	Lower	Upper
237	100	277948		
235	62.3		50.0	75.0
272	12.6		10.2	15.2




Manual Integrations
APPROVED


mohammad
5/19/2021 11:38:38 AM

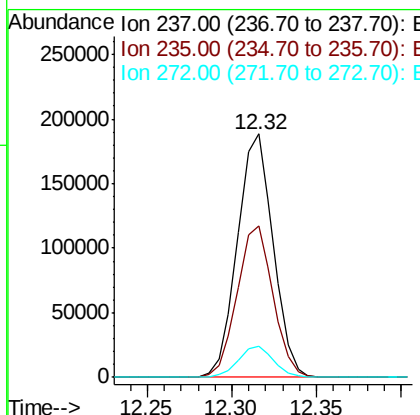

#41
2,4,6-Trichlorophenol
Concen: 41.822 ng/ul
RT: 12.59 min Scan# 1650
Delta R.T. -0.00 min
Lab File: BM030064.D
Acq: 18 May 2021 13:01

Tgt Ion	Ratio	Resp	Lower	Upper
196	100	384150		
198	95.4		77.0	115.4
200	31.6		23.7	35.5









#42
 2,4,5-Trichlorophenol
 Concen: 42.179 ng/ul
 RT: 12.67 min Scan# 1663
 Delta R.T. -0.00 min
 Lab File: BM030064.D
 Acq: 18 May 2021 13:01

Instrument :
 BNA_M
 ClientSampleId :
 SLCS458

Tot Ion	Ratio	Resp	Lower	Upper
196	100	410036		
198	95.6	75.3	112.9	
200	30.2	24.6	36.8	




Manual Integrations
 APPROVED


mohammad
 5/19/2021 11:38:38 AM



#43
 1,1'-Biphenyl
 Concen: 38.088 ng/ul
 RT: 13.00 min Scan# 1719
 Delta R.T. -0.00 min
 Lab File: BM030064.D
 Acq: 18 May 2021 13:01

Tgt Ion	Ratio	Resp	Lower	Upper
154	100	1443241		
153	40.4	33.3	49.9	
76	13.3	10.3	15.5	





#44

2-Chloronaphthalene

Concen: 38.722 ng/ul

RT: 13.03 min Scan# 1725

Delta R.T. -0.00 min

Lab File: BM030064.D

Acq: 18 May 2021 13:01

Instrument :

BNA_M

ClientSampleId :

SLCS458

Tot Ion: 162 Resp: 1126018

Ion Ratio Lower Upper

162 100


164 32.3 25.8 38.6

127 38.6 31.0 46.6

Manual Integrations
APPROVED

mohammad

5/19/2021 11:38:38 AM



Abundance Ion 162.00 (161.70 to 162.70): E

Ion 164.00 (163.70 to 164.70): E

Ion 127.00 (126.70 to 127.70): E

1000000

800000

600000



400000

200000

0

13.03

Time-->



#45

2-Nitroaniline

Concen: 50.562 ng/ul

RT: 13.26 min Scan# 1763

Delta R.T. -0.01 min

Lab File: BM030064.D

Acq: 18 May 2021 13:01


Tgt Ion: 65 Resp: 371630

Ion Ratio Lower Upper

65 100

92 65.7 53.2 79.8

138 96.0 81.1 121.7



Abundance Ion 65.00 (64.70 to 65.70): BM0

Ion 92.00 (91.70 to 92.70): BM0

Ion 138.00 (137.70 to 138.70): E

300000

250000

200000

150000


100000


50000

0

13.26

Time-->





#47

Dimethylphthalate

Concen: 39.450 ng/ul

RT: 13.64 min Scan# 1828

Delta R.T. -0.00 min

Lab File: BM030064.D

Acq: 18 May 2021 13:01

Instrument :

BNA_M

ClientSampleId :

SLCS458

Tot Ion:163 Resp: 1492505

Ion Ratio Lower Upper


163 100

194 3.7 3.4 5.0




164 10.1 7.8 11.8

Manual Integrations
APPROVED

mohammad
5/19/2021 11:38:38 AM



Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

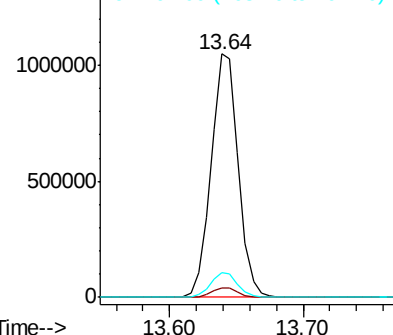

#48

2,6-Dinitrotoluene

Concen: 46.442 ng/ul

RT: 13.76 min Scan# 1849

Delta R.T. -0.00 min

Lab File: BM030064.D

Acq: 18 May 2021 13:01


Tgt Ion:165 Resp: 315411

Ion Ratio Lower Upper



165 100


89 62.0 52.5 78.7

121 22.4 18.8 28.2



Abundance Ion 165.00 (164.70 to 165.70): E
Ion 89.00 (88.70 to 89.70): BM
Ion 121.00 (120.70 to 121.70): E

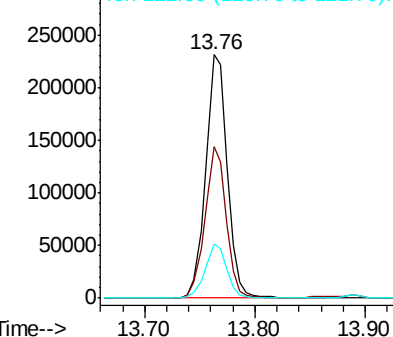







#50
Acenaphthylene
Concen: 37.015 ng/ul
RT: 13.89 min Scan# 1870
Delta R.T. -0.00 min
Lab File: BM030064.D
Acq: 18 May 2021 13:01

Instrument :
BNA_M
ClientSampleId :
SLCS458

Tot Ion	Ratio	Lower	Upper
152	100		
151	19.7	16.6	24.8
153	12.9	10.6	16.0




Manual Integrations
APPROVED


mohammad
5/19/2021 11:38:38 AM



#51
3-Nitroaniline
Concen: 37.617 ng/ul
RT: 14.10 min Scan# 1906
Delta R.T. -0.00 min
Lab File: BM030064.D
Acq: 18 May 2021 13:01

Tgt Ion	Ratio	Lower	Upper
138	100		
108	9.6	8.5	12.7
92	119.7	100.1	150.1





#52

Acenaphthene

Concen: 38.423 ng/ul

RT: 14.23 min Scan# 1929

Delta R.T. -0.00 min

Lab File: BM030064.D

Acq: 18 May 2021 13:01

Instrument :

BNA_M

ClientSampleId :

SLCS458

Tot Ion:153 Resp: 1257493

Ion Ratio Lower Upper

153 100


152 46.6 37.7 56.5

154 88.8 70.2 105.4

Manual Integrations
APPROVED

mohammad

5/19/2021 11:38:38 AM






Abundance

Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E

Ion 154.00 (153.70 to 154.70): E

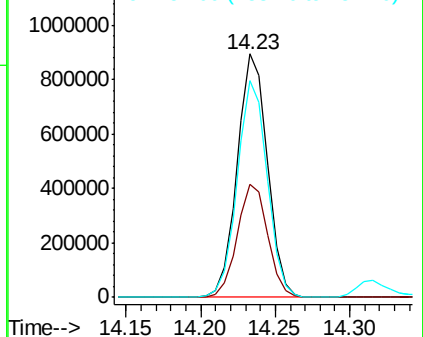

#53

2,4-Dinitrophenol

Concen: 37.184 ng/ul

RT: 14.32 min Scan# 1943

Delta R.T. -0.00 min

Lab File: BM030064.D

Acq: 18 May 2021 13:01


Tgt Ion:184 Resp: 171824

Ion Ratio Lower Upper

184 100

63 74.2 57.2 85.8

154 60.0 45.8 68.6






Abundance

Ion 184.00 (183.70 to 184.70): E

Ion 63.00 (62.70 to 63.70): BM

Ion 154.00 (153.70 to 154.70): E

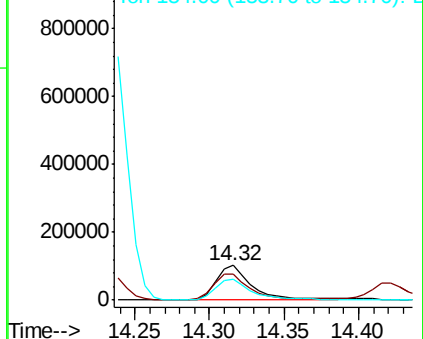







#55
4-Nitrophenol
Concen: 39.630 ng/ul
RT: 14.42 min Scan# 1961
Delta R.T. -0.00 min
Lab File: BM030064.D
Acq: 18 May 2021 13:01

Instrument :
BNA_M
ClientSampleId :
SLCS458

Tot Ion	Ratio	Resp	Lower	Upper
109	100			
139	135.0	102.1	153.1	
65	146.9	114.6	172.0	




Manual Integrations
APPROVED


mohammad
5/19/2021 11:38:38 AM

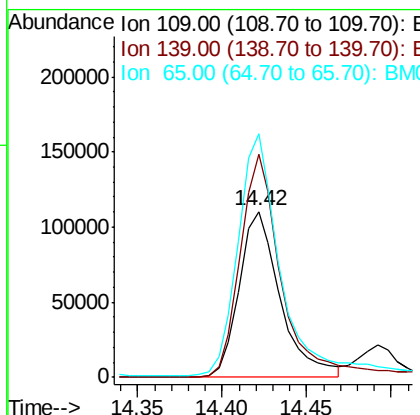

#56
Dibenzofuran
Concen: 38.860 ng/ul
RT: 14.57 min Scan# 1987
Delta R.T. -0.00 min
Lab File: BM030064.D
Acq: 18 May 2021 13:01

Tgt Ion	Ratio	Resp	Lower	Upper
168	100			
139	38.2	29.8	44.6	









#57
2,4-Dinitrotoluene
Concen: 45.772 ng/ul
RT: 14.56 min Scan# 1985
Delta R.T. -0.00 min
Lab File: BM030064.D
Acq: 18 May 2021 13:01

Instrument :
BNA_M
ClientSampleId :
SLCS458

Tot Ion	Ratio	Resp	Lower	Upper
165	100	460007		
63	59.4		40.7	61.1
182	3.0		2.1	3.1




Manual Integrations
APPROVED


mohammad
5/19/2021 11:38:38 AM

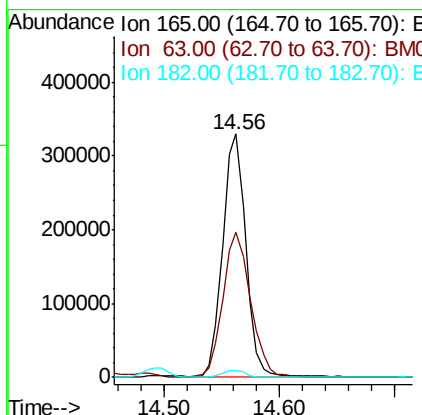

#58
2,3,4,6-Tetrachlorophenol
Concen: 39.816 ng/ul
RT: 14.81 min Scan# 2027
Delta R.T. -0.00 min
Lab File: BM030064.D
Acq: 18 May 2021 13:01

Tgt Ion	Ratio	Resp	Lower	Upper
232	100	368577		
131	45.7		38.3	57.5
130	2.3		2.0	3.0
166	31.5		24.6	37.0









#59
Diethylphthalate
Concen: 40.277 ng/ul
RT: 15.02 min Scan# 2062
Delta R.T. 0.01 min
Lab File: BM030064.D
Acq: 18 May 2021 13:01

Instrument :
BNA_M
ClientSampleId :
SLCS458

Tot Ion	Ratio	Lower	Upper
149	100		
177	21.6	17.2	25.8
150	12.5	10.0	15.0




Manual Integrations
APPROVED


mohammad
5/19/2021 11:38:38 AM



#61
Fluorene
Concen: 39.146 ng/ul
RT: 15.23 min Scan# 2098
Delta R.T. 0.01 min
Lab File: BM030064.D
Acq: 18 May 2021 13:01

Tgt Ion	Ratio	Lower	Upper
166	100		
165	97.7	78.4	117.6
167	13.3	10.9	16.3









#62
4-Chlorophenyl-phenylether
Concen: 39.591 ng/ul
RT: 15.23 min Scan# 2098
Delta R.T. 0.01 min
Lab File: BM030064.D
Acq: 18 May 2021 13:01

Instrument :
BNA_M
ClientSampleId :
SLCS458

Tot Ion	Ratio	Lower	Upper
204	100		
206	32.4	26.2	39.2
141	56.3	47.2	70.8




Manual Integrations
APPROVED


mohammad
5/19/2021 11:38:38 AM

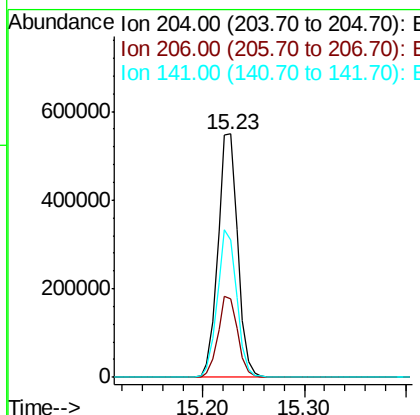

#63
4-Nitroaniline
Concen: 40.719 ng/ul m
RT: 15.27 min Scan# 2105
Delta R.T. -0.00 min
Lab File: BM030064.D
Acq: 18 May 2021 13:01

Tgt Ion	Ratio	Lower	Upper
138	100		
92	54.2	44.8	67.2
108	83.1	65.3	97.9






#66
 4,6-Dinitro-2-methylphenol
 Concen: 42.269 ng/ul
 RT: 15.33 min Scan# 2115
 Delta R.T. 0.01 min
 Lab File: BM030064.D
 Acq: 18 May 2021 13:01

Instrument :
 BNA_M
 ClientSampleId :
 SLCS458

Tot Ion	Ratio	Lower	Upper
198	100		
182	3.7	4.3	6.5#
77	25.7	23.0	34.4

Manual Integrations
 APPROVED

mohammad
 5/19/2021 11:38:38 AM



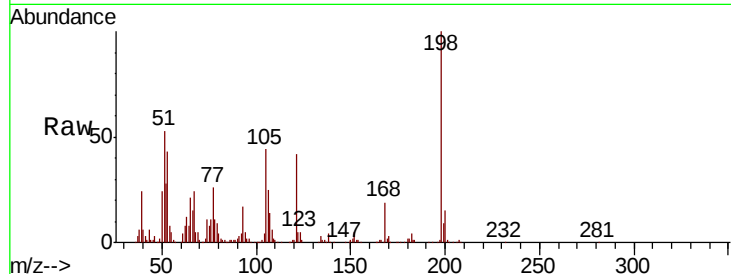


Abundance

Ion 198.00 (197.70 to 198.70): E


Ion 182.00 (181.70 to 182.70): E

Ion 77.00 (76.70 to 77.70): E

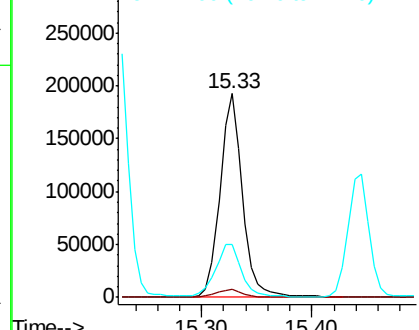

#67
 N-Nitrosodiphenylamine
 Concen: 38.812 ng/ul
 RT: 15.44 min Scan# 2135
 Delta R.T. 0.01 min
 Lab File: BM030064.D
 Acq: 18 May 2021 13:01

Tgt Ion	Ratio	Lower	Upper
169	100		
168	65.9	53.0	79.4
167	36.1	27.8	41.6






Abundance

Ion 169.00 (168.70 to 169.70): E

Ion 168.00 (167.70 to 168.70): E

Ion 167.00 (166.70 to 167.70): E

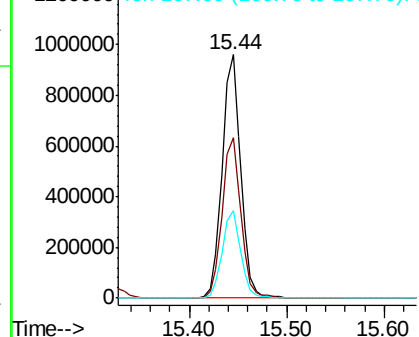







#68
 4-Bromophenyl-phenylether
 Concen: 40.093 ng/ul
 RT: 16.12 min Scan# 2249
 Delta R.T. -0.00 min
 Lab File: BM030064.D
 Acq: 18 May 2021 13:01

Instrument :
 BNA_M
 ClientSampleId :
 SLCS458

Tot Ion	Ratio	Lower	Upper
248	100		
250	99.1	77.5	116.3
141	76.0	55.1	82.7




Manual Integrations
 APPROVED


mohammad
 5/19/2021 11:38:38 AM



#69
 Hexachlorobenzene
 Concen: 38.692 ng/ul
 RT: 16.23 min Scan# 2268
 Delta R.T. -0.00 min
 Lab File: BM030064.D
 Acq: 18 May 2021 13:01

Tgt Ion	Ratio	Lower	Upper
284	100		
142	37.8	26.4	39.6
249	30.6	24.5	36.7









#70
Atrazine
Concen: 39.194 ng/ul
RT: 16.40 min Scan# 2298
Delta R.T. -0.00 min
Lab File: BM030064.D
Acq: 18 May 2021 13:01

Instrument :
BNA_M
ClientSampled :
SLCS458

Tot Ion	Ratio	Resp	Lower	Upper
200	100	472519		
173	26.2	20.5	30.7	
215	47.9	38.2	57.2	




Manual Integrations
APPROVED


mohammad
5/19/2021 11:38:38 AM



#71
Pentachlorophenol
Concen: 39.149 ng/ul
RT: 16.58 min Scan# 2328
Delta R.T. -0.00 min
Lab File: BM030064.D
Acq: 18 May 2021 13:01

Tgt Ion	Ratio	Resp	Lower	Upper
266	100	298262		
264	61.2	49.8	74.8	
268	63.1	51.9	77.9	









#72
Phenanthrene
Concen: 38.852 ng/ul
RT: 16.96 min Scan# 2393
Delta R.T. -0.00 min
Lab File: BM030064.D
Acq: 18 May 2021 13:01

Instrument :
BNA_M
ClientSampleId :
SLCS458

Tot Ion:178 Resp: 2304406
Ion Ratio Lower Upper
178 100
179 15.4 12.2 18.4
176 19.1 15.0 22.4




Manual Integrations
APPROVED


mohammad
5/19/2021 11:38:38 AM

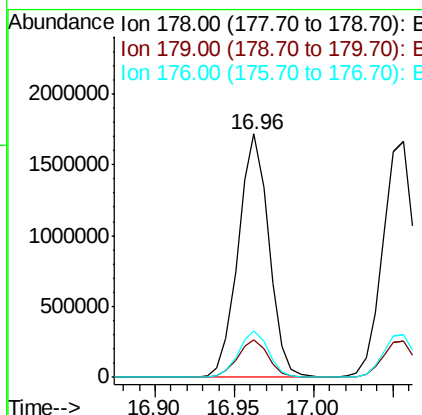

#74
Anthracene
Concen: 38.784 ng/ul
RT: 17.06 min Scan# 2409
Delta R.T. 0.01 min
Lab File: BM030064.D
Acq: 18 May 2021 13:01

Tgt Ion:178 Resp: 2351766
Ion Ratio Lower Upper
178 100
179 15.2 12.2 18.2
176 18.1 14.9 22.3





#75

1,2,3,4-Tetrachlorobenzene

Concen: 36.470 ng/uL

RT: 12.96 min Scan# 1712

Delta R.T. -0.00 min

Lab File: BM030064.D

Acq: 18 May 2021 13:01

Instrument :

BNA_M





ClientSampled :

SLCS458

Tot Ion:	216	Resp:	580302
Ion Ratio		Lower	Upper
216	100		
214	77.6	63.9	95.9
218	48.7	39.7	59.5

Manual Integrations
APPROVED

mohammad
5/19/2021 11:38:38 AM

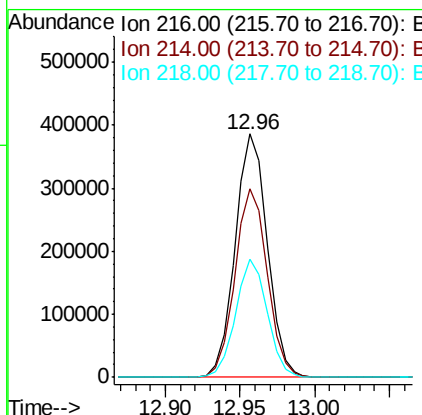

#76

Pentachlorobenzene

Concen: 37.386 ng/uL




RT: 14.49 min Scan# 1973


Delta R.T. -0.00 min

Lab File: BM030064.D

Acq: 18 May 2021 13:01

Tgt Ion:	250	Resp:	567302
Ion Ratio		Lower	Upper
250	100		
248	63.4	51.3	76.9
252	64.4	51.5	77.3









#77
 Carbazole
 Concen: 37.295 ng/ul
 RT: 17.33 min Scan# 2456
 Delta R.T. 0.01 min
 Lab File: BM030064.D
 Acq: 18 May 2021 13:01

Instrument :
 BNA_M
 ClientSampleId :
 SLCS458

Tot Ion	Ratio	Lower	Upper
167	100		
166	21.8	17.6	26.4
139	12.9	10.2	15.2




Manual Integrations
 APPROVED


mohammad
 5/19/2021 11:38:38 AM

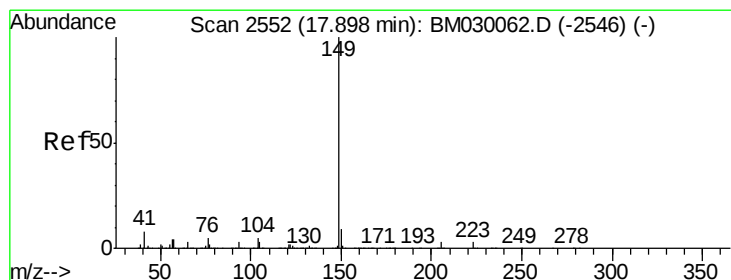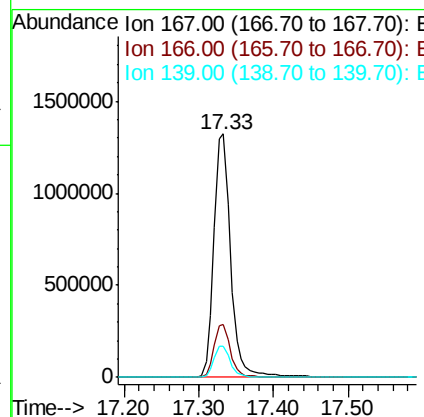

#78
 Di-n-butylphthalate
 Concen: 43.156 ng/ul
 RT: 17.90 min Scan# 2552
 Delta R.T. -0.00 min
 Lab File: BM030064.D
 Acq: 18 May 2021 13:01

Tgt Ion	Ratio	Lower	Upper
149	100		
150	9.2	7.4	11.0
104	5.4	4.2	6.2

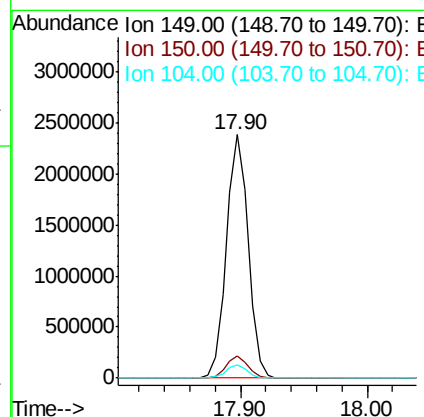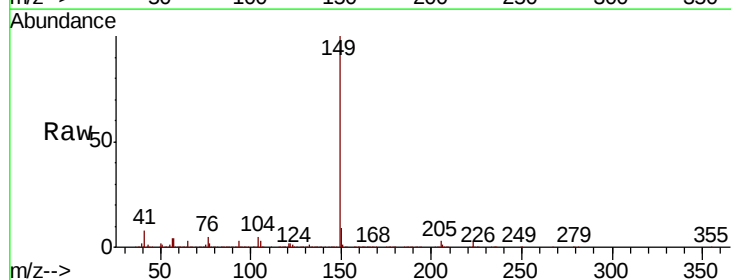







#80
Fluoranthene
Concen: 40.404 ng/ul
RT: 18.99 min Scan# 2737
Delta R.T. 0.01 min
Lab File: BM030064.D
Acq: 18 May 2021 13:01

Instrument :
BNA_M
ClientSampleId :
SLCS458

Tot Ion	Ratio	Lower	Upper
202	100		
101	11.9	9.0	13.4
100	9.0	7.0	10.6




Manual Integrations
APPROVED


mohammad
5/19/2021 11:38:38 AM

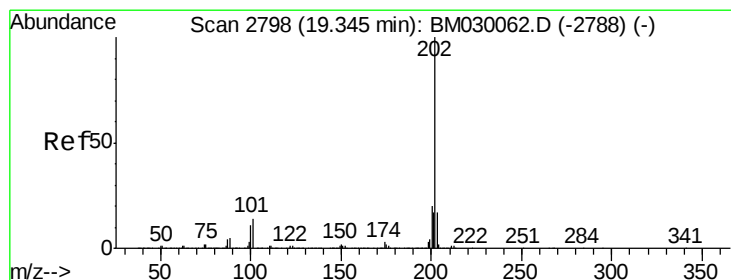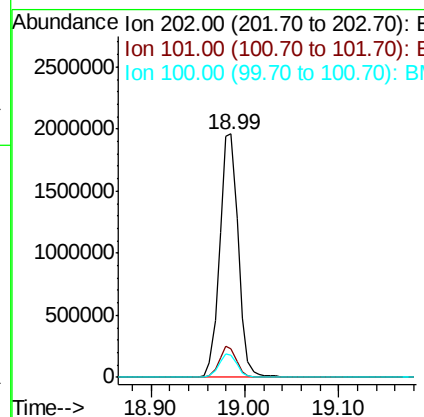

#82
Pyrene
Concen: 39.607 ng/ul
RT: 19.34 min Scan# 2798
Delta R.T. -0.00 min
Lab File: BM030064.D
Acq: 18 May 2021 13:01

Tgt Ion	Ratio	Lower	Upper
202	100		
101	15.0	11.8	17.6
100	12.4	9.2	13.8

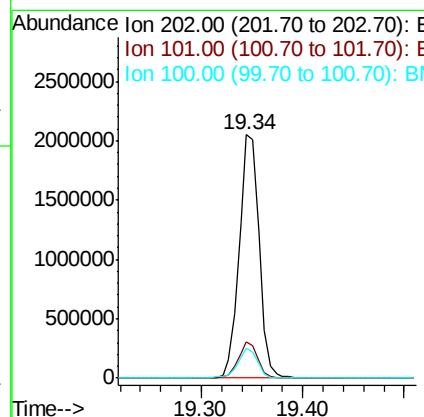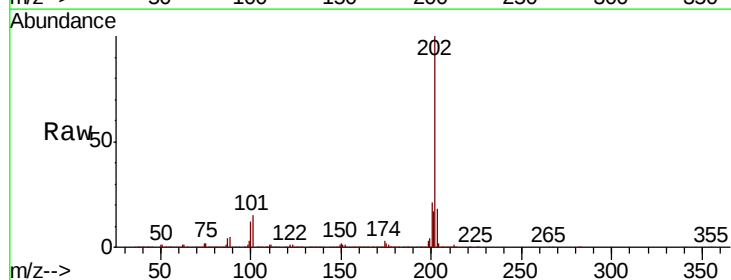







#83
Butylbenzylphthalate
Concen: 52.499 ng/ul
RT: 20.26 min Scan# 2954
Delta R.T. -0.00 min
Lab File: BM030064.D
Acq: 18 May 2021 13:01

Instrument :
BNA_M
ClientSampleId :
SLCS458

Tot Ion	Ratio	Lower	Upper
149	100		
91	73.2	60.6	91.0
206	20.4	15.4	23.0




Manual Integrations
APPROVED


mohammad
5/19/2021 11:38:38 AM

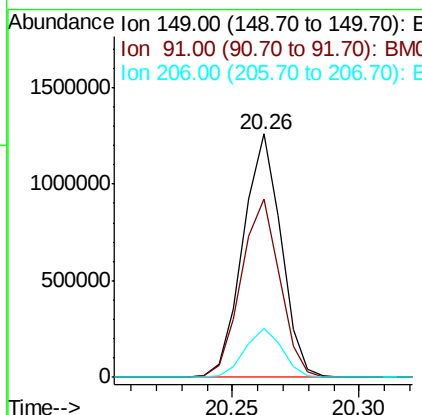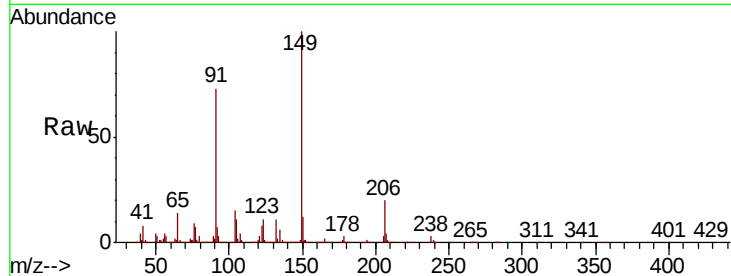

#84
3,3'-Dichlorobenzidine
Concen: 42.362 ng/ul
RT: 21.04 min Scan# 3086
Delta R.T. -0.00 min
Lab File: BM030064.D
Acq: 18 May 2021 13:01

Tgt Ion	Ratio	Lower	Upper
252	100		
254	64.9	51.0	76.6
126	11.8	9.4	14.0









#85
Benzo(a)anthracene
Concen: 40.192 ng/ul
RT: 21.10 min Scan# 3096
Delta R.T. -0.00 min
Lab File: BM030064.D
Acq: 18 May 2021 13:01

Instrument :
BNA_M
ClientSampled :
SLCS458

Tot Ion:228 Resp: 2820870
Ion Ratio Lower Upper
228 100
229 19.8 15.9 23.9
226 27.1 21.4 32.0




Manual Integrations
APPROVED


mohammad
5/19/2021 11:38:38 AM

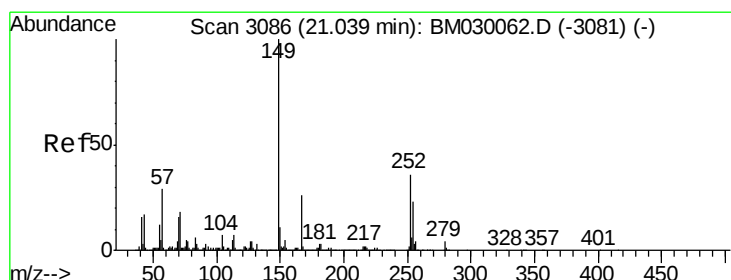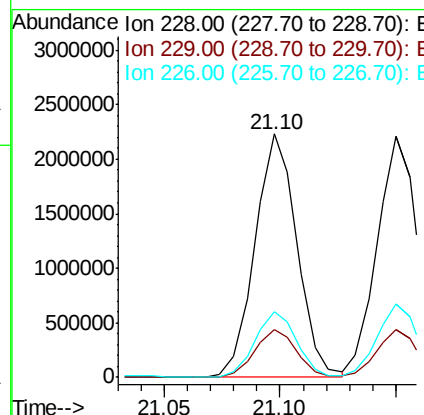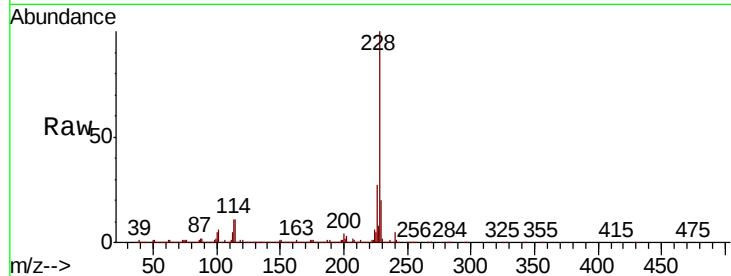

#86
Bis(2-ethylhexyl)phthalate
Concen: 50.010 ng/ul
RT: 21.04 min Scan# 3086
Delta R.T. -0.00 min
Lab File: BM030064.D
Acq: 18 May 2021 13:01

Tgt Ion:149 Resp: 2165843
Ion Ratio Lower Upper
149 100
167 26.3 21.1 31.7
279 4.0 3.5 5.3

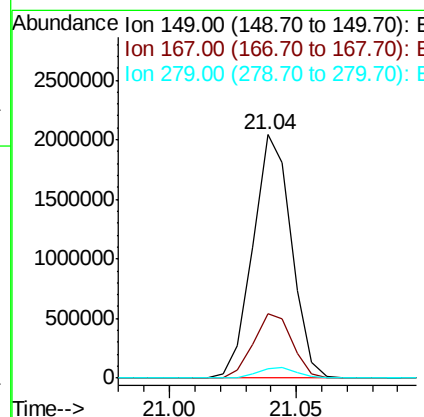

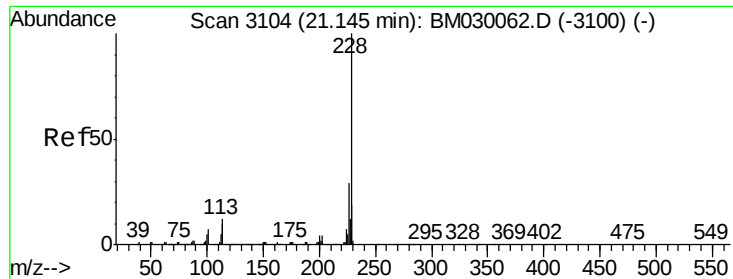

#87

Chrysene

Concen: 38.992 ng/ul

RT: 21.15 min Scan# 3105

Delta R.T. 0.01 min

Lab File: BM030064.D

Acq: 18 May 2021 13:01

Instrument :

BNA_M

ClientSampleId :

SLCS458

Tot Ion:228 Resp: 2725665

Ion Ratio Lower Upper


228 100

226 30.5 23.9 35.9

229 20.0 15.6 23.4

Manual Integrations
APPROVED




mohammad
5/19/2021 11:38:38 AM

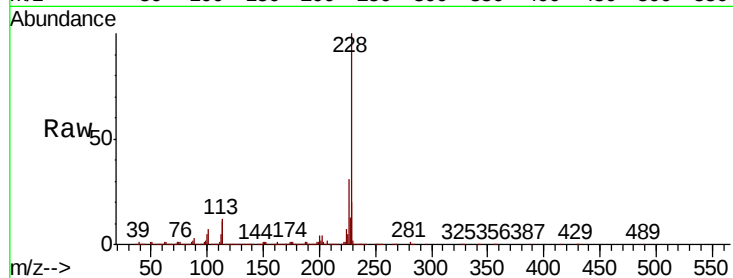

Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

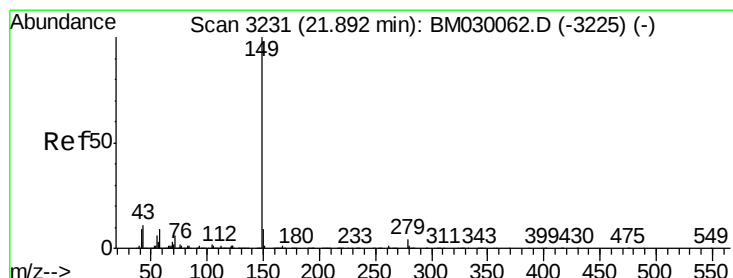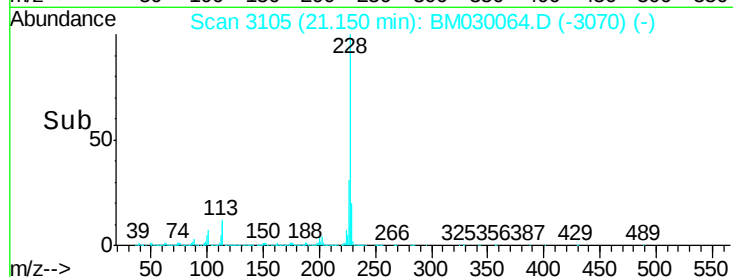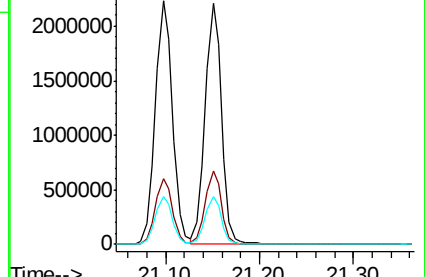

#89

Di-n-octyl phthalate

Concen: 45.548 ng/ul


RT: 21.90 min Scan# 3232

Delta R.T. 0.01 min

Lab File: BM030064.D



Acq: 18 May 2021 13:01


Tgt Ion:149 Resp: 3590263

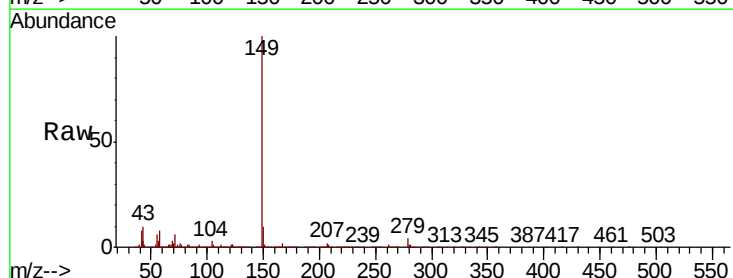

Abundance Ion 149.00 (148.70 to 149.70): E

Ion 149.00 (148.70 to 149.70): E

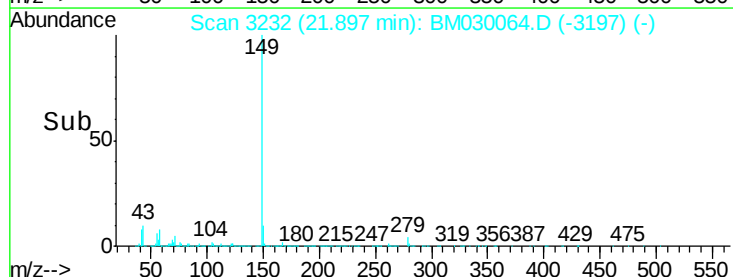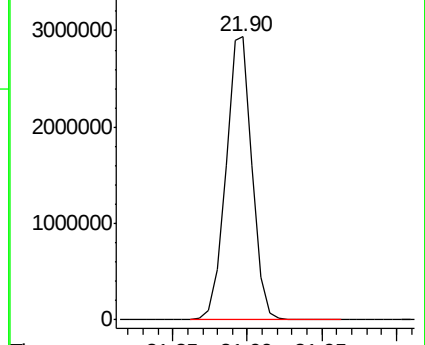







#90
Benzo(b)fluoranthene
Concen: 43.191 ng/ul
RT: 22.62 min Scan# 3355
Delta R.T. 0.01 min
Lab File: BM030064.D
Acq: 18 May 2021 13:01

Instrument :
BNA_M
ClientSampled :
SLCS458

Tot Ion	Ratio	Lower	Upper
252	100		
253	22.3	17.4	26.2
125	10.8	8.6	12.8




Manual Integrations
APPROVED


mohammad
5/19/2021 11:38:38 AM

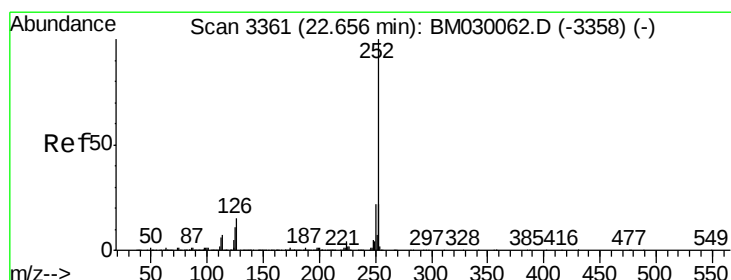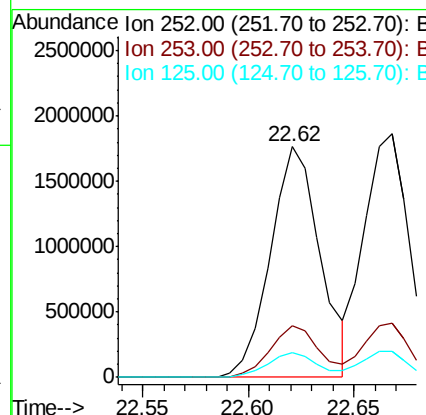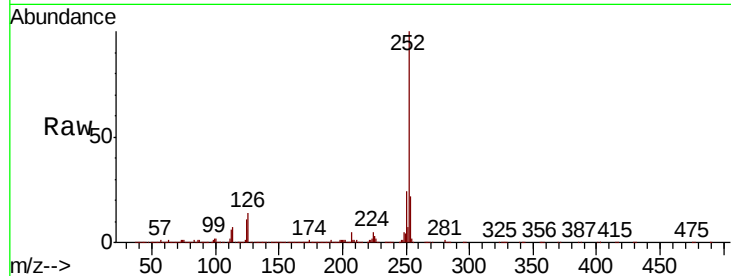

#91
Benzo(k)fluoranthene
Concen: 40.293 ng/ul
RT: 22.67 min Scan# 3363
Delta R.T. 0.01 min
Lab File: BM030064.D
Acq: 18 May 2021 13:01

Tgt Ion	Ratio	Lower	Upper
252	100		
253	22.2	17.8	26.8
125	10.6	8.4	12.6

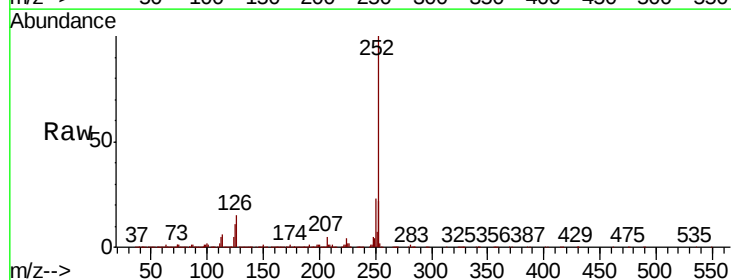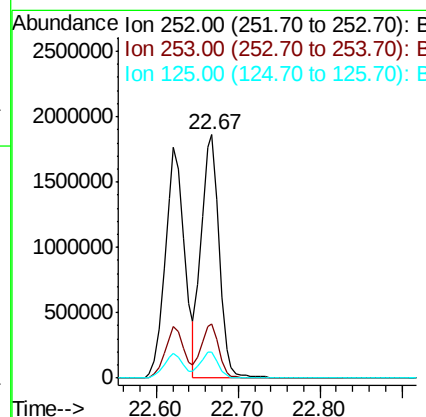







#93
Benzo(a)pyrene
Concen: 41.147 ng/ul
RT: 23.17 min Scan# 3448
Delta R.T. 0.01 min
Lab File: BM030064.D
Acq: 18 May 2021 13:01

Instrument :
BNA_M
ClientSampleId :
SLCS458

Tot Ion	Ratio	Lower	Upper
252	100		
253	21.9	17.9	26.9
125	12.0	9.6	14.4




Manual Integrations
APPROVED


mohammad
5/19/2021 11:38:38 AM

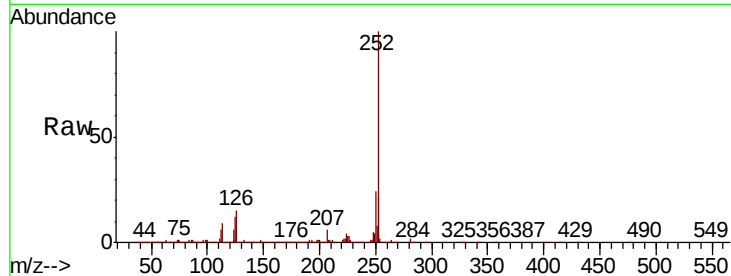

#94
Indeno(1,2,3-cd)pyrene
Concen: 41.492 ng/ul
RT: 25.40 min Scan# 3828
Delta R.T. 0.02 min
Lab File: BM030064.D
Acq: 18 May 2021 13:01

Tgt Ion	Ratio	Lower	Upper
276	100		
138	27.6	21.1	31.7
277	25.7	20.3	30.5



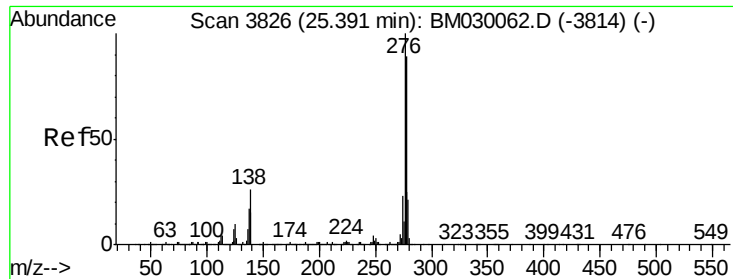





#95
Dibenzo(a,h)anthracene
Concen: 41.487 ng/ul
RT: 25.41 min Scan# 3829
Delta R.T. 0.02 min
Lab File: BM030064.D
Acq: 18 May 2021 13:01

Instrument :
BNA_M
ClientSampled :
SLCS458

Tot Ion	Ratio	Lower	Upper
278	100		
139	16.9	13.5	20.3
279	23.6	18.6	28.0

Manual Integrations
APPROVED

mohammad
5/19/2021 11:38:38 AM

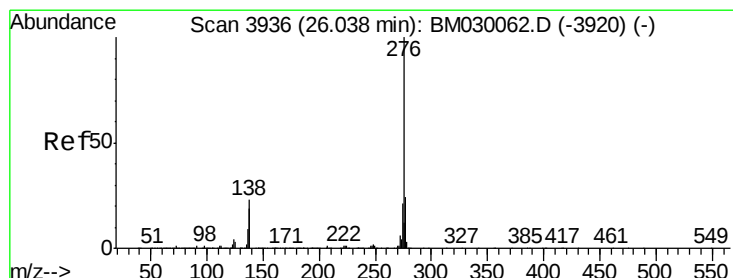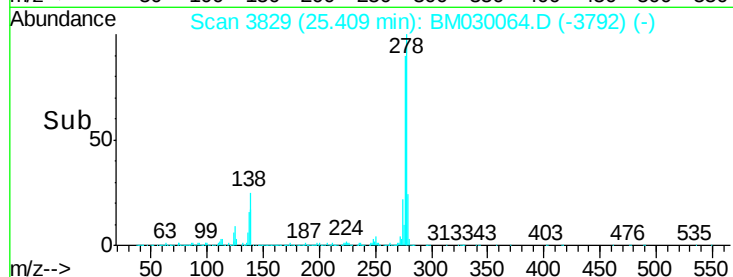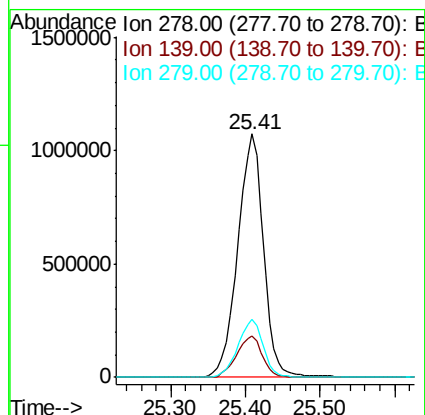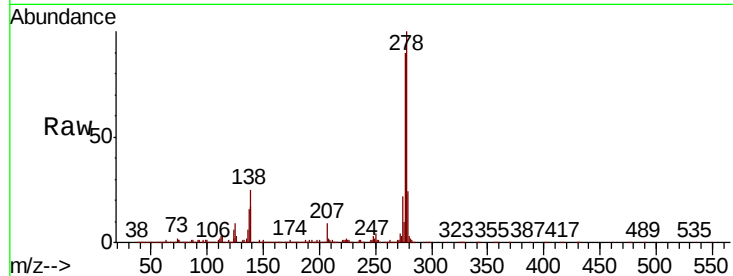

#96
Benzo(g,h,i)perylene
Concen: 39.981 ng/ul
RT: 26.05 min Scan# 3938
Delta R.T. 0.01 min
Lab File: BM030064.D
Acq: 18 May 2021 13:01

Tgt Ion	Ratio	Lower	Upper
276	100		
138	22.0	17.8	26.8
277	23.6	18.5	27.7

