

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM051821\
 Data File : BM030072.D
 Acq On : 18 May 2021 19:16
 Operator : CG/JU
 Sample : M2445-02
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BG1Z4

Manual Integrations
 APPROVED

mohammad
 5/19/2021 11:38:50 AM

Quant Time: May 19 01:41:46 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 18 16:38:21 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.52	152	121031	20.00	ng/ul	0.00
20) Naphthalene-d8	10.29	136	549467	20.00	ng/ul	0.00
38) Acenaphthene-d10	14.17	164	376163	20.00	ng/ul	0.00
64) Phenanthrene-d10	16.92	188	801979	20.00	ng/ul	0.00
79) Chrysene-d12	21.11	240	856192	20.00	ng/ul	0.00
88) Perylene-d12	23.26	264	925844	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.05	96	4500m	1.48	ng/uL	0.01
4) Pyridine-d5	0.00	84	0d	0.00	ng/ul	
7) Phenol-d5	6.72	99	52079	4.63	ng/ul	0.01
9) Bis-(2-Chloroethyl)ether-d	6.87	67	192585	27.59	ng/ul	0.00
11) 2-Chlorophenol-d4	7.06	132	193162	22.24	ng/ul	0.00
15) 4-Methylphenol-d8	8.24	113	114817	12.33	ng/ul	0.00
21) Nitrobenzene-d5	8.67	128	115229	30.43	ng/ul	0.00
24) 2-Nitrophenol-d4	9.39	143	130390	30.51	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	9.93	165	193735	22.61	ng/ul	0.00
31) 4-Chloroaniline-d4	10.52	131	11003m	0.84	ng/ul	0.08
46) Dimethylphthalate-d6	13.59	166	961835	32.99	ng/ul	0.00
49) Acenaphthylene-d8	13.86	160	1110026	30.04	ng/ul	0.00
54) 4-Nitrophenol-d4	14.48	143	11589m	2.44	ng/ul	0.08
60) Fluorene-d10	15.17	176	839514	33.92	ng/ul	0.00
65) 4,6-Dinitro-2-methylphenol	15.31	200	160269	30.77	ng/ul	0.00
73) Anthracene-d10	17.02	188	1430696	35.43	ng/ul	0.00
81) Pyrene-d10	19.32	212	1684410	38.35	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.12	264	1885901	35.93	ng/ul	0.00
Target Compounds						
47) Dimethylphthalate	13.64	163	50234	1.721	ng/ul	Ovalue 99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM051821\
Data File : BM030072.D
Acq On : 18 May 2021 19:16
Operator : CG/JU
Sample : M2445-02
Misc :
ALS Vial : 11 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
BG1Z4

Manual Integrations
APPROVED

mohammad
5/19/2021 11:38:50 AM

Quant Time: May 19 01:41:46 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM050721.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 18 16:38:21 2021
Response via : Initial Calibration

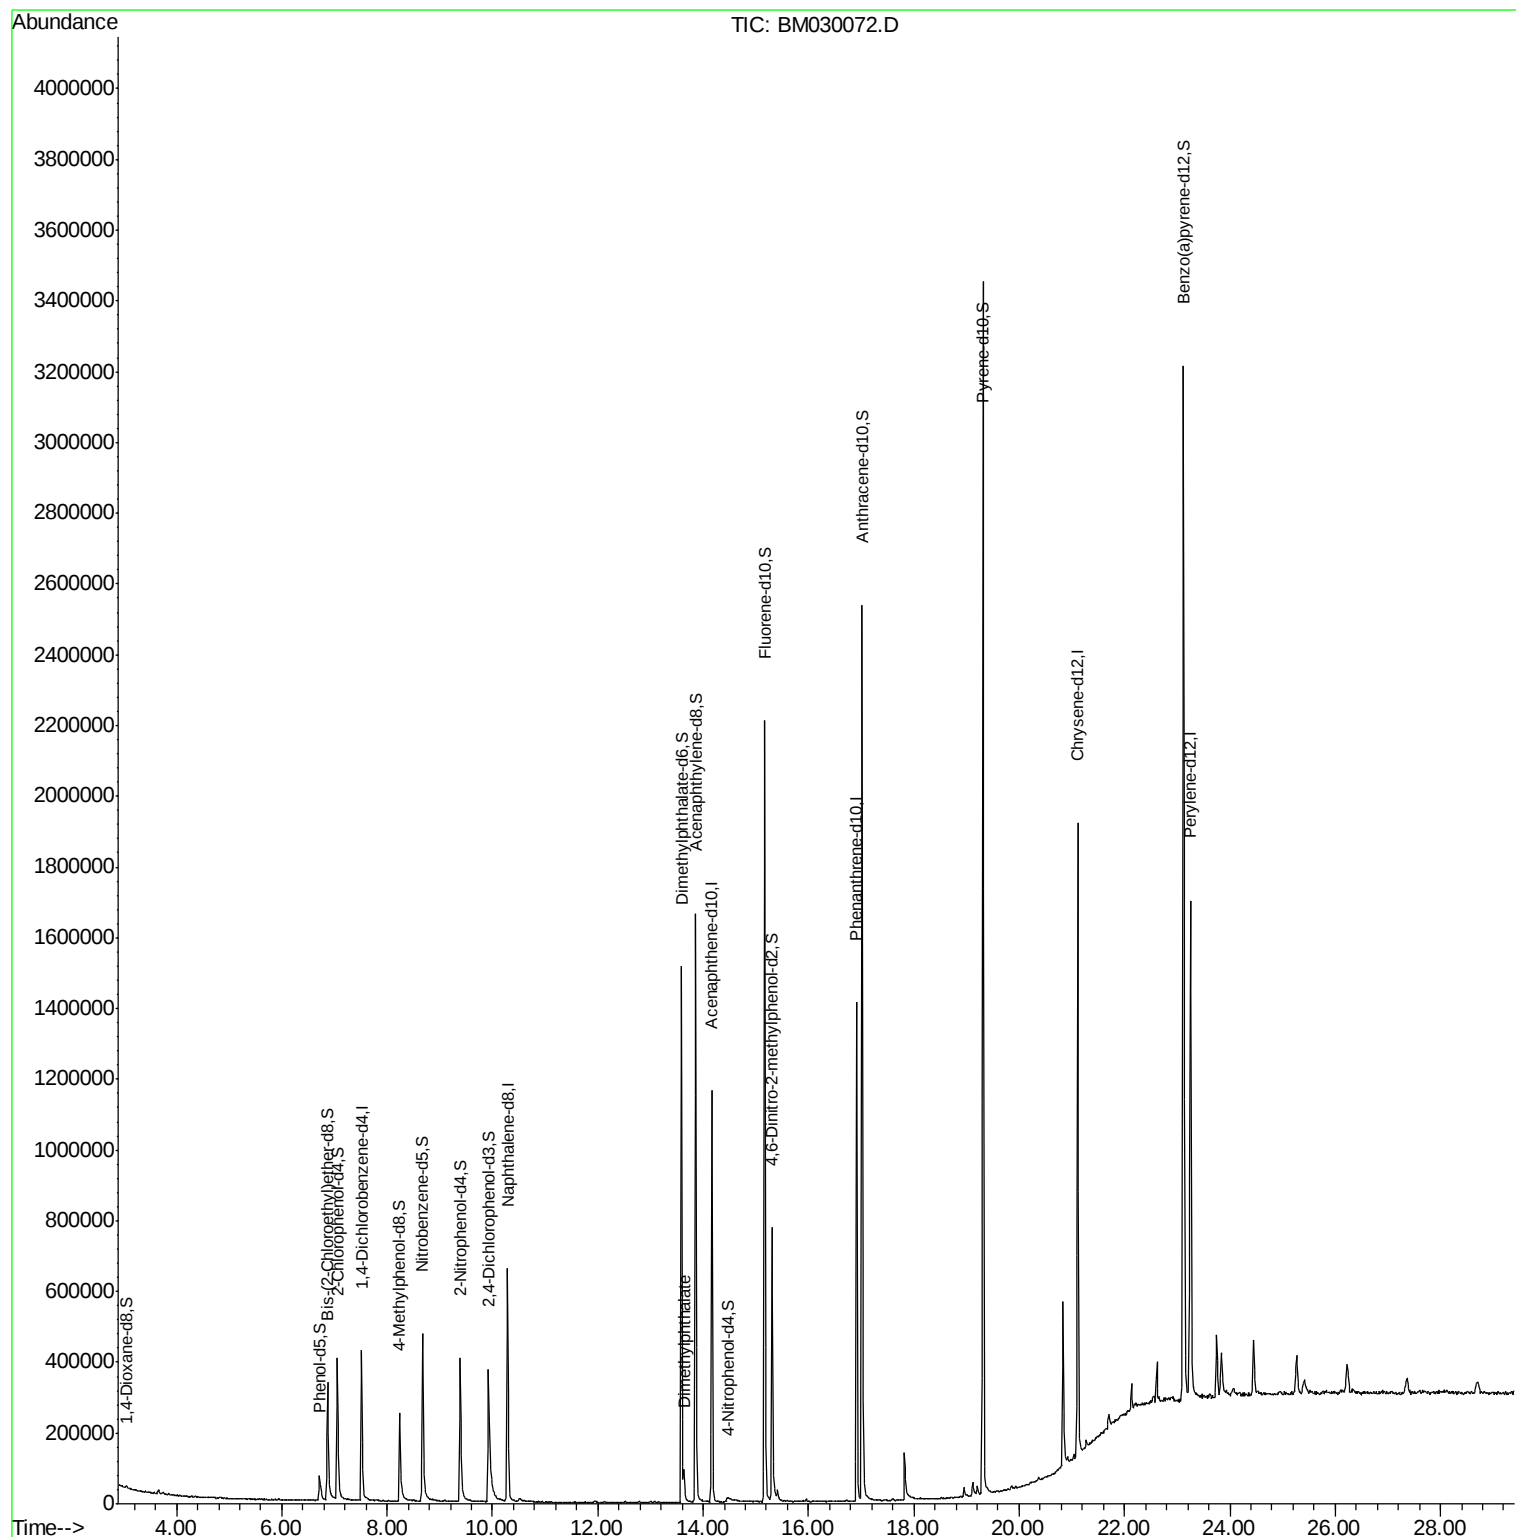

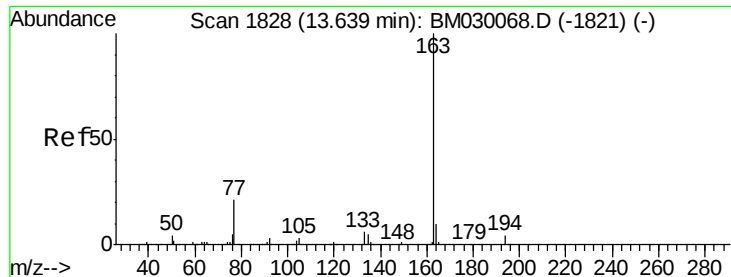

#47
 Dimethylphthalate
 Concen: 1.721 ng/ul
 RT: 13.64 min Scan# 1828
 Delta R.T. -0.00 min
 Lab File: BM030072.D
 Acq: 18 May 2021 19:16

Instrument :
 BNA_M
 ClientSampleId :
 BG1Z4

Tot Ion:	163	Resp:	50234
Ion Ratio	Lower	Upper	
163	100		
194	3.7	3.4	5.0
164	9.9	7.8	11.8

Manual Integrations
 APPROVED

mohammad
 5/19/2021 11:38:50 AM

