


Data Path : Z:\HPCHEM1\BNA_M\Data\BM051915\
 Data File : BM001341.D
 Acq On : 19 May 2015 10:08
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF043015.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue May 19 13:22:43 2015

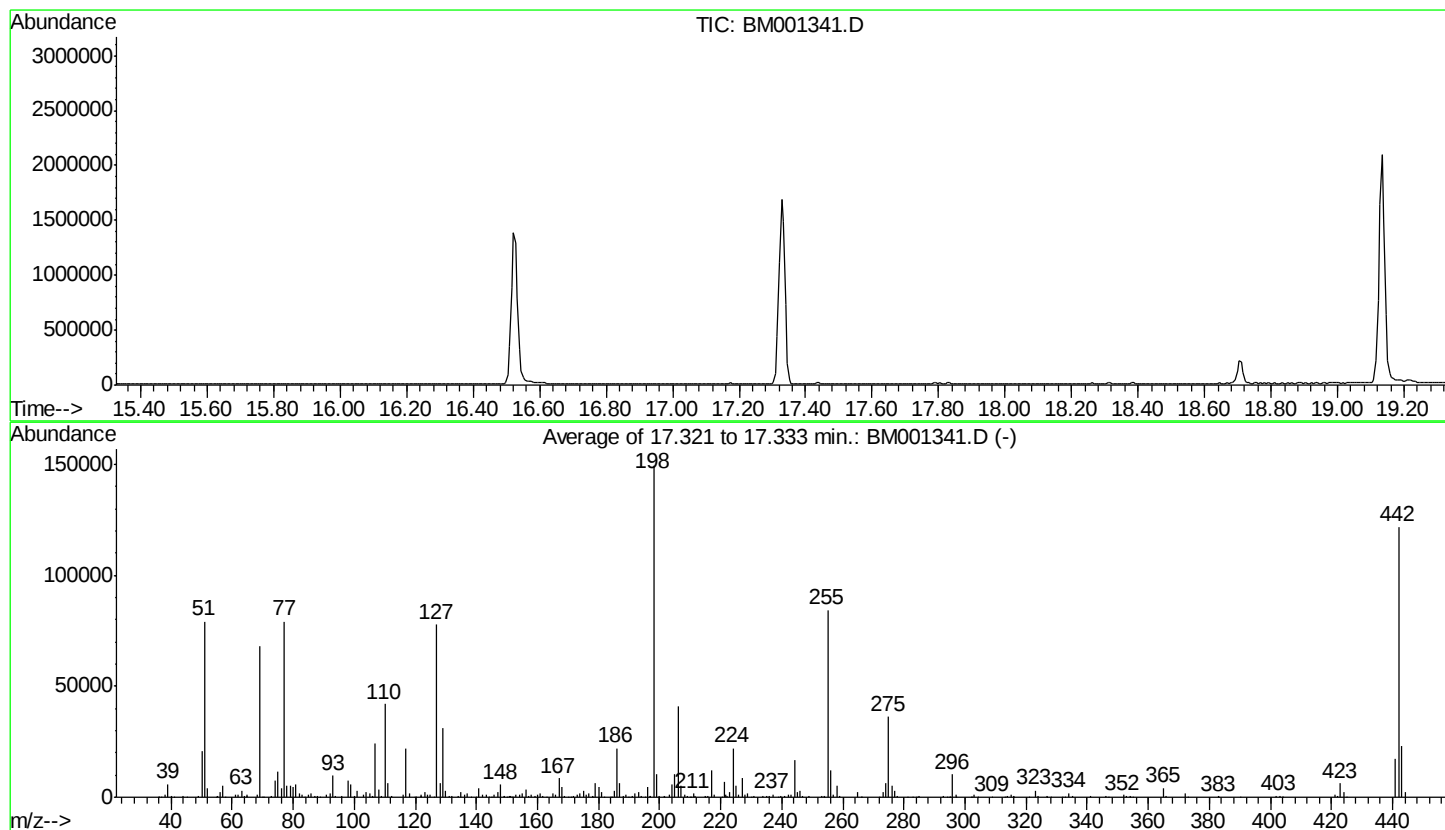

AutoFind: Scans 2488, 2489, 2490; Background Corrected with Scan 2482

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	53.0	79186	PASS
68	69	0.00	2	1.7	1167	PASS
69	198	0.00	100	45.7	68277	PASS
70	69	0.00	2	0.4	306	PASS
127	198	10	80	52.1	77882	PASS
197	198	0.00	2	0.3	422	PASS
198	198	100	100	100.0	149493	PASS
199	198	5	9	7.1	10630	PASS
275	198	10	60	24.3	36346	PASS
365	198	1	100	2.8	4160	PASS
441	442	0.01	24	14.4	17550	PASS
442	198	50	100	81.6	122032	PASS
443	442	15	24	18.8	22960	PASS