

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM051916\
 Data File : BM005508.D
 Acq On : 19 May 2016 20:50
 Operator : UM/SJ
 Sample : H2841-15
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9WT0

Quant Time: May 20 01:02:24 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM051816.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 20 01:00:58 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.83	152	75978	20.00	ng/ul	0.00
18) Naphthalene-d8	10.63	136	402005	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.46	164	286566	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.20	188	814486	20.00	ng/ul	0.00
75) Chrysene-d12	21.37	240	1365851	20.00	ng/ul	0.00
83) Perylene-d12	23.66	264	1723422	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.32	96	3860	1.96	ng/uL	0.00
5) Phenol-d5	6.99	99	114415	15.67	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.17	67	61928	15.49	ng/ul	0.00
9) 2-Chlorophenol-d4	7.36	132	85136	15.19	ng/ul	0.00
13) 4-Methylphenol-d8	8.53	113	99064	15.94	ng/ul	0.00
19) Nitrobenzene-d5	8.99	128	43985	15.20	ng/ul	0.00
22) 2-Nitrophenol-d4	9.71	143	47272	14.97	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.24	165	100783	16.06	ng/ul	0.00
29) 4-Chloroaniline-d4	10.76	131	106550	14.76	ng/ul	0.00
43) Dimethylphthalate-d6	13.87	166	370782	15.74	ng/ul	0.00
46) Acenaphthylene-d8	14.16	160	443822	15.96	ng/ul	0.00
51) 4-Nitrophenol-d4	14.64	143	78804	16.30	ng/ul	0.00
57) Fluorene-d10	15.46	176	343962	16.55	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.56	200	53004	12.35	ng/ul	0.00
70) Anthracene-d10	17.30	188	617847	16.49	ng/ul	0.00
76) Pyrene-d10	19.59	212	885258	16.12	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.51	264	1314945	17.07	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
44) Dimethylphthalate	13.92	163	84954	3.54	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM051916\
Data File : BM005508.D
Acq On : 19 May 2016 20:50
Operator : UM/SJ
Sample : H2841-15
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
D9WT0

Quant Time: May 20 01:02:24 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM051816.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri May 20 01:00:58 2016
Response via : Initial Calibration

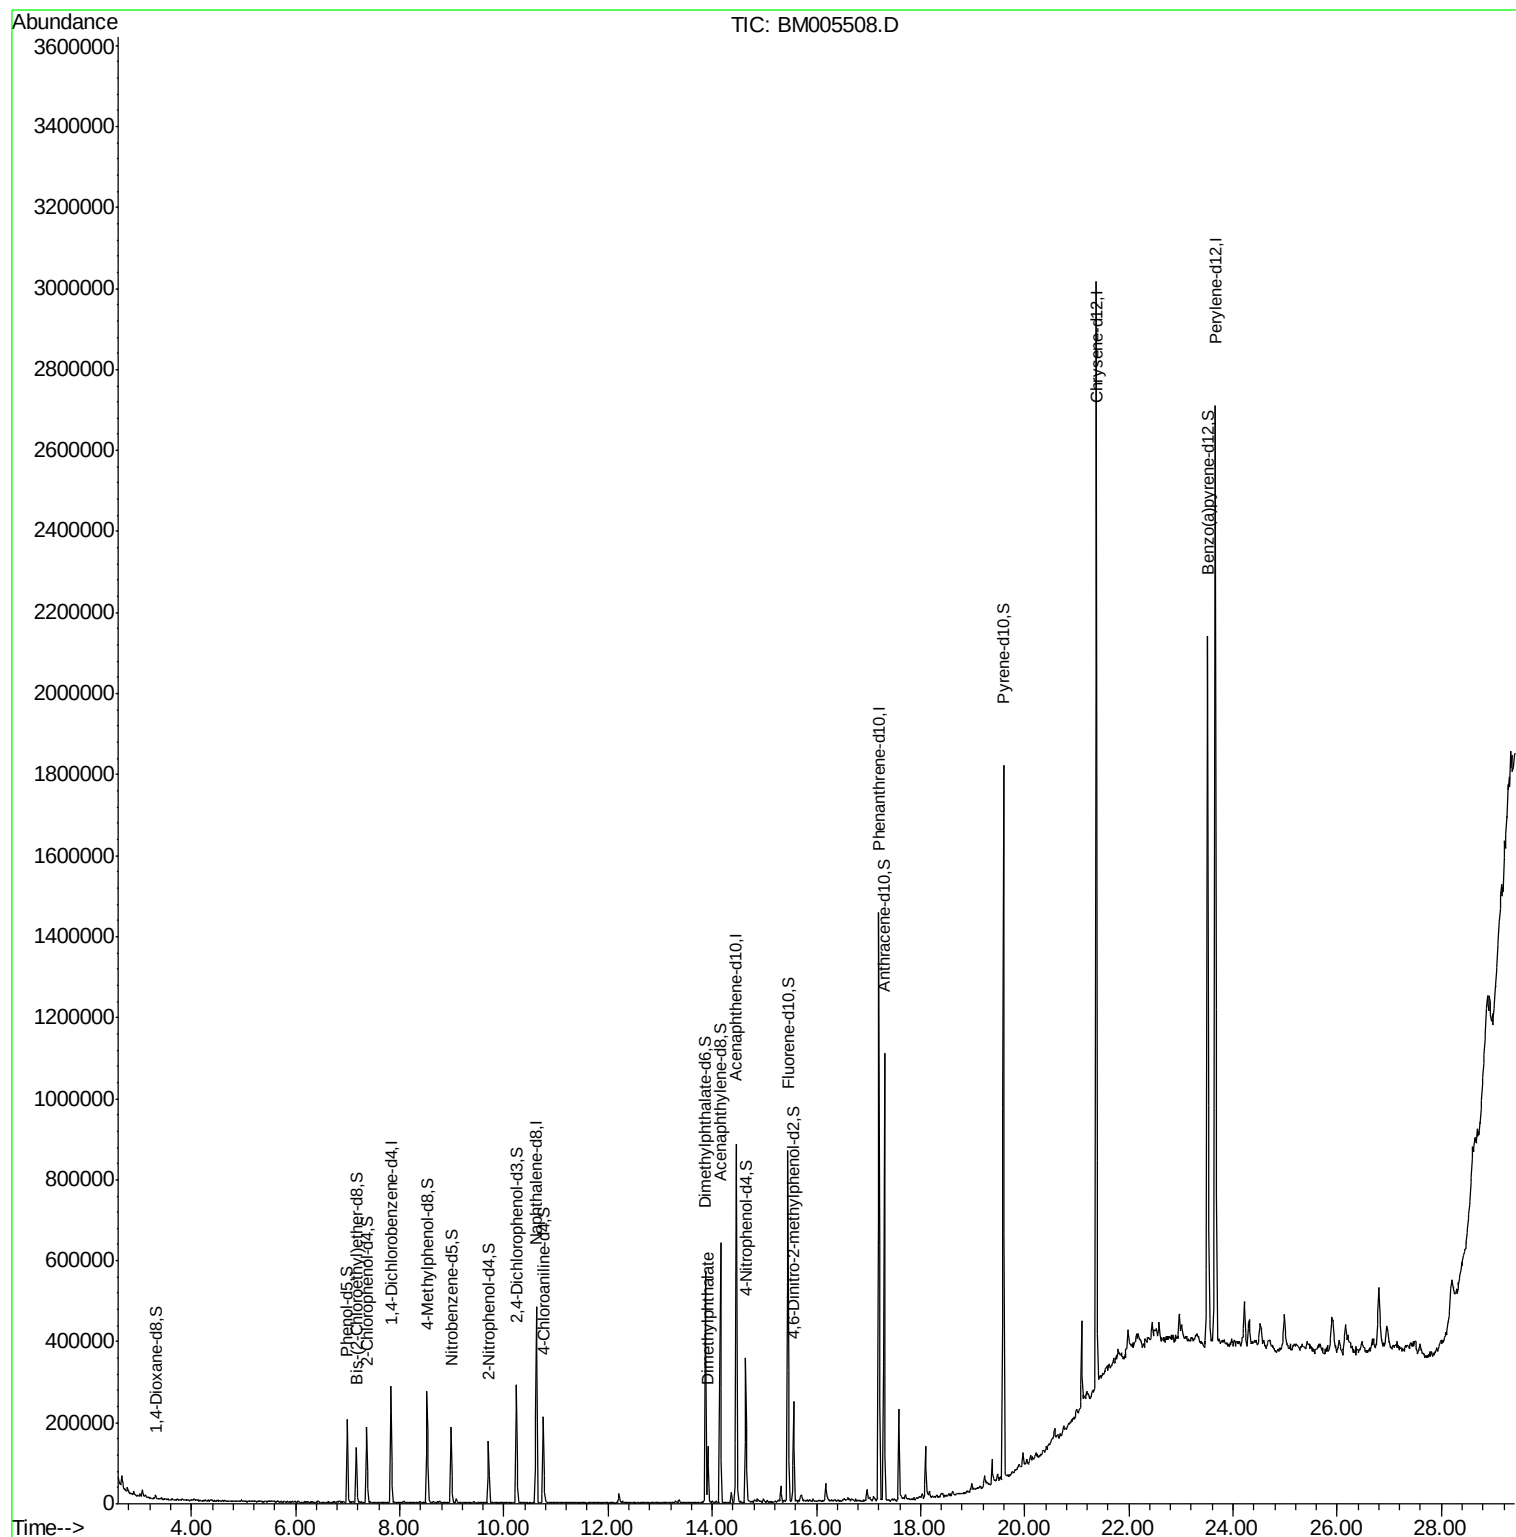

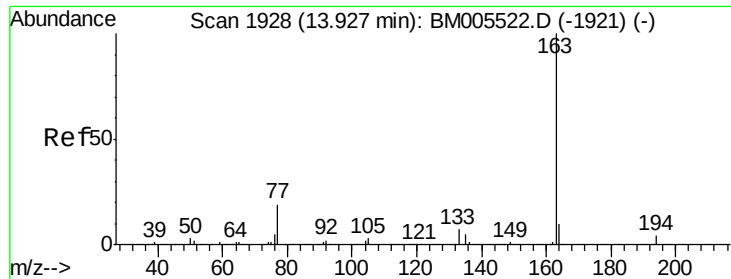

#44

Dimethylphthalate

Concen: 3.54 ng/ul

RT: 13.92 min Scan# 1927

Delta R.T. -0.00 min

Lab File: BM005508.D

Acq: 19 May 2016 20:50

Instrument :

BNA_M

ClientSampleId :

D9WT0


Tgt Ion:163 Resp: 84954

Ion Ratio Lower Upper

163 100

194 4.5 3.4 5.0

164 9.1 7.9 11.9

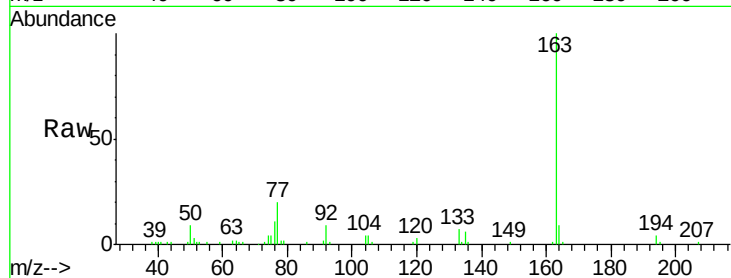

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

