
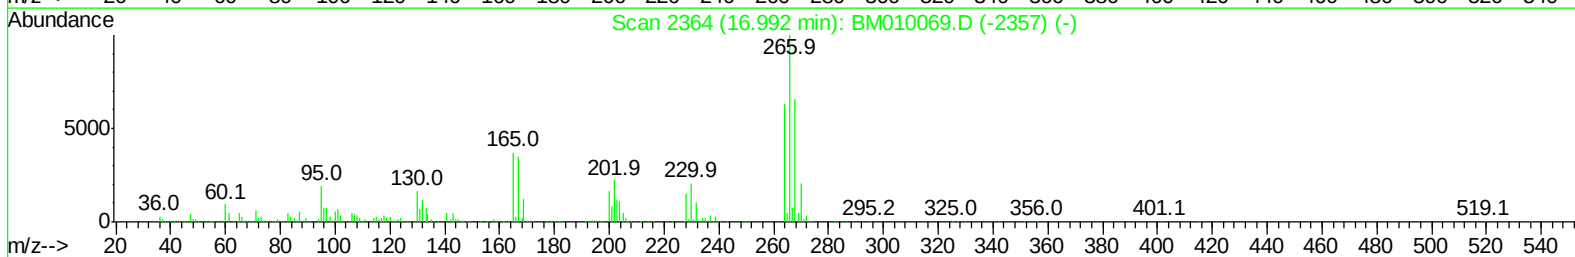
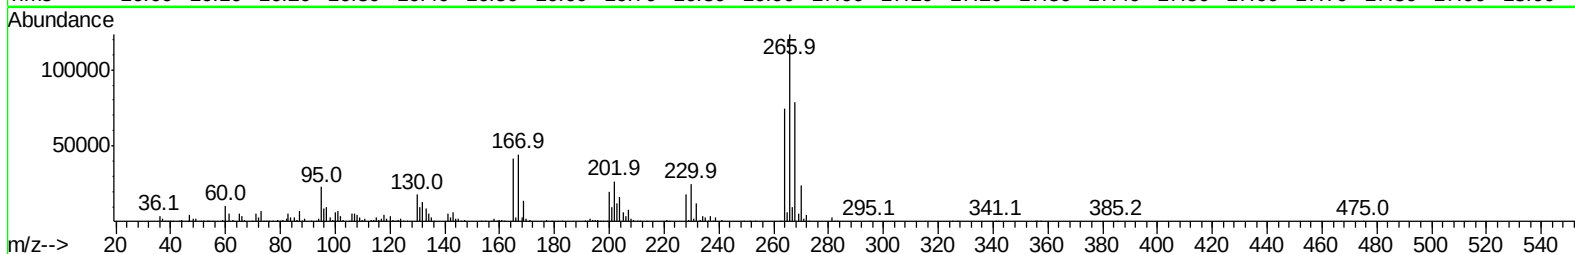


Data Path : Z:\HPCHEM1\BNA M\Data\BM051917\
Data File : BM010065.D
Acq On : 19 May 2017 09:12
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 19 18:30:18 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM051917.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 19 14:14:03 2017
Response via : Initial Calibration

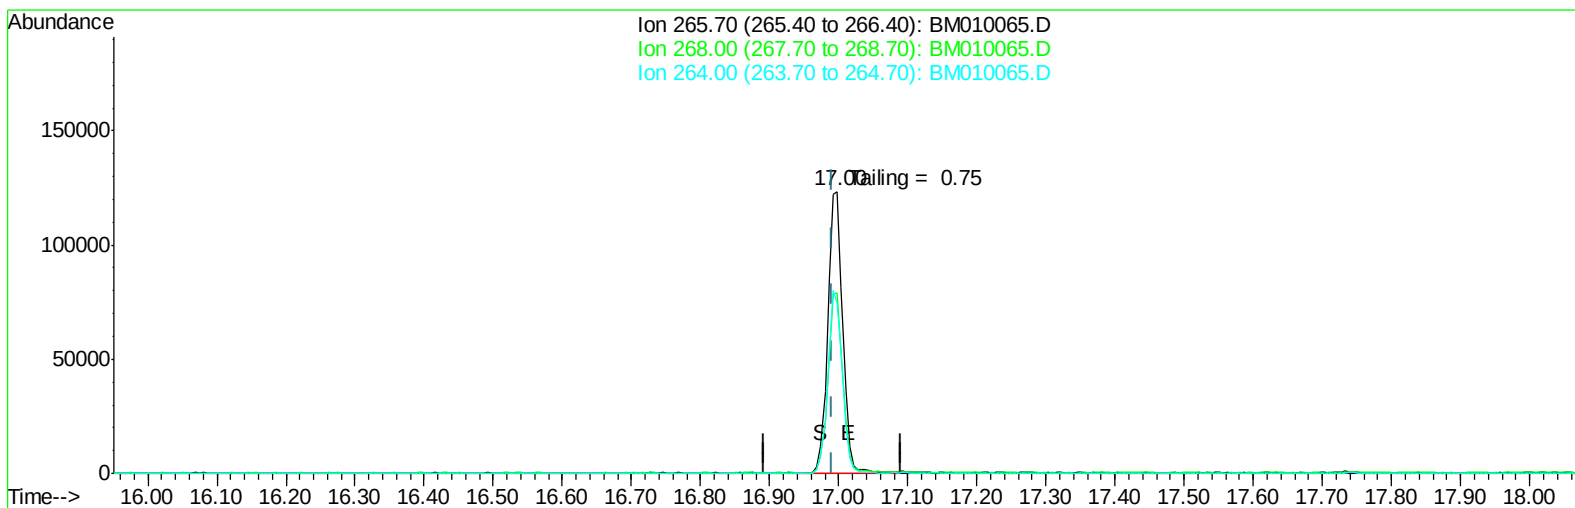

TIC: BM010065.D

(69) Pentachlorophenol (C)




16.998min (+0.006) 0.00ng

response 184590

Ion	Exp%	Act%
265.70	100	100
268.00	65.00	64.02
264.00	61.20	60.42
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA M\Data\BM051917\
Data File : BM010065.D
Acq On : 19 May 2017 09:12
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 19 18:30:18 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM051917.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 19 14:14:03 2017
Response via : Initial Calibration

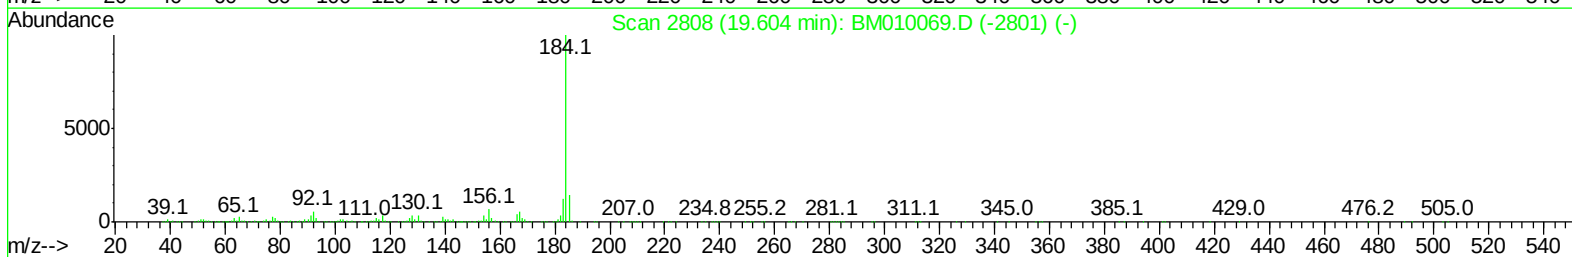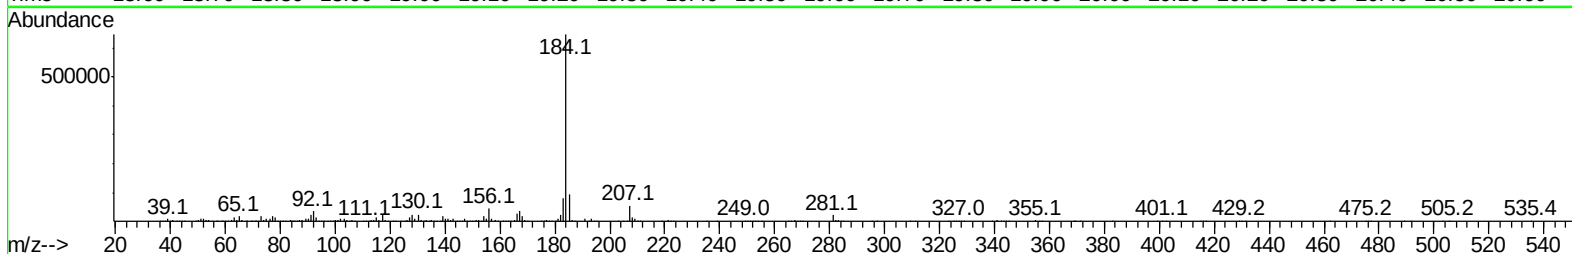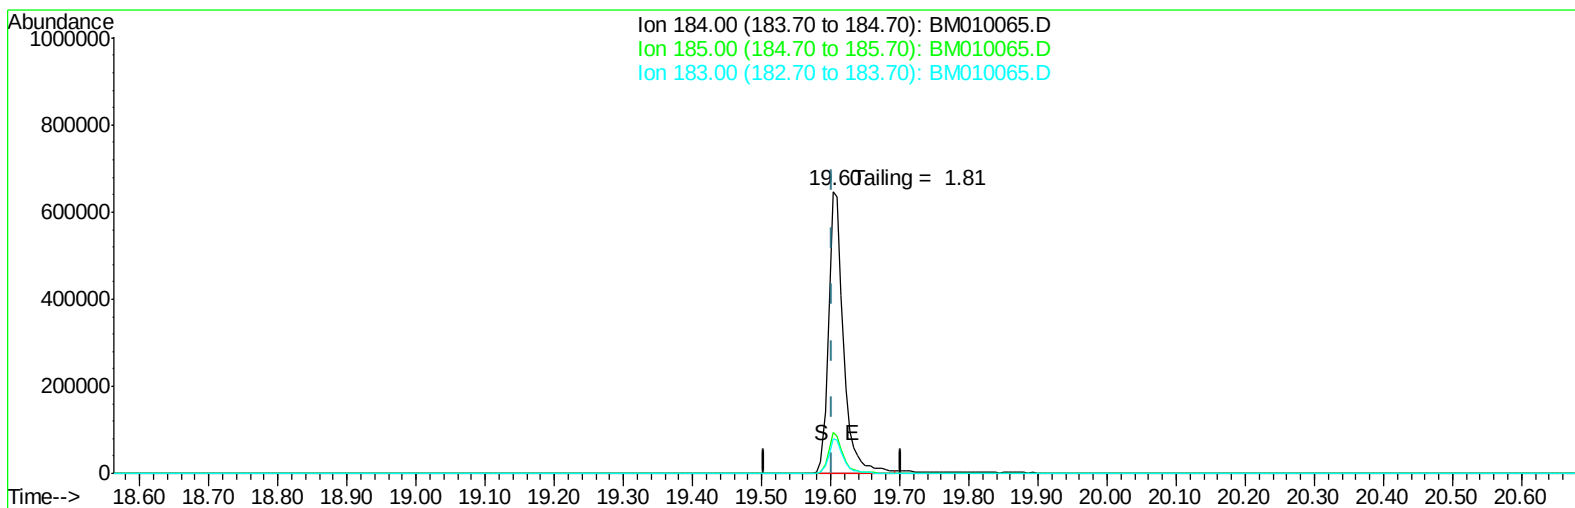

TIC: BM010065.D

(76) Benzidine

19.604min (-0.000) 81503.97ng

response 969647

Ion	Exp%	Act%
184.00	100	100
185.00	14.10	14.72
183.00	11.10	12.19
0.00	0.00	0.00