


Data Path : Z:\HPCHEM1\BNA M\Data\BM051917\
 Data File : BM010065.D
 Acq On : 19 May 2017 09:12
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM051917.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat May 20 04:25:49 2017

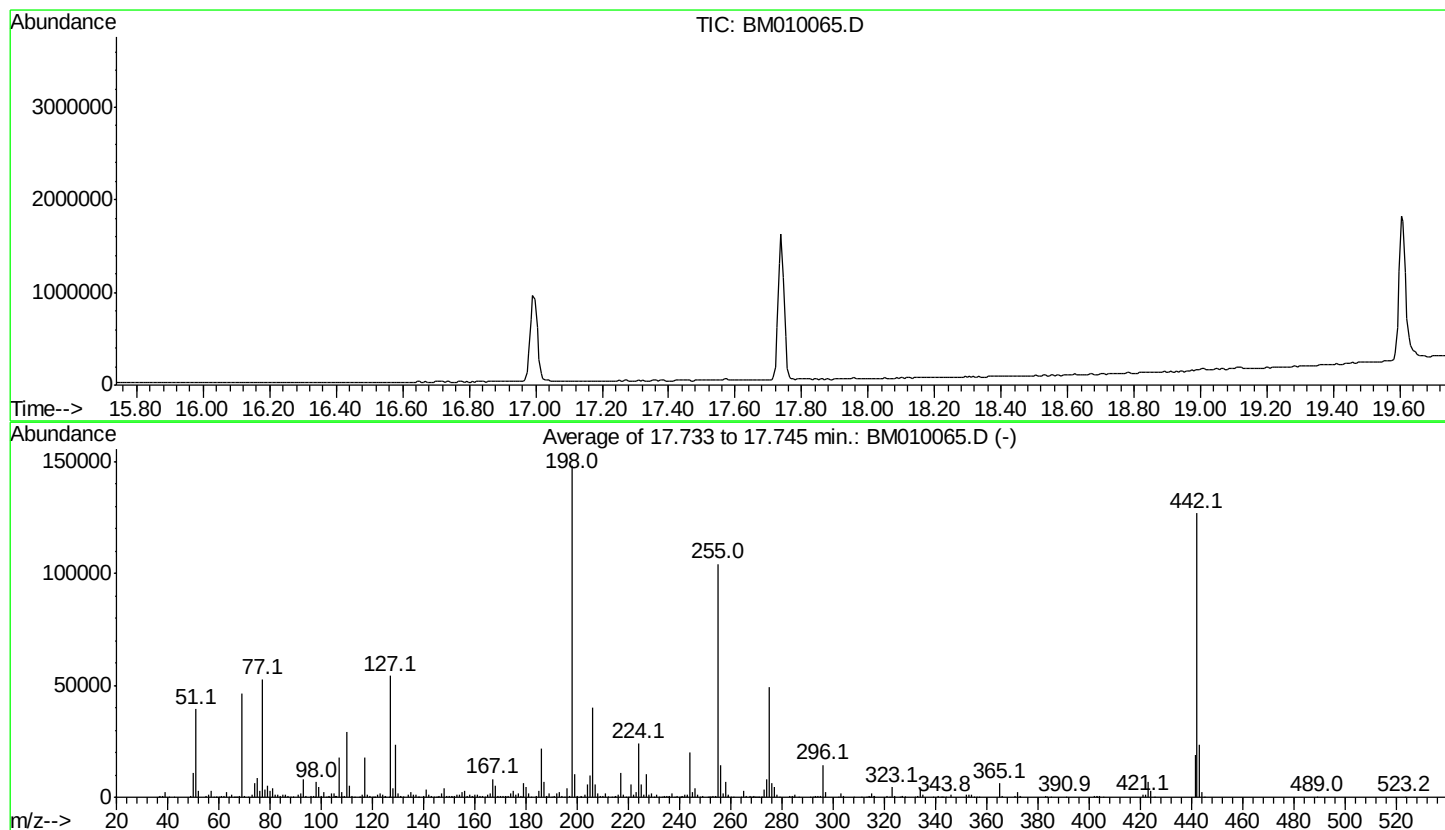

AutoFind: Scans 2490, 2491, 2492; Background Corrected with Scan 2483

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.5	39253	PASS
68	69	0.00	2	1.8	852	PASS
69	198	0.00	100	31.4	46504	PASS
70	69	0.00	2	0.8	364	PASS
127	198	10	80	36.6	54234	PASS
197	198	0.00	2	0.5	776	PASS
198	198	100	100	100.0	148290	PASS
199	198	5	9	6.8	10118	PASS
275	198	10	60	33.3	49442	PASS
365	198	1	100	4.2	6159	PASS
441	442	0.01	24	15.0	18985	PASS
442	198	50	100	85.6	126885	PASS
443	442	15	24	18.4	23312	PASS