


Data Path : Z:\HPCHEM1\BNA M\Data\BM051917\
 Data File : BM010074.D
 Acq On : 19 May 2017 17:49
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM051917.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat May 20 04:25:49 2017

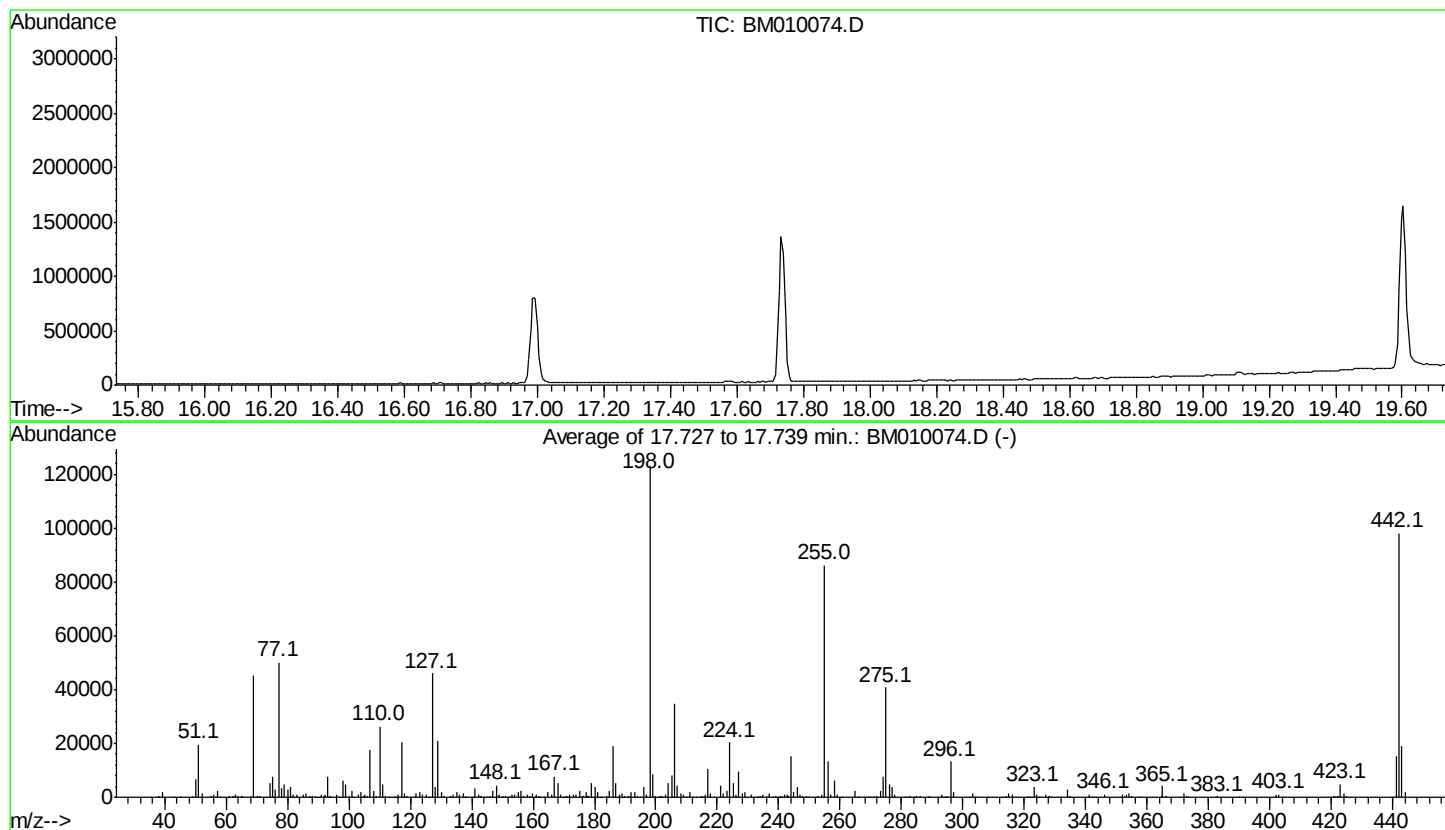

AutoFind: Scans 2489, 2490, 2491; Background Corrected with Scan 2483

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	15.9	19554	PASS
68	69	0.00	2	1.4	617	PASS
69	198	0.00	100	36.9	45389	PASS
70	69	0.00	2	0.9	406	PASS
127	198	10	80	37.3	45928	PASS
197	198	0.00	2	0.7	810	PASS
198	198	100	100	100.0	123168	PASS
199	198	5	9	6.8	8341	PASS
275	198	10	60	33.1	40821	PASS
365	198	1	100	3.3	4074	PASS
441	442	0.01	24	15.3	15016	PASS
442	198	50	100	79.7	98120	PASS
443	442	15	24	19.4	19007	PASS