

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM051920\
 Data File : BM026025.D
 Acq On : 19 May 2020 20:15
 Operator : MA/SJ
 Sample : L2669-10
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SVOC-GCP2-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM026029.D

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.240	58	60	61	rBV2	3383	2518	0.13%	0.027%
2	3.781	149	152	157	rVB3	6901	9865	0.50%	0.106%
3	4.040	194	196	201	rVB5	3242	3426	0.17%	0.037%
4	4.146	212	214	218	rVB4	2057	2093	0.11%	0.022%
5	5.875	505	508	509	rBV3	2810	2696	0.14%	0.029%
6	5.892	509	511	514	rVV4	2210	2017	0.10%	0.022%
7	5.934	514	518	522	rVB7	2262	3989	0.20%	0.043%
8	6.075	539	542	543	rBV3	1609	1980	0.10%	0.021%
9	6.187	559	561	564	rVB4	1770	2178	0.11%	0.023%
10	6.369	589	592	596	rBV6	1853	3337	0.17%	0.036%
11	6.628	634	636	639	rBV4	2506	3521	0.18%	0.038%
12	7.075	709	712	715	rBV4	1777	1975	0.10%	0.021%
13	7.157	724	726	730	rBV5	1454	2014	0.10%	0.022%
14	7.245	736	741	743	rBV5	1844	2210	0.11%	0.024%
15	7.504	778	785	795	rBV	556926	875696	44.60%	9.368%
16	7.686	813	816	820	rBV4	2188	4404	0.22%	0.047%
17	7.863	844	846	851	rVB3	2176	2611	0.13%	0.028%
18	7.986	864	867	869	rBV4	2086	2701	0.14%	0.029%
19	8.545	959	962	965	rBV4	1592	2151	0.11%	0.023%
20	8.581	965	968	970	rVB3	2104	2258	0.11%	0.024%
21	8.710	988	990	993	rBV3	2004	2483	0.13%	0.027%
22	9.333	1093	1096	1100	rBV5	1807	2297	0.12%	0.025%
23	9.928	1194	1197	1201	rBV5	2028	2839	0.14%	0.030%
24	10.263	1247	1254	1265	rBV	719565	1179121	60.05%	12.614%
25	10.369	1269	1272	1276	rBV4	1541	2467	0.13%	0.026%
26	10.516	1293	1297	1299	rVB3	1552	2089	0.11%	0.022%
27	10.539	1299	1301	1304	rBV4	2314	2867	0.15%	0.031%
28	10.727	1329	1333	1336	rVB4	2255	3104	0.16%	0.033%
29	11.057	1387	1389	1391	rVB3	2270	2222	0.11%	0.024%
30	11.227	1413	1418	1421	rBV5	2181	3132	0.16%	0.034%
31	11.604	1478	1482	1487	rBV6	2967	4097	0.21%	0.044%
32	12.580	1647	1648	1654	rBV5	1805	2193	0.11%	0.023%
33	13.551	1810	1813	1816	rVB5	1846	2439	0.12%	0.026%
34	13.633	1823	1827	1832	rVB5	6138	8749	0.45%	0.094%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM051920\
 Data File : BM026025.D
 Acq On : 19 May 2020 20:15
 Operator : MA/SJ
 Sample : L2669-10
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SVOC-GCP2-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
 Title : SVOA CALIBRATION

35	13.886	1865	1870	1873	rBV5	2031	3479	0.18%	0.037%
36	14.145	1907	1914	1924	rBV	1035406	1460296	74.37%	15.623%
37	14.857	2033	2035	2040	rVB4	2106	2527	0.13%	0.027%
38	15.027	2059	2064	2066	rBV4	1999	3839	0.20%	0.041%
39	15.198	2090	2093	2097	rVB4	7421	10139	0.52%	0.108%
40	15.398	2125	2127	2130	rBV3	2465	2617	0.13%	0.028%
41	15.439	2130	2134	2137	rBV6	1896	3652	0.19%	0.039%
42	15.980	2222	2226	2229	rBV5	1503	2422	0.12%	0.026%
43	16.198	2261	2263	2267	rVB4	2240	2076	0.11%	0.022%
44	16.451	2300	2306	2311	rBV7	5229	8758	0.45%	0.094%
45	16.545	2320	2322	2325	rBV4	1928	2674	0.14%	0.029%
46	16.686	2342	2346	2350	rBV6	3628	5532	0.28%	0.059%
47	16.892	2375	2381	2392	rVV	1256290	1726420	87.92%	18.470%
48	16.986	2395	2397	2398	rVV2	3060	2565	0.13%	0.027%
49	17.004	2398	2400	2405	rVB4	4319	4189	0.21%	0.045%
50	17.221	2436	2437	2440	rVB3	2626	2221	0.11%	0.024%
51	17.515	2483	2487	2490	rBV5	4063	5276	0.27%	0.056%
52	17.827	2538	2540	2542	rBV3	2301	2036	0.10%	0.022%
53	17.856	2542	2545	2548	rVV5	2152	2600	0.13%	0.028%
54	18.086	2582	2584	2586	rBV2	2538	2394	0.12%	0.026%
55	18.398	2634	2637	2639	rBV4	1864	2220	0.11%	0.024%
56	18.468	2644	2649	2653	rBV8	4173	7616	0.39%	0.081%
57	18.515	2655	2657	2660	rBV4	1688	2192	0.11%	0.023%
58	18.621	2673	2675	2677	rBV3	1733	1981	0.10%	0.021%
59	18.739	2693	2695	2698	rBV4	2431	3104	0.16%	0.033%
60	18.898	2720	2722	2725	rVB4	2178	2277	0.12%	0.024%
61	19.274	2782	2786	2787	rBV4	4734	6106	0.31%	0.065%
62	19.833	2879	2881	2882	rBV2	4685	3195	0.16%	0.034%
63	21.091	3090	3095	3101	rBV	1647875	1963627	100.00%	21.007%
64	23.215	3450	3456	3467	rVB	1164369	1945619	99.08%	20.815%


Sum of corrected areas: 9347388

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM051920\
Data File : BM026025.D
Acq On : 19 May 2020 20:15
Operator : MA/SJ
Sample : L2669-10
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SVOC-GCP2-BLANK

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

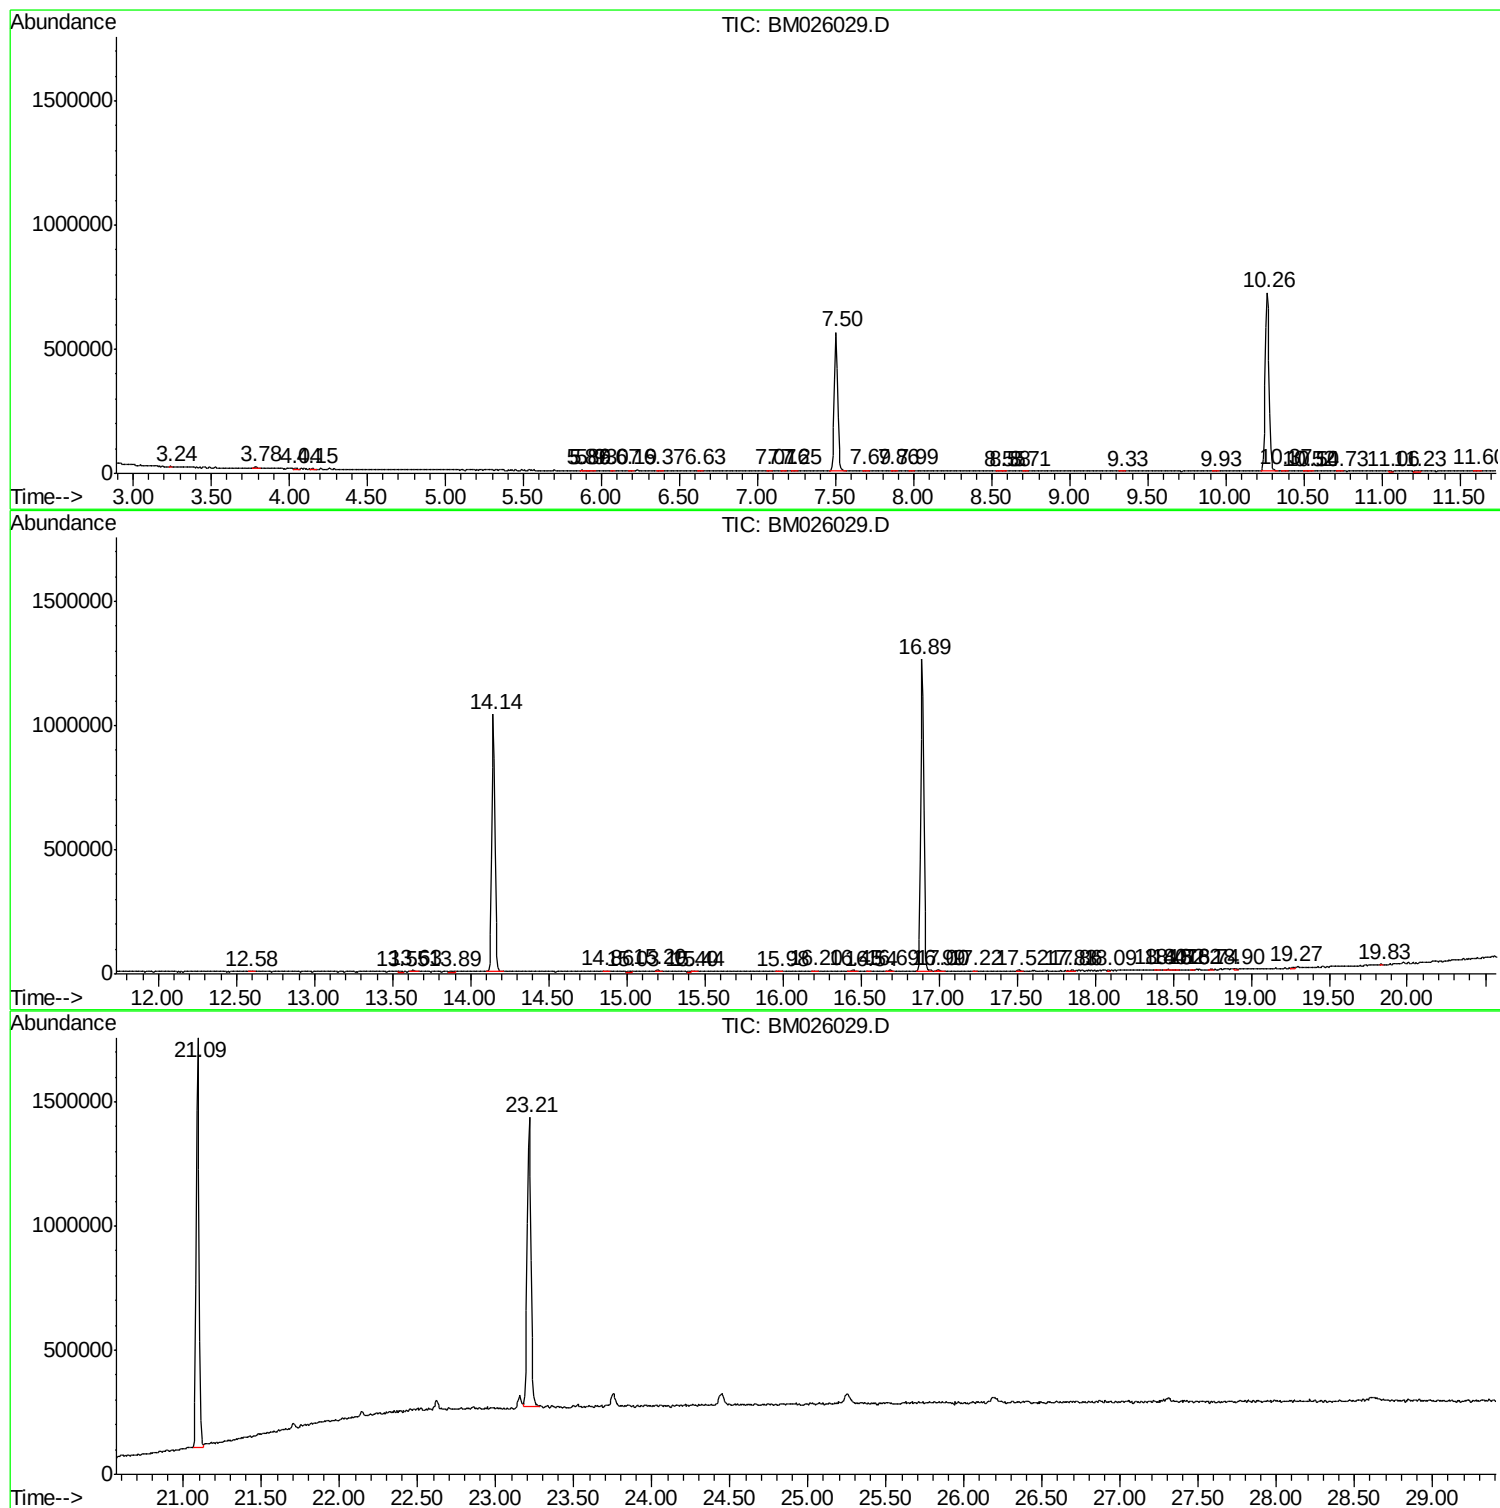

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM051920\
Data File : BM026025.D
Acq On : 19 May 2020 20:15
Operator : MA/SJ
Sample : L2669-10
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SVOC-GCP2-BLANK

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM051920\
Data File : BM026025.D
Acq On : 19 May 2020 20:15
Operator : MA/SJ
Sample : L2669-10
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SVOC-GCP2-BLANK

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM051320MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc